

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
 Data File : BN016710.D
 Acq On : 04 Oct 2021 14:41
 Operator : CG/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Oct 04 15:15:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 04 15:14:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.642	152	25239	0.40	ng	0.00
7) Naphthalene-d8	10.406	136	112431	0.40	ng	0.00
13) Acenaphthene-d10	14.268	164	59809	0.40	ng	0.00
19) Phenanthrene-d10	17.029	188	111207	0.40	ng	0.00
29) Chrysene-d12	21.238	240	102448	0.40	ng	0.00
35) Perylene-d12	23.494	264	98715	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.254	112	24432	0.38	ng	0.00
5) Phenol-d6	6.821	99	26787	0.38	ng	0.00
8) Nitrobenzene-d5	8.784	82	27001	0.37	ng	0.00
11) 2-Methylnaphthalene-d10	12.007	152	63795	0.38	ng	0.00
14) 2,4,6-Tribromophenol	15.778	330	8405	0.31	ng	0.00
15) 2-Fluorobiphenyl	12.898	172	89068	0.37	ng	0.00
27) Fluoranthene-d10	19.068	212	112103	0.38	ng	0.00
31) Terphenyl-d14	19.683	244	92888	0.42	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.253	88	4372	0.38	ng	100
3) n-Nitrosodimethylamine	3.576	42	7062	0.38	ng	100
6) bis(2-Chloroethyl)ether	7.080	93	26760	0.39	ng	100
9) Naphthalene	10.457	128	116710	0.38	ng	100
10) Hexachlorobutadiene	10.748	225	21988	0.38	ng	# 100
12) 2-Methylnaphthalene	12.082	142	75453	0.39	ng	100
16) Acenaphthylene	13.989	152	95374	0.36	ng	100
17) Acenaphthene	14.332	154	65362	0.37	ng	100
18) Fluorene	15.321	166	78129	0.38	ng	100
20) 4,6-Dinitro-2-methylph...	15.423	198	467	0.04	ng	100
21) 4-Bromophenyl-phenylether	16.226	248	24597	0.36	ng	100
22) Hexachlorobenzene	16.336	284	28830	0.36	ng	100
23) Atrazine	16.506	200	17631	0.35	ng	100
24) Pentachlorophenol	16.689	266	3618	0.14	ng	99
25) Phenanthrene	17.066	178	123259	0.37	ng	100
26) Anthracene	17.163	178	104221	0.36	ng	100
28) Fluoranthene	19.097	202	137115	0.38	ng	100
30) Pyrene	19.465	202	137639	0.42	ng	100
32) Benzo(a)anthracene	21.216	228	126207	0.40	ng	100
33) Chrysene	21.270	228	132155	0.42	ng	100
34) Bis(2-ethylhexyl)phtha...	21.174	149	67092	0.54	ng	100
36) Indeno(1,2,3-cd)pyrene	25.781	276	118655	0.34	ng	100
37) Benzo(b)fluoranthene	22.813	252	131541	0.41	ng	100
38) Benzo(k)fluoranthene	22.861	252	124259	0.40	ng	100
39) Benzo(a)pyrene	23.392	252	115306	0.41	ng	100
40) Dibenzo(a,h)anthracene	25.798	278	92771	0.33	ng	100
41) Benzo(g,h,i)perylene	26.476	276	107635	0.35	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016710.D
Acq On : 04 Oct 2021 14:41
Operator : CG/JU
Sample : SSTDICCC0.4
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Quant Time: Oct 04 15:15:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 04 15:14:53 2021
Response via : Initial Calibration

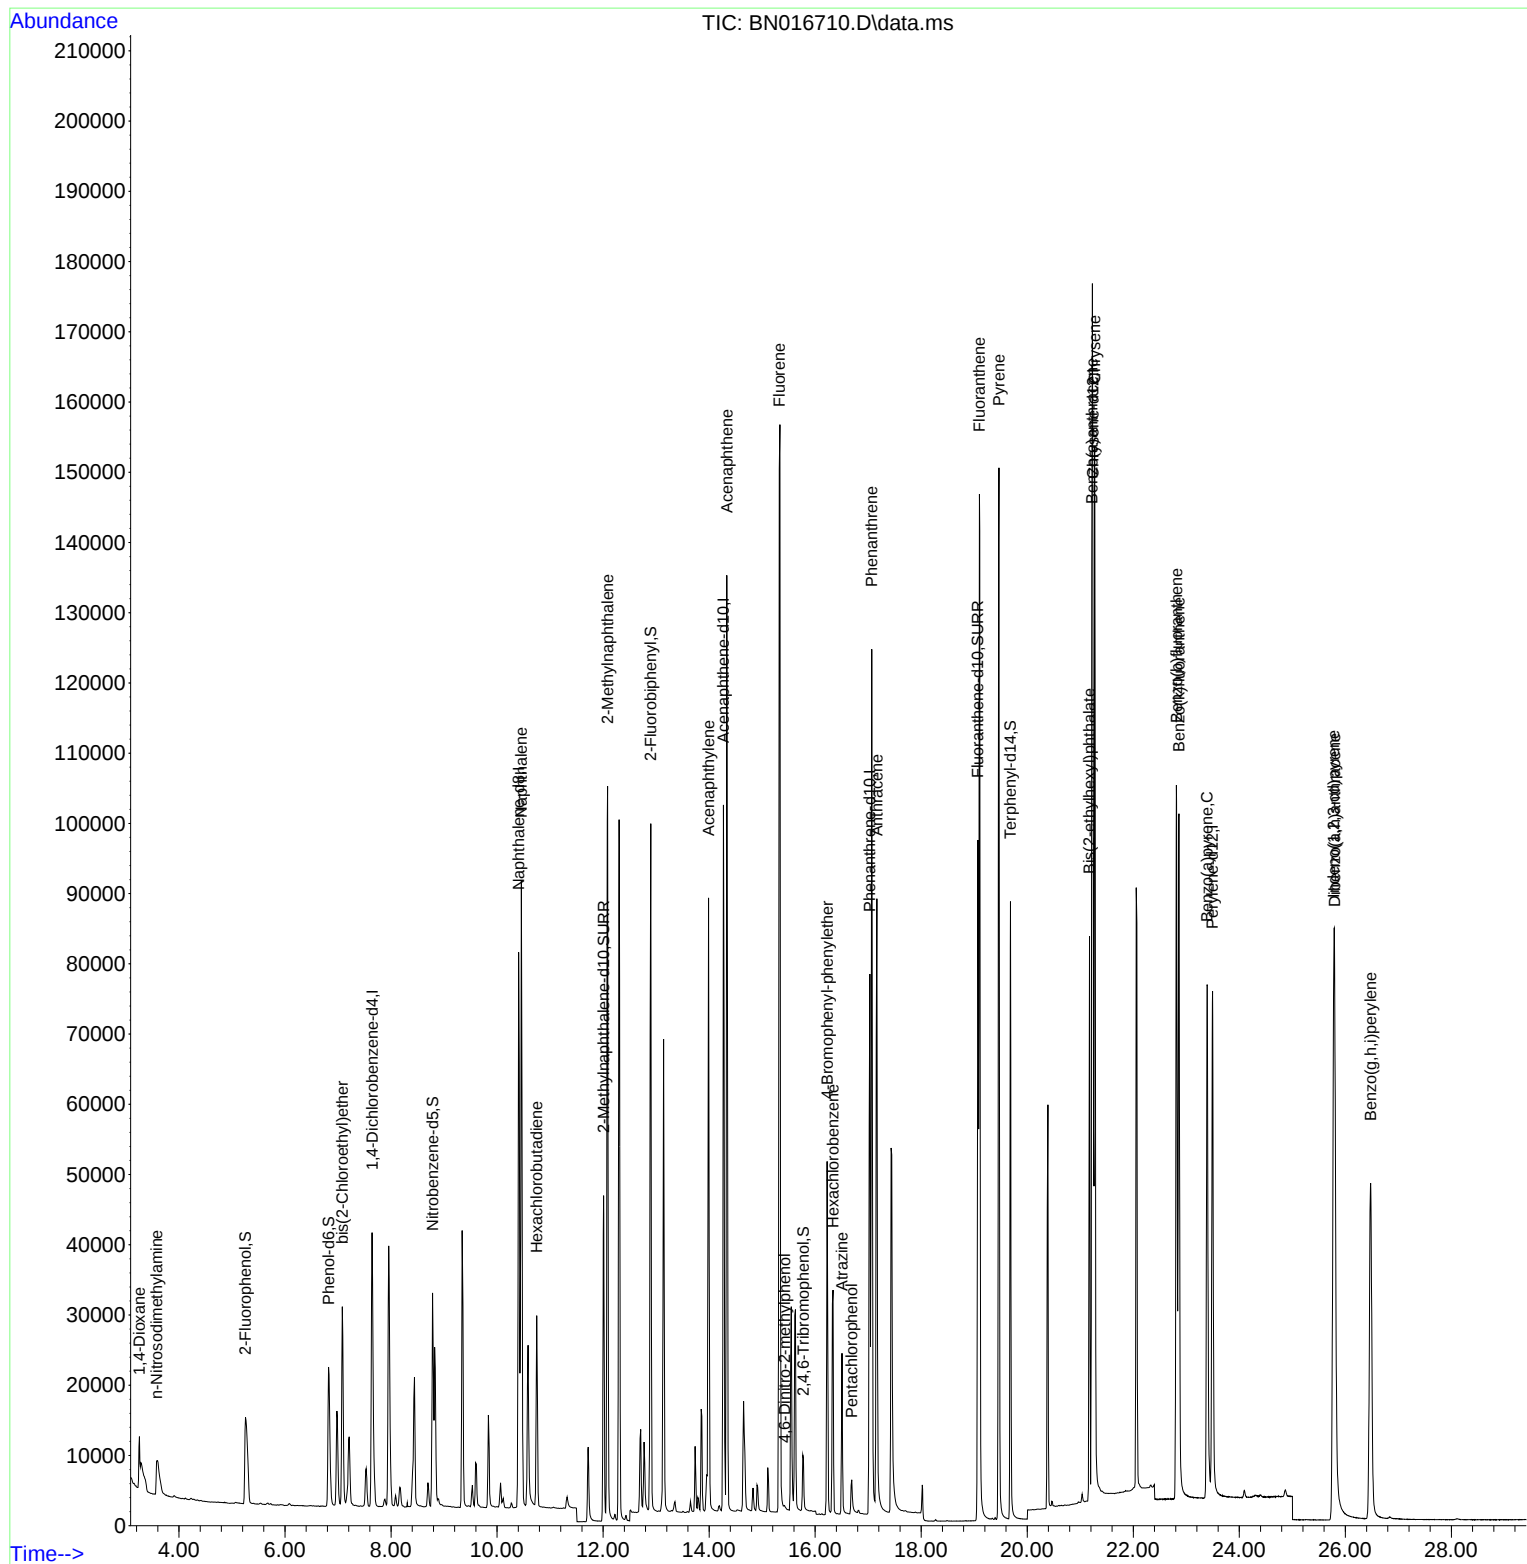







#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.642 min Scan# 495
 Delta R.T. 0.000 min
 Lab File: BN016710.D
 Acq: 04 Oct 2021 14:41

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4

Tgt Ion:152 Resp: 25239




Ion	Ratio	Lower	Upper
152	100		
150	154.1	123.3	184.9
115	58.8	47.0	70.6

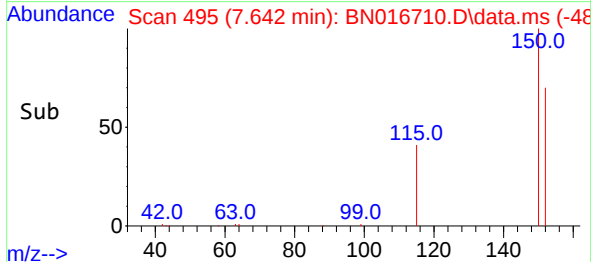


#2
 1,4-Dioxane
 Concen: 0.38 ng
 RT: 3.253 min Scan# 19
 Delta R.T. 0.000 min
 Lab File: BN016710.D
 Acq: 04 Oct 2021 14:41

Tgt Ion: 88 Resp: 4372

Ion	Ratio	Lower	Upper
88	100		
43	77.1	61.7	92.5
58	77.7	62.2	93.2

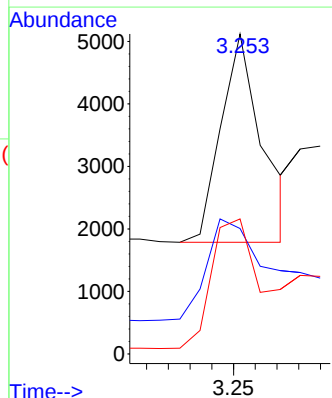







#3
n-Nitrosodimethylamine
Concen: 0.38 ng
RT: 3.576 min Scan# 54
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion: 42 Resp: 7062




Ion	Ratio	Lower	Upper
42	100		
74	155.0	124.0	186.0
44	7.0	5.6	8.4

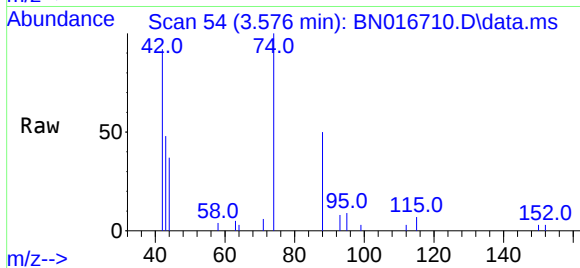


#4
2-Fluorophenol
Concen: 0.38 ng
RT: 5.254 min Scan# 236
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion: 112 Resp: 24432

Ion	Ratio	Lower	Upper
112	100		
64	53.6	42.9	64.3
63	26.9	21.5	32.3


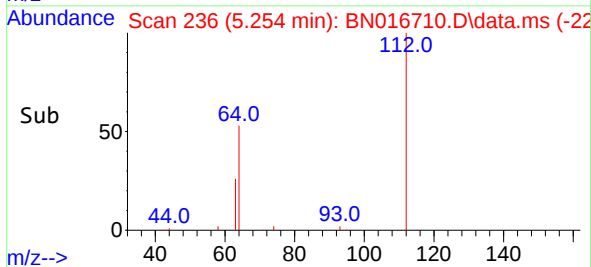

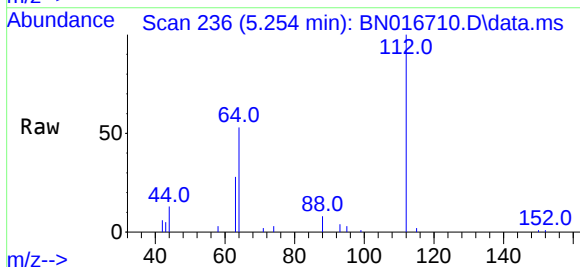




#5
Phenol-d6
Concen: 0.38 ng
RT: 6.821 min Scan# 406
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion: 99 Resp: 26787
Ion Ratio Lower Upper
99 100
42 16.8 13.4 20.2
71 30.0 24.0 36.0

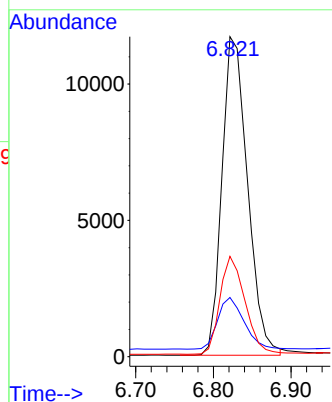

#6
bis(2-Chloroethyl)ether
Concen: 0.39 ng
RT: 7.080 min Scan# 434
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion: 93 Resp: 26760
Ion Ratio Lower Upper
93 100
63 73.8 59.0 88.6
95 33.0 26.4 39.6


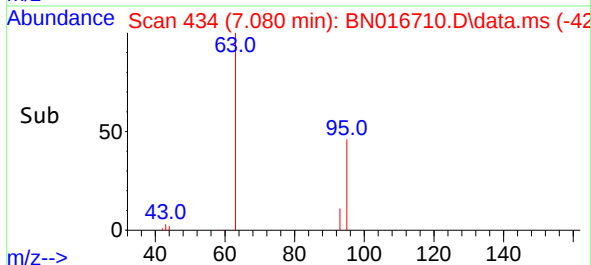

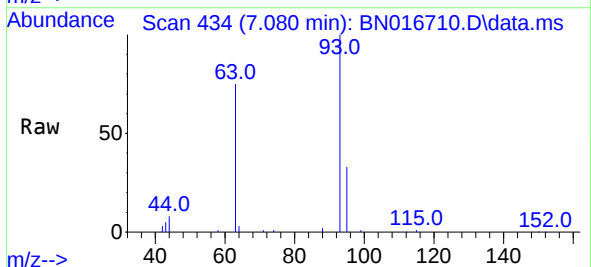




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.406 min Scan# 733
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	136	Resp:	112431
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.9	13.3
54	8.1	6.5	9.7
68	6.6	5.3	7.9



#8
Nitrobenzene-d5
Concen: 0.37 ng
RT: 8.784 min Scan# 605
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion:	82	Resp:	27001
Ion	Ratio	Lower	Upper
82	100		
128	42.2	33.8	50.6
54	48.1	38.5	57.7



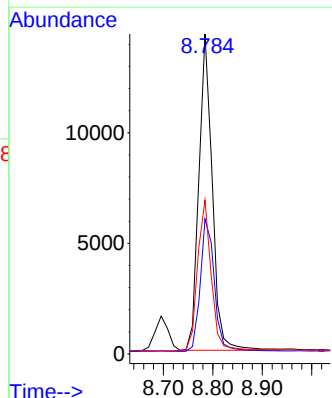





#9
Naphthalene
Concen: 0.38 ng
RT: 10.457 min Scan# 737
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:128 Resp: 116710
Ion Ratio Lower Upper
128 100
129 10.9 8.7 13.1
127 12.9 10.3 15.5



#10
Hexachlorobutadiene
Concen: 0.38 ng
RT: 10.748 min Scan# 760
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion:225 Resp: 21988
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.9 51.1 76.7


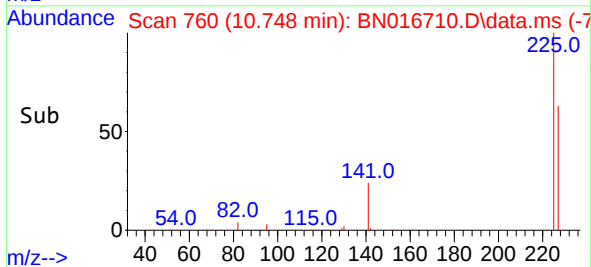

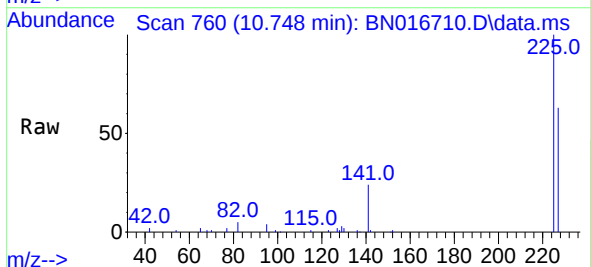


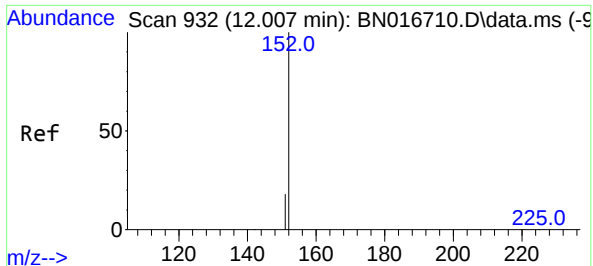

#11
2-Methylnaphthalene-d10
Concen: 0.38 ng
RT: 12.007 min Scan# 932
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:152 Resp: 63795
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.4

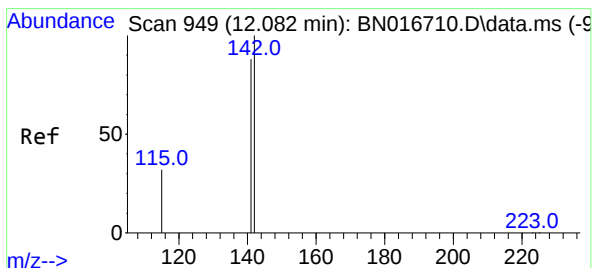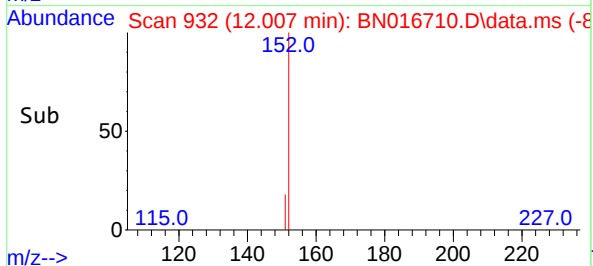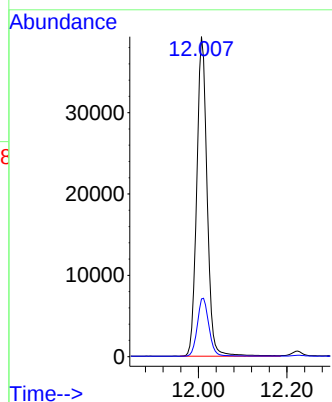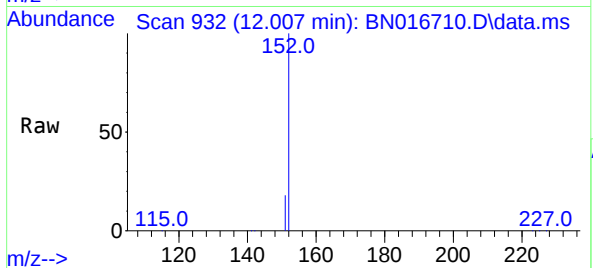

#12
2-Methylnaphthalene
Concen: 0.39 ng
RT: 12.082 min Scan# 949
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion:142 Resp: 75453
Ion Ratio Lower Upper
142 100
141 88.3 70.6 106.0
115 32.6 26.1 39.1


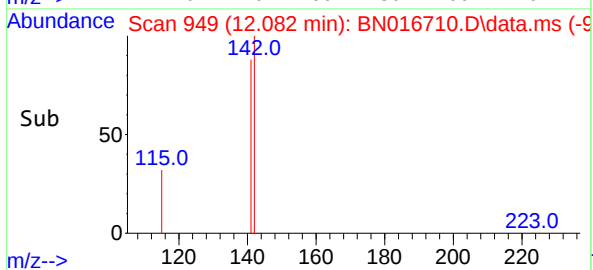
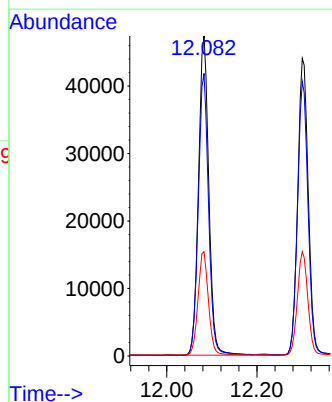
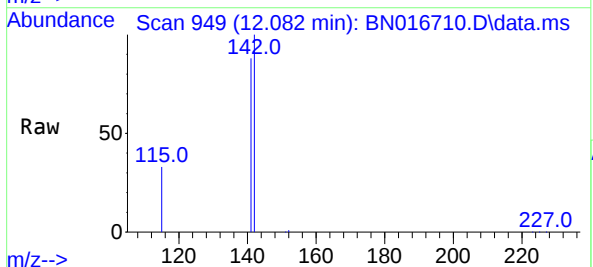




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.268 min Scan# 1183
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:164 Resp: 59809
Ion Ratio Lower Upper
164 100
162 103.3 82.6 124.0
160 47.7 38.2 57.2

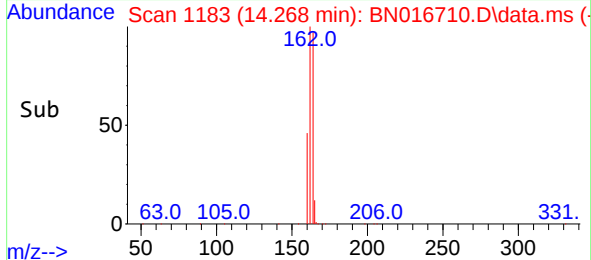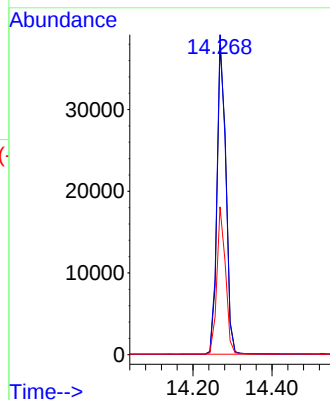

#14
2,4,6-Tribromophenol
Concen: 0.31 ng
RT: 15.778 min Scan# 1302
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion:330 Resp: 8405
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 30.1 24.2 36.2


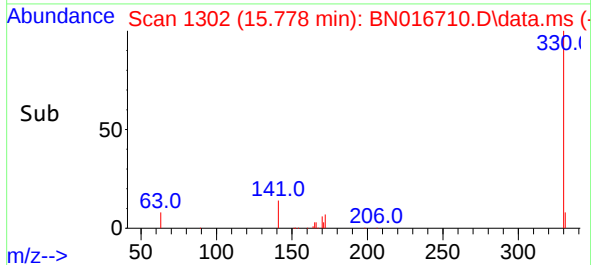
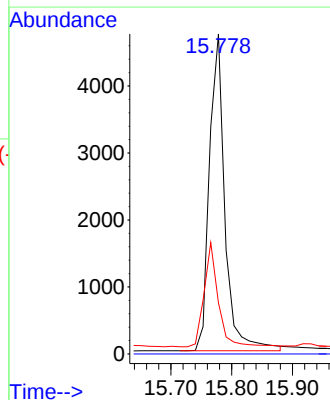
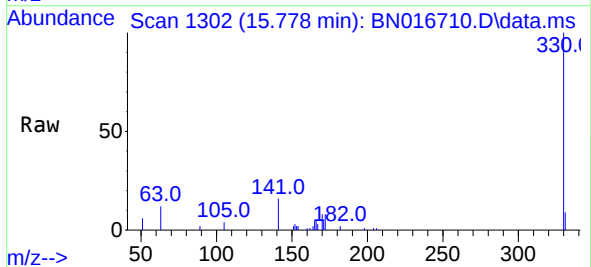




#15
2-Fluorobiphenyl
Concen: 0.37 ng
RT: 12.898 min Scan# 1075
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:172 Resp: 89068
Ion Ratio Lower Upper
172 100
171 33.6 26.9 40.3
170 21.7 17.4 26.0

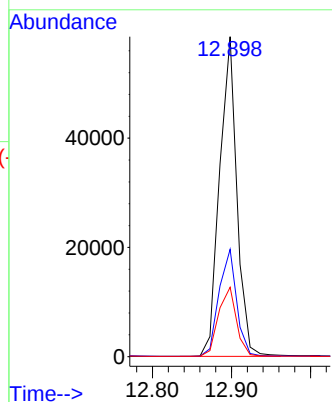

#16
Acenaphthylene
Concen: 0.36 ng
RT: 13.989 min Scan# 1161
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion:152 Resp: 95374
Ion Ratio Lower Upper
152 100
151 19.4 15.5 23.3
153 13.0 10.4 15.6


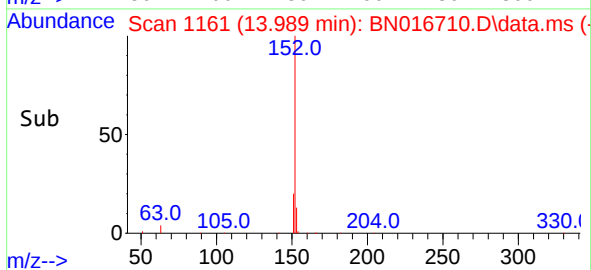
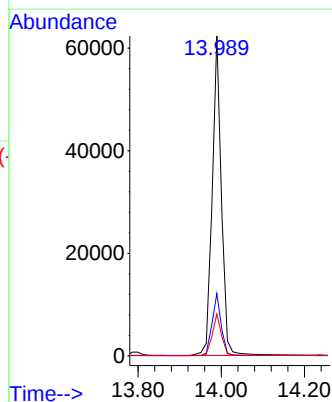



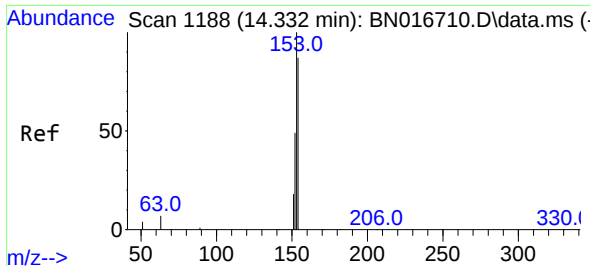

#17
Acenaphthene
Concen: 0.37 ng
RT: 14.332 min Scan# 1188
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:154 Resp: 65362
Ion Ratio Lower Upper
154 100
153 112.6 90.1 135.1
152 54.5 43.6 65.4

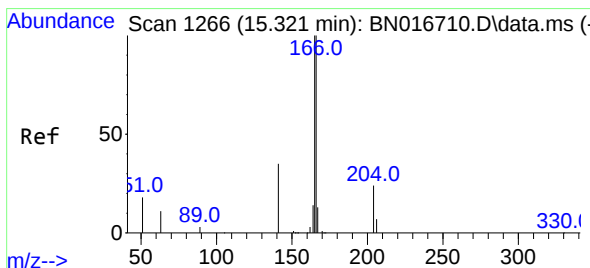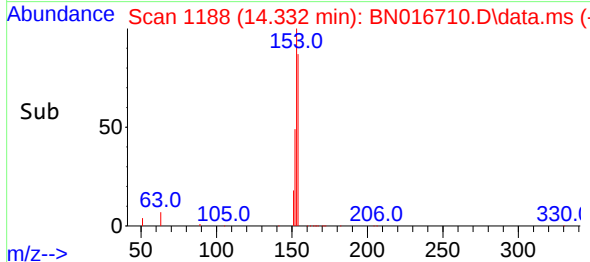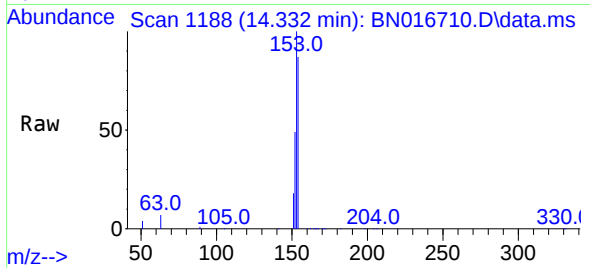

#18
Fluorene
Concen: 0.38 ng
RT: 15.321 min Scan# 1266
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion:166 Resp: 78129
Ion Ratio Lower Upper
166 100
165 97.6 78.1 117.1
167 13.4 10.7 16.1


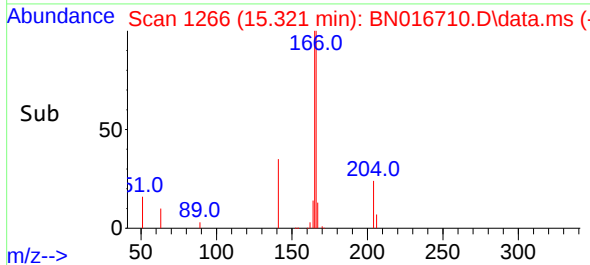

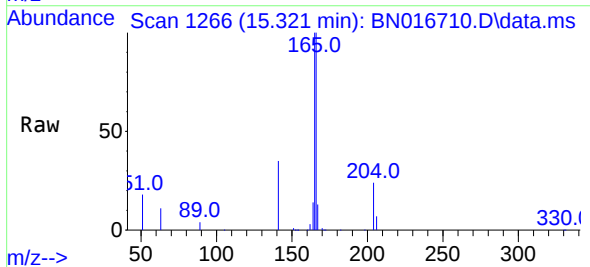




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.029 min Scan# 1404
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:188 Resp: 111207
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.3 5.8 8.8

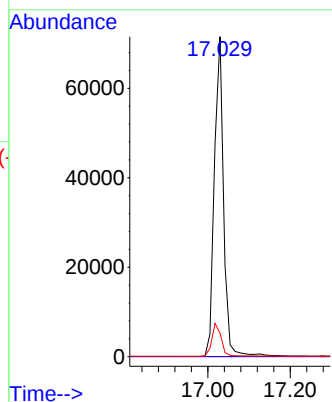

#20
4,6-Dinitro-2-methylphenol
Concen: 0.04 ng
RT: 15.423 min Scan# 1274
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion:198 Resp: 467
Ion Ratio Lower Upper
198 100
182 32.7 26.2 39.2
77 0.0 0.0 0.0


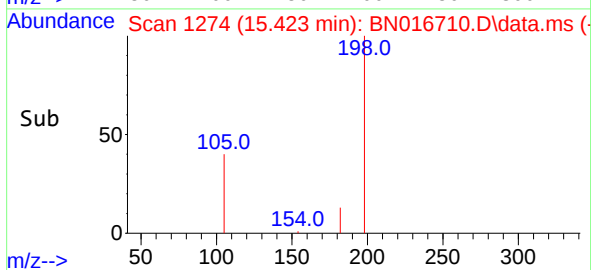




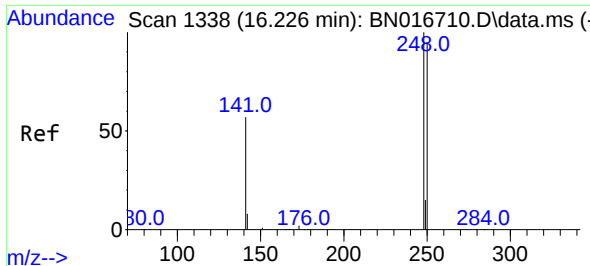

#21
4-Bromophenyl-phenylether
Concen: 0.36 ng
RT: 16.226 min Scan# 1338
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:248 Resp: 24597
Ion Ratio Lower Upper
248 100
250 95.3 76.2 114.4
141 57.0 45.6 68.4

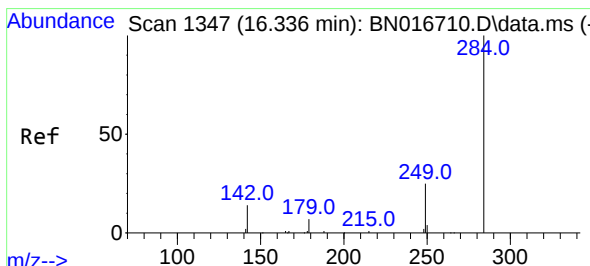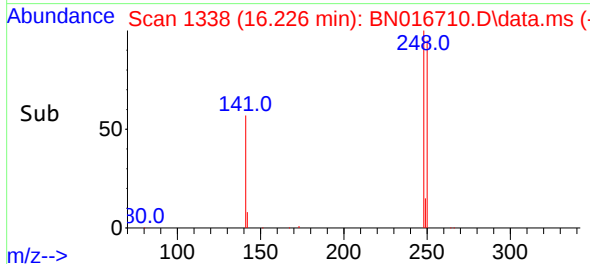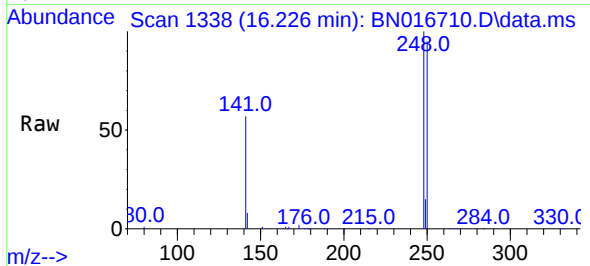

#22
Hexachlorobenzene
Concen: 0.36 ng
RT: 16.336 min Scan# 1347
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion:284 Resp: 28830
Ion Ratio Lower Upper
284 100
142 32.2 25.8 38.6
249 29.1 23.3 34.9


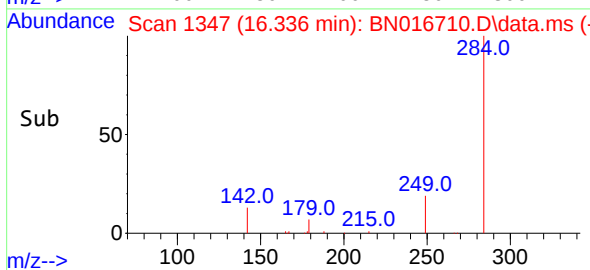

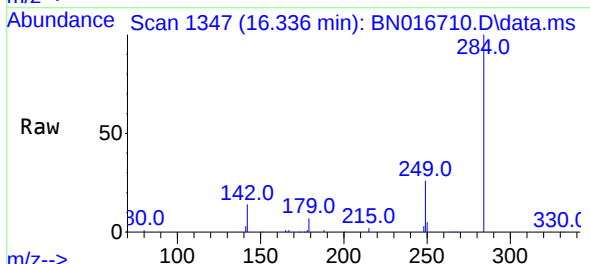


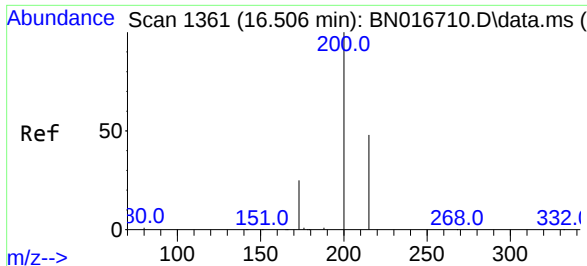

#23
Atrazine
Concen: 0.35 ng
RT: 16.506 min Scan# 1361
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:200 Resp: 17631
Ion Ratio Lower Upper
200 100
173 25.1 20.1 30.1
215 48.5 38.8 58.2

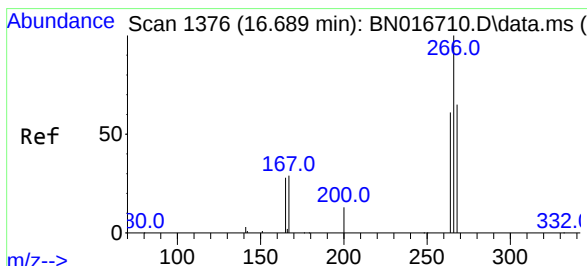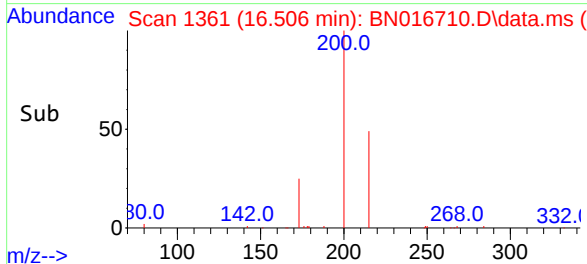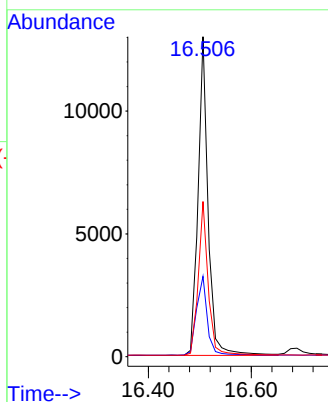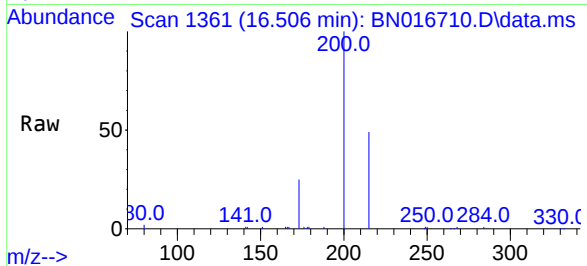

#24
Pentachlorophenol
Concen: 0.14 ng
RT: 16.689 min Scan# 1376
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion:266 Resp: 3618
Ion Ratio Lower Upper
266 100
264 62.5 49.3 73.9
268 65.0 51.8 77.8


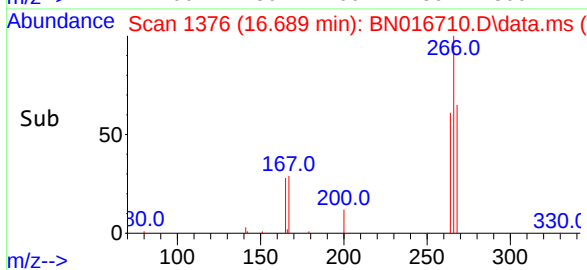
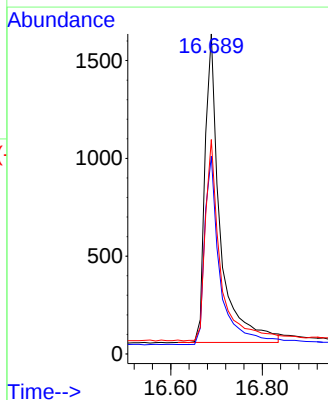
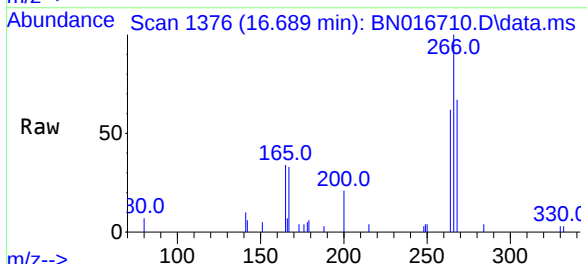




#25
Phenanthrene
Concen: 0.37 ng
RT: 17.066 min Scan# 1407
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:178 Resp: 123259
Ion Ratio Lower Upper
178 100
176 18.8 15.0 22.6
179 15.5 12.4 18.6

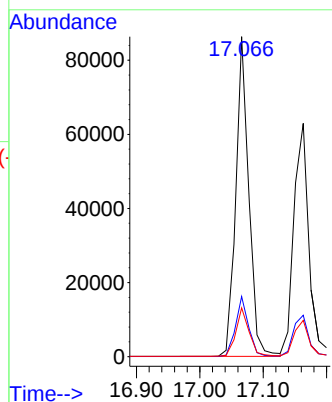

#26
Anthracene
Concen: 0.36 ng
RT: 17.163 min Scan# 1415
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion:178 Resp: 104221
Ion Ratio Lower Upper
178 100
176 18.1 14.5 21.7
179 15.3 12.2 18.4


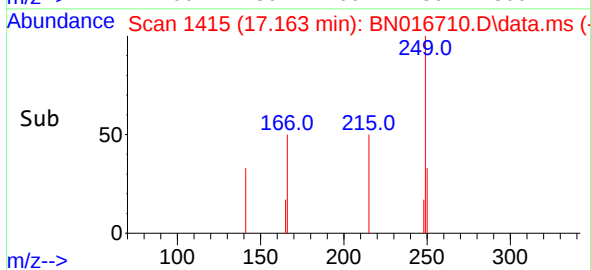






#27
Fluoranthene-d10
Concen: 0.38 ng
RT: 19.068 min Scan# 1697
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:212 Resp: 112103
Ion Ratio Lower Upper
212 100
106 13.3 10.6 16.0
104 7.3 5.8 8.8

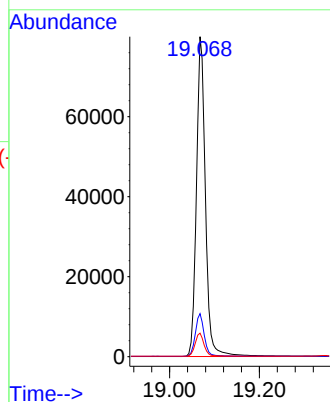

#28
Fluoranthene
Concen: 0.38 ng
RT: 19.097 min Scan# 1703
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion:202 Resp: 137115
Ion Ratio Lower Upper
202 100
101 11.1 8.9 13.3
203 17.3 13.8 20.8



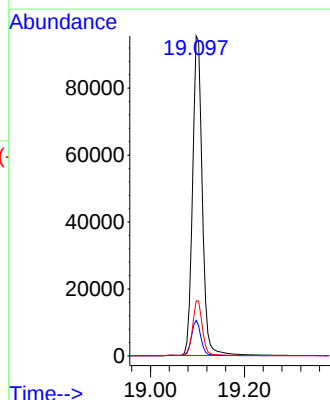





#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.238 min Scan# 2002
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:240 Resp: 102448
Ion Ratio Lower Upper
240 100
120 8.3 6.6 10.0
236 25.9 20.7 31.1

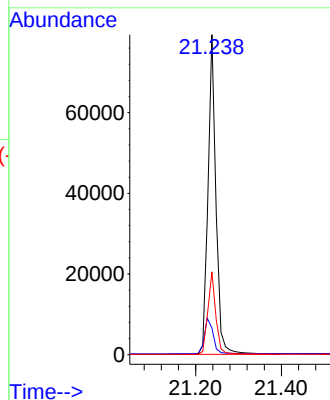

#30
Pyrene
Concen: 0.42 ng
RT: 19.465 min Scan# 1777
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion:202 Resp: 137639
Ion Ratio Lower Upper
202 100
200 20.6 16.5 24.7
203 17.4 13.9 20.9


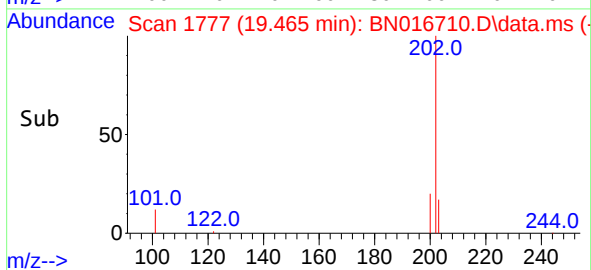
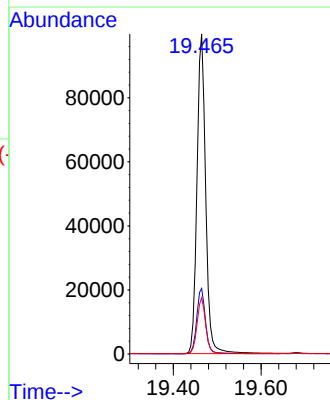





#31
 Terphenyl-d14
 Concen: 0.42 ng
 RT: 19.683 min Scan# 1821
 Delta R.T. 0.000 min
 Lab File: BN016710.D
 Acq: 04 Oct 2021 14:41




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4


Tgt Ion:244 Resp: 92888
 Ion Ratio Lower Upper
 244 100
 212 7.2 5.8 8.6
 122 11.1 8.9 13.3

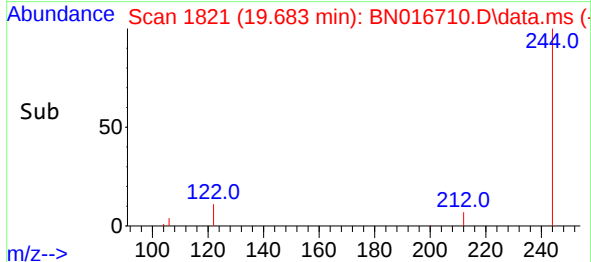

#32
 Benzo(a)anthracene
 Concen: 0.40 ng
 RT: 21.216 min Scan# 2000
 Delta R.T. 0.000 min
 Lab File: BN016710.D
 Acq: 04 Oct 2021 14:41

Tgt Ion:228 Resp: 126207
 Ion Ratio Lower Upper
 228 100
 226 27.9 22.3 33.5
 229 19.2 15.4 23.0



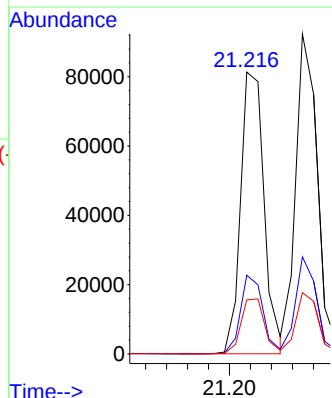



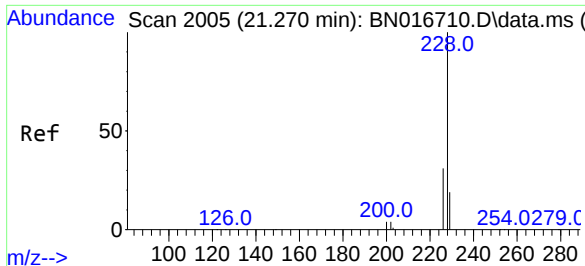

#33
Chrysene
Concen: 0.42 ng
RT: 21.270 min Scan# 2005
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:228 Resp: 132155
Ion Ratio Lower Upper
228 100
226 30.3 24.2 36.4
229 19.2 15.4 23.0

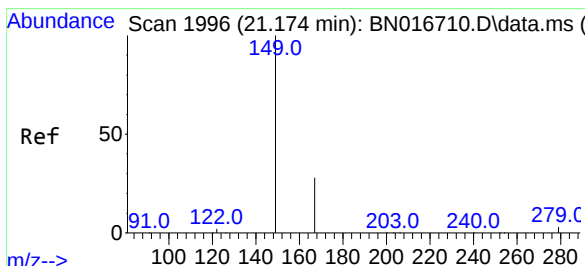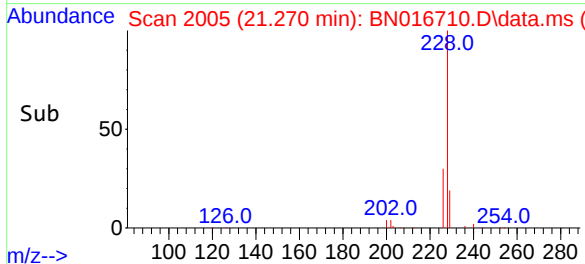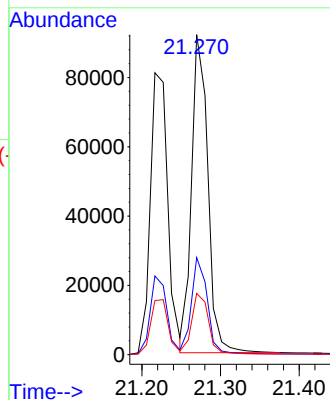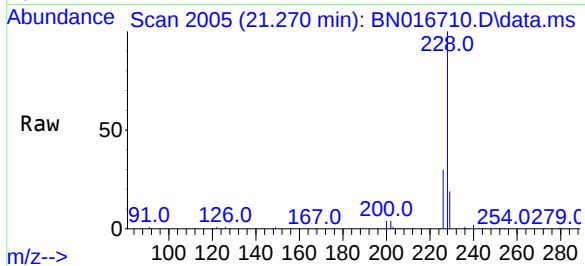

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.54 ng
RT: 21.174 min Scan# 1996
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41


Tgt Ion:149 Resp: 67092
Ion Ratio Lower Upper
149 100
167 27.8 22.2 33.4
279 4.3 3.4 5.2

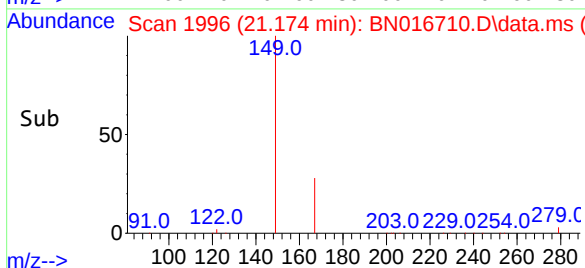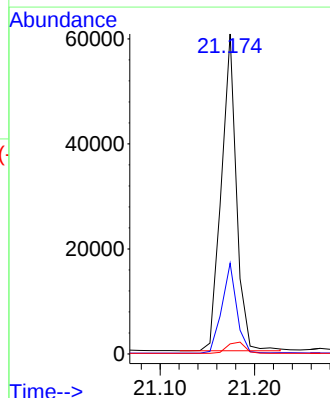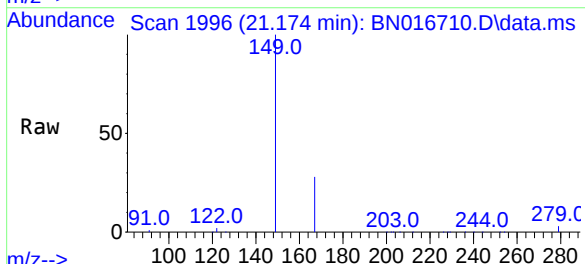






#35
Perylene-d12
Concen: 0.40 ng
RT: 23.494 min Scan# 2430
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4







Tgt Ion:264 Resp: 98715
Ion Ratio Lower Upper
264 100
260 24.7 19.8 29.6
265 25.4 20.3 30.5

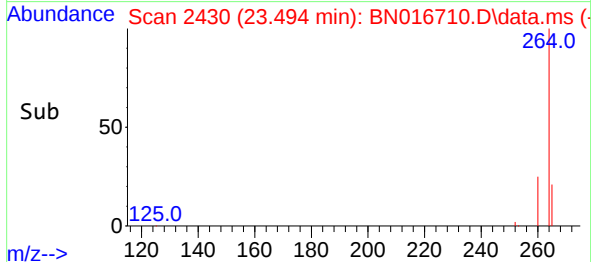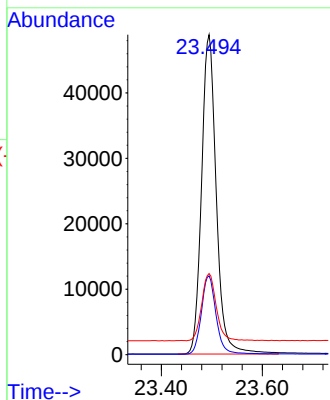

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.34 ng
RT: 25.781 min Scan# 3098
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion:276 Resp: 118655
Ion Ratio Lower Upper
276 100
138 24.0 19.2 28.8
277 25.0 20.0 30.0


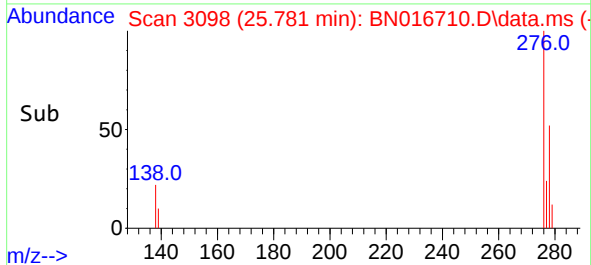
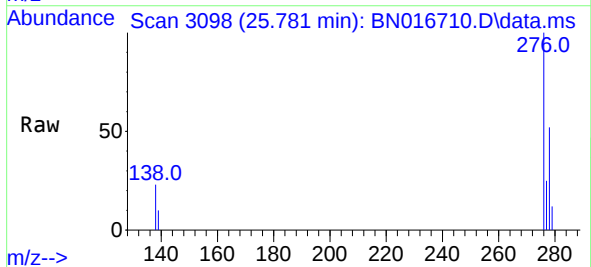
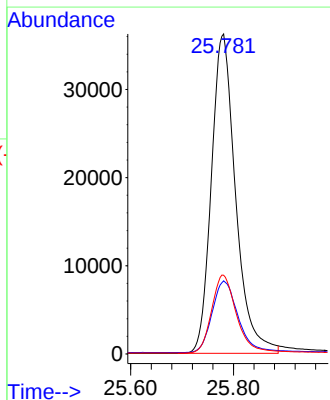




#37
Benzo(b)fluoranthene
Concen: 0.41 ng
RT: 22.813 min Scan# 2231
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:252 Resp: 131541
Ion Ratio Lower Upper
252 100
253 22.3 17.8 26.8
125 10.4 8.3 12.5

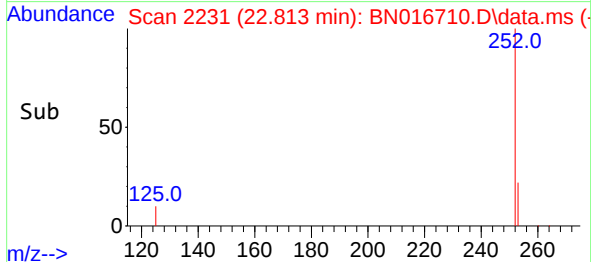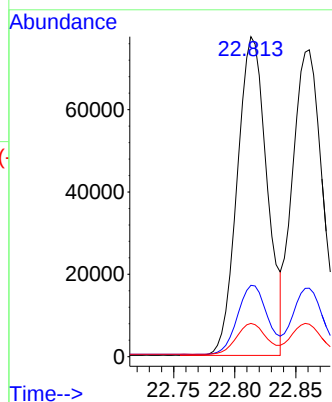

#38
Benzo(k)fluoranthene
Concen: 0.40 ng
RT: 22.861 min Scan# 2245
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41


Tgt Ion:252 Resp: 124259
Ion Ratio Lower Upper
252 100
253 22.3 17.8 26.8
125 10.6 8.5 12.7

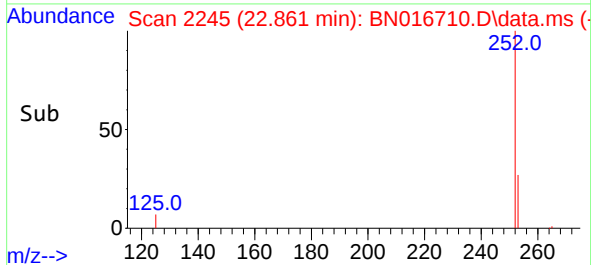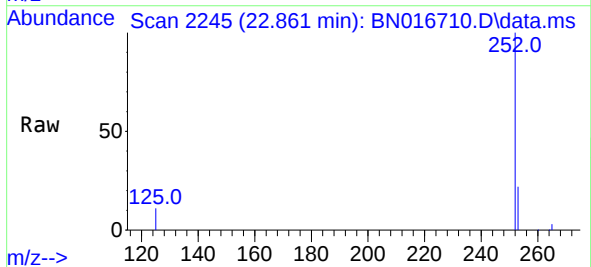






#39
Benzo(a)pyrene
Concen: 0.41 ng
RT: 23.392 min Scan# 2400
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4







Tgt Ion:252 Resp: 115306
Ion Ratio Lower Upper
252 100
253 22.4 17.9 26.9
125 11.8 9.4 14.2

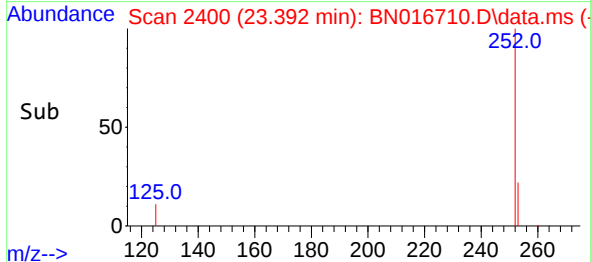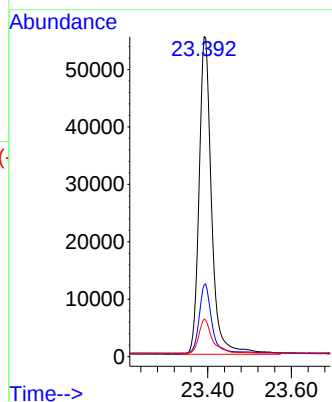

#40
Dibenzo(a,h)anthracene
Concen: 0.33 ng
RT: 25.798 min Scan# 3103
Delta R.T. 0.000 min
Lab File: BN016710.D
Acq: 04 Oct 2021 14:41

Tgt Ion:278 Resp: 92771
Ion Ratio Lower Upper
278 100
139 16.4 13.1 19.7
279 24.1 19.3 28.9

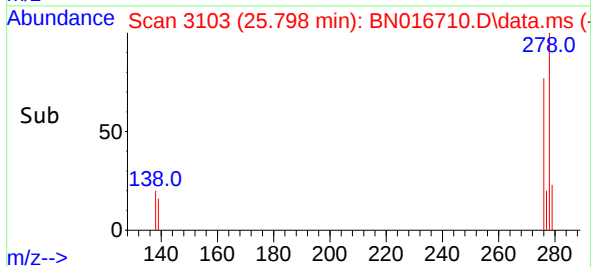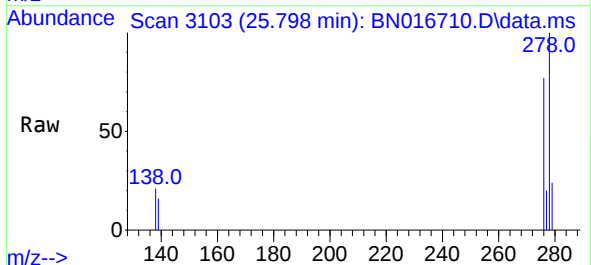

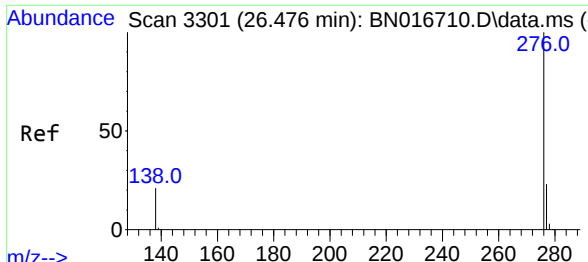

#41
 Benzo(g,h,i)perylene
 Concen: 0.35 ng
 RT: 26.476 min Scan# 3301
 Delta R.T. 0.000 min
 Lab File: BN016710.D
 Acq: 04 Oct 2021 14:41

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4

Tgt Ion:276 Resp: 107635
 Ion Ratio Lower Upper
 276 100
 277 23.7 19.0 28.4
 138 21.3 17.0 25.6

