

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
 Data File : BN016712.D
 Acq On : 04 Oct 2021 15:54
 Operator : CG/JU
 Sample : SSTDIC0.8
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC0.8

Quant Time: Oct 04 16:33:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 04 15:14:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.642	152	26485	0.40	ng	0.00
7) Naphthalene-d8	10.406	136	115912	0.40	ng	0.00
13) Acenaphthene-d10	14.268	164	60221	0.40	ng	0.00
19) Phenanthrene-d10	17.029	188	109681	0.40	ng	0.00
29) Chrysene-d12	21.238	240	105556	0.40	ng	0.00
35) Perylene-d12	23.494	264	102515	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.254	112	55568	0.82	ng	0.00
5) Phenol-d6	6.822	99	62164	0.84	ng	0.00
8) Nitrobenzene-d5	8.784	82	64208	0.85	ng	0.00
11) 2-Methylnaphthalene-d10	12.007	152	141272	0.82	ng	0.00
14) 2,4,6-Tribromophenol	15.778	330	21614	0.79	ng	0.00
15) 2-Fluorobiphenyl	12.898	172	194584	0.80	ng	0.00
27) Fluoranthene-d10	19.073	212	246211	0.84	ng	0.00
31) Terphenyl-d14	19.683	244	201257	0.88	ng	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.253	88	10842	0.89	ng	# 76
3) n-Nitrosodimethylamine	3.576	42	16934	0.87	ng	99
6) bis(2-Chloroethyl)ether	7.080	93	60405	0.84	ng	99
9) Naphthalene	10.457	128	255989	0.81	ng	100
10) Hexachlorobutadiene	10.749	225	48132	0.81	ng	# 100
12) 2-Methylnaphthalene	12.083	142	165475	0.82	ng	99
16) Acenaphthylene	13.989	152	222819	0.85	ng	100
17) Acenaphthene	14.332	154	144188	0.81	ng	100
18) Fluorene	15.334	166	174472	0.83	ng	100
20) 4,6-Dinitro-2-methylph...	15.423	198	4100	0.32	ng	# 65
21) 4-Bromophenyl-phenylether	16.226	248	55633	0.82	ng	99
22) Hexachlorobenzene	16.336	284	62362	0.79	ng	100
23) Atrazine	16.506	200	42184	0.85	ng	99
24) Pentachlorophenol	16.689	266	14430	0.55	ng	99
25) Phenanthrene	17.066	178	265492	0.80	ng	100
26) Anthracene	17.163	178	236907	0.83	ng	100
28) Fluoranthene	19.097	202	297440	0.83	ng	100
30) Pyrene	19.465	202	300875	0.88	ng	100
32) Benzo(a)anthracene	21.227	228	281761	0.87	ng	96
33) Chrysene	21.270	228	287978	0.88	ng	100
34) Bis(2-ethylhexyl)phtha...	21.174	149	146899	1.14	ng	100
36) Indeno(1,2,3-cd)pyrene	25.778	276	295724	0.81	ng	100
37) Benzo(b)fluoranthene	22.813	252	289768	0.88	ng	99
38) Benzo(k)fluoranthene	22.861	252	284393	0.87	ng	100
39) Benzo(a)pyrene	23.395	252	261119	0.89	ng	99
40) Dibenzo(a,h)anthracene	25.802	278	235314	0.80	ng	99
41) Benzo(g,h,i)perylene	26.476	276	258586	0.80	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016712.D
Acq On : 04 Oct 2021 15:54
Operator : CG/JU
Sample : SSTDICC0.8
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Quant Time: Oct 04 16:33:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 04 15:14:53 2021
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.642 min Scan# 495
 Delta R.T. 0.000 min
 Lab File: BN016712.D
 Acq: 04 Oct 2021 15:54




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:152 Resp: 26485
 Ion Ratio Lower Upper
 152 100
 150 156.2 123.3 184.9
 115 58.7 47.0 70.6



#2
 1,4-Dioxane
 Concen: 0.89 ng
 RT: 3.253 min Scan# 19
 Delta R.T. 0.000 min
 Lab File: BN016712.D
 Acq: 04 Oct 2021 15:54

Tgt Ion: 88 Resp: 10842
 Ion Ratio Lower Upper
 88 100
 43 39.7 61.7 92.5#
 58 72.6 62.2 93.2









#3
n-Nitrosodimethylamine
Concen: 0.87 ng
RT: 3.576 min Scan# 54
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion: 42 Resp: 16934




Ion	Ratio	Lower	Upper
42	100		
74	153.4	124.0	186.0
44	6.6	5.6	8.4




#4
2-Fluorophenol
Concen: 0.82 ng
RT: 5.254 min Scan# 236
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion: 112 Resp: 55568

Ion	Ratio	Lower	Upper
112	100		
64	53.8	42.9	64.3
63	27.1	21.5	32.3









#5
Phenol-d6
Concen: 0.84 ng
RT: 6.822 min Scan# 406
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion: 99 Resp: 62164
Ion Ratio Lower Upper
99 100
42 16.6 13.4 20.2
71 29.9 24.0 36.0



#6
bis(2-Chloroethyl)ether
Concen: 0.84 ng
RT: 7.080 min Scan# 434
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion: 93 Resp: 60405
Ion Ratio Lower Upper
93 100
63 72.7 59.0 88.6
95 32.7 26.4 39.6









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.406 min Scan# 733
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	136	Resp:	115912
Ion Ratio	Lower	Upper	
136	100		
137	10.9	8.9	13.3
54	8.0	6.5	9.7
68	6.6	5.3	7.9



#8
Nitrobenzene-d5
Concen: 0.85 ng
RT: 8.784 min Scan# 605
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion:	82	Resp:	64208
Ion Ratio	Lower	Upper	
82	100		
128	42.0	33.8	50.6
54	46.9	38.5	57.7









#9
Naphthalene
Concen: 0.81 ng
RT: 10.457 min Scan# 737
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:128 Resp: 255989
Ion Ratio Lower Upper
128 100
129 10.9 8.7 13.1
127 13.0 10.3 15.5



#10
Hexachlorobutadiene
Concen: 0.81 ng
RT: 10.749 min Scan# 760
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion:225 Resp: 48132
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.1 51.1 76.7







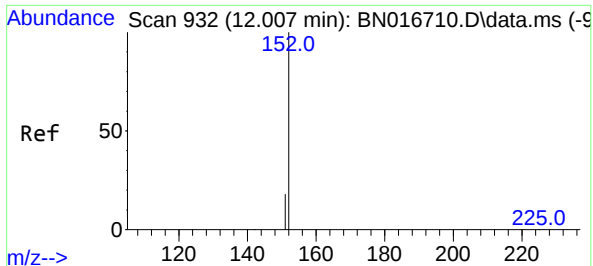

#11
2-Methylnaphthalene-d10
Concen: 0.82 ng
RT: 12.007 min Scan# 932
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:152 Resp: 141272
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.4



#12
2-Methylnaphthalene
Concen: 0.82 ng
RT: 12.083 min Scan# 949
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion:142 Resp: 165475
Ion Ratio Lower Upper
142 100
141 87.1 70.6 106.0
115 31.9 26.1 39.1









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.268 min Scan# 1183
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:164 Resp: 60221
Ion Ratio Lower Upper
164 100
162 103.9 82.6 124.0
160 47.9 38.2 57.2



#14
2,4,6-Tribromophenol
Concen: 0.79 ng
RT: 15.778 min Scan# 1302
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion:330 Resp: 21614
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 30.0 24.2 36.2









#15
2-Fluorobiphenyl
Concen: 0.80 ng
RT: 12.898 min Scan# 1075
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:172 Resp: 194584
Ion Ratio Lower Upper
172 100
171 34.0 26.9 40.3
170 22.1 17.4 26.0



#16
Acenaphthylene
Concen: 0.85 ng
RT: 13.989 min Scan# 1161
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion:152 Resp: 222819
Ion Ratio Lower Upper
152 100
151 19.4 15.5 23.3
153 13.1 10.4 15.6







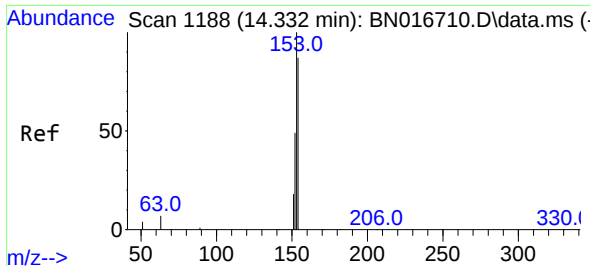

#17
Acenaphthene
Concen: 0.81 ng
RT: 14.332 min Scan# 1188
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:154 Resp: 144188
Ion Ratio Lower Upper
154 100
153 112.8 90.1 135.1
152 54.4 43.6 65.4

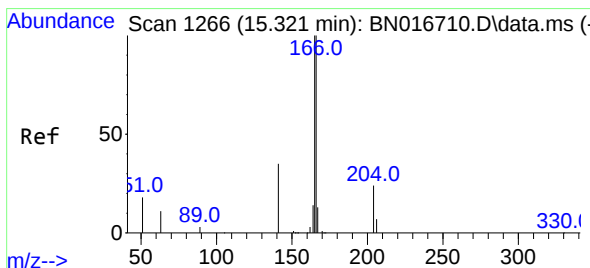

#18
Fluorene
Concen: 0.83 ng
RT: 15.334 min Scan# 1267
Delta R.T. 0.013 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion:166 Resp: 174472
Ion Ratio Lower Upper
166 100
165 97.8 78.1 117.1
167 13.4 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.029 min Scan# 1404
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:188 Resp: 109681
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.6 5.8 8.8



#20
4,6-Dinitro-2-methylphenol
Concen: 0.32 ng
RT: 15.423 min Scan# 1274
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54


Tgt Ion:198 Resp: 4100
Ion Ratio Lower Upper
198 100
182 13.2 26.2 39.2#
77 0.0 0.0 0.0








#21
4-Bromophenyl-phenylether
Concen: 0.82 ng
RT: 16.226 min Scan# 1338
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8




Tgt Ion:248 Resp: 55633

Ion	Ratio	Lower	Upper
248	100		
250	95.0	76.2	114.4
141	58.7	45.6	68.4






#22
Hexachlorobenzene
Concen: 0.79 ng
RT: 16.336 min Scan# 1347
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54



Tgt Ion:284 Resp: 62362

Ion	Ratio	Lower	Upper
284	100		
142	32.3	25.8	38.6
249	29.4	23.3	34.9







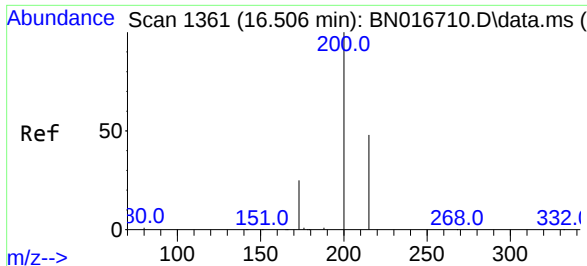

#23
Atrazine
Concen: 0.85 ng
RT: 16.506 min Scan# 1361
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:200 Resp: 42184
Ion Ratio Lower Upper
200 100
173 25.5 20.1 30.1
215 47.9 38.8 58.2

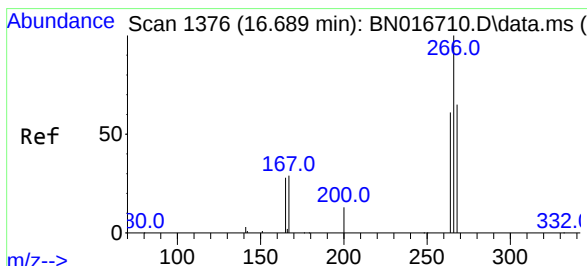

#24
Pentachlorophenol
Concen: 0.55 ng
RT: 16.689 min Scan# 1376
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion:266 Resp: 14430
Ion Ratio Lower Upper
266 100
264 62.9 49.3 73.9
268 63.9 51.8 77.8









#25
Phenanthrene
Concen: 0.80 ng
RT: 17.066 min Scan# 1407
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:178 Resp: 265492
Ion Ratio Lower Upper
178 100
176 18.9 15.0 22.6
179 15.5 12.4 18.6



#26
Anthracene
Concen: 0.83 ng
RT: 17.163 min Scan# 1415
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion:178 Resp: 236907
Ion Ratio Lower Upper
178 100
176 18.3 14.5 21.7
179 15.3 12.2 18.4









#27
Fluoranthene-d10
Concen: 0.84 ng
RT: 19.073 min Scan# 1698
Delta R.T. 0.005 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:212 Resp: 246211
Ion Ratio Lower Upper
212 100
106 13.3 10.6 16.0
104 7.3 5.8 8.8



#28
Fluoranthene
Concen: 0.83 ng
RT: 19.097 min Scan# 1703
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion:202 Resp: 297440
Ion Ratio Lower Upper
202 100
101 11.1 8.9 13.3
203 17.4 13.8 20.8









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.238 min Scan# 2002
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:240 Resp: 105556
Ion Ratio Lower Upper
240 100
120 8.7 6.6 10.0
236 26.0 20.7 31.1



#30
Pyrene
Concen: 0.88 ng
RT: 19.465 min Scan# 1777
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion:202 Resp: 300875
Ion Ratio Lower Upper
202 100
200 20.5 16.5 24.7
203 17.5 13.9 20.9









#31
Terphenyl-d14
Concen: 0.88 ng
RT: 19.683 min Scan# 1821
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:244 Resp: 201257
Ion Ratio Lower Upper
244 100
212 7.1 5.8 8.6
122 11.2 8.9 13.3



#32
Benzo(a)anthracene
Concen: 0.87 ng
RT: 21.227 min Scan# 2001
Delta R.T. 0.011 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion:228 Resp: 281761
Ion Ratio Lower Upper
228 100
226 25.5 22.3 33.5
229 20.2 15.4 23.0









#33
Chrysene
Concen: 0.88 ng
RT: 21.270 min Scan# 2005
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:228 Resp: 287978
Ion Ratio Lower Upper
228 100
226 30.6 24.2 36.4
229 19.2 15.4 23.0



#34
Bis(2-ethylhexyl)phthalate
Concen: 1.14 ng
RT: 21.174 min Scan# 1996
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54


Tgt Ion:149 Resp: 146899
Ion Ratio Lower Upper
149 100
167 27.9 22.2 33.4
279 4.2 3.4 5.2








#35
Perylene-d12
Concen: 0.40 ng
RT: 23.494 min Scan# 2430
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8







Tgt Ion:264 Resp: 102515
Ion Ratio Lower Upper
264 100
260 24.7 19.8 29.6
265 25.1 20.3 30.5



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.81 ng
RT: 25.778 min Scan# 3097
Delta R.T. -0.003 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion:276 Resp: 295724
Ion Ratio Lower Upper
276 100
138 24.4 19.2 28.8
277 25.0 20.0 30.0









#37
Benzo(b)fluoranthene
Concen: 0.88 ng
RT: 22.813 min Scan# 2231
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:252 Resp: 289768
Ion Ratio Lower Upper
252 100
253 21.9 17.8 26.8
125 9.9 8.3 12.5



#38
Benzo(k)fluoranthene
Concen: 0.87 ng
RT: 22.861 min Scan# 2245
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54


Tgt Ion:252 Resp: 284393
Ion Ratio Lower Upper
252 100
253 22.1 17.8 26.8
125 10.4 8.5 12.7








#39
Benzo(a)pyrene
Concen: 0.89 ng
RT: 23.395 min Scan# 2401
Delta R.T. 0.004 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8







Tgt Ion:252 Resp: 261119
Ion Ratio Lower Upper
252 100
253 22.1 17.9 26.9
125 11.0 9.4 14.2



#40
Dibenzo(a,h)anthracene
Concen: 0.80 ng
RT: 25.802 min Scan# 3104
Delta R.T. 0.004 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Tgt Ion:278 Resp: 235314
Ion Ratio Lower Upper
278 100
139 16.2 13.1 19.7
279 23.8 19.3 28.9



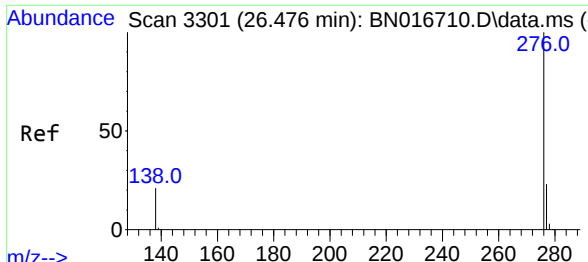

#41
Benzo(g,h,i)perylene
Concen: 0.80 ng
RT: 26.476 min Scan# 3301
Delta R.T. 0.000 min
Lab File: BN016712.D
Acq: 04 Oct 2021 15:54

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion:276 Resp: 258586
Ion Ratio Lower Upper
276 100
277 24.1 19.0 28.4
138 21.1 17.0 25.6

