

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
 Data File : BN016714.D
 Acq On : 04 Oct 2021 17:07
 Operator : CG/JU
 Sample : SSTDIC5.0
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC5.0

Quant Time: Oct 04 17:36:45 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 04 15:14:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.642	152	26279	0.40	ng	0.00
7) Naphthalene-d8	10.406	136	104416	0.40	ng	0.00
13) Acenaphthene-d10	14.268	164	55509	0.40	ng	0.00
19) Phenanthrene-d10	17.029	188	103378	0.40	ng	0.00
29) Chrysene-d12	21.238	240	100292	0.40	ng	# 0.00
35) Perylene-d12	23.494	264	106341	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.254	112	311343	4.65	ng	0.00
5) Phenol-d6	6.831	99	357861	4.88	ng	0.00
8) Nitrobenzene-d5	8.784	82	393432	5.78	ng	0.00
11) 2-Methylnaphthalene-d10	12.007	152	743966	4.82	ng	0.00
14) 2,4,6-Tribromophenol	15.778	330	156460	6.19	ng	0.00
15) 2-Fluorobiphenyl	12.898	172	1039924	4.63	ng	0.00
27) Fluoranthene-d10	19.073	212	1414721	5.15	ng	0.00
31) Terphenyl-d14	19.683	244	1149843	5.27	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.253	88	57662	4.77	ng	# 69
3) n-Nitrosodimethylamine	3.567	42	99714	5.14	ng	100
6) bis(2-Chloroethyl)ether	7.080	93	320660	4.50	ng	99
9) Naphthalene	10.457	128	1334255	4.70	ng	100
10) Hexachlorobutadiene	10.749	225	254482	4.78	ng	# 100
12) 2-Methylnaphthalene	12.082	142	842208	4.65	ng	99
16) Acenaphthylene	13.989	152	1282665	5.28	ng	100
17) Acenaphthene	14.332	154	794277	4.86	ng	98
18) Fluorene	15.334	166	966155	5.00	ng	99
20) 4,6-Dinitro-2-methylph...	15.410	198	96187	8.03	ng	# 54
21) 4-Bromophenyl-phenylether	16.226	248	330472	5.15	ng	99
22) Hexachlorobenzene	16.336	284	352433	4.74	ng	100
23) Atrazine	16.506	200	283830	6.08	ng	97
24) Pentachlorophenol	16.676	266	164978	6.71	ng	99
25) Phenanthrene	17.066	178	1484243	4.77	ng	100
26) Anthracene	17.163	178	1399986	5.21	ng	100
28) Fluoranthene	19.102	202	1613927	4.81	ng	99
30) Pyrene	19.465	202	1703602	5.25	ng	100
32) Benzo(a)anthracene	21.227	228	1691139	5.49	ng	96
33) Chrysene	21.280	228	1641777	5.27	ng	97
34) Bis(2-ethylhexyl)phtha...	21.174	149	1125157	9.17	ng	99
36) Indeno(1,2,3-cd)pyrene	25.781	276	1944096	5.12	ng	100
37) Benzo(b)fluoranthene	22.817	252	1773448	5.19	ng	99
38) Benzo(k)fluoranthene	22.865	252	1691114	5.01	ng	99
39) Benzo(a)pyrene	23.395	252	1634338	5.37	ng	99
40) Dibenzo(a,h)anthracene	25.805	278	1588140	5.19	ng	99
41) Benzo(g,h,i)perylene	26.483	276	1706452	5.09	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016714.D
Acq On : 04 Oct 2021 17:07
Operator : CG/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Oct 04 17:36:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 04 15:14:53 2021
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.642 min Scan# 495
 Delta R.T. 0.000 min
 Lab File: BN016714.D
 Acq: 04 Oct 2021 17:07




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:152 Resp: 26279
 Ion Ratio Lower Upper
 152 100
 150 158.6 123.3 184.9
 115 58.8 47.0 70.6



#2
 1,4-Dioxane
 Concen: 4.77 ng
 RT: 3.253 min Scan# 19
 Delta R.T. 0.000 min
 Lab File: BN016714.D
 Acq: 04 Oct 2021 17:07

Tgt Ion: 88 Resp: 57662
 Ion Ratio Lower Upper
 88 100
 43 28.2 61.7 92.5#
 58 73.6 62.2 93.2









#3
n-Nitrosodimethylamine
Concen: 5.14 ng
RT: 3.567 min Scan# 53
Delta R.T. -0.009 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 99714
Ion Ratio Lower Upper
42 100
74 154.5 124.0 186.0
44 6.4 5.6 8.4



#4
2-Fluorophenol
Concen: 4.65 ng
RT: 5.254 min Scan# 236
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion: 112 Resp: 311343
Ion Ratio Lower Upper
112 100
64 53.6 42.9 64.3
63 27.0 21.5 32.3









#5
Phenol-d6
Concen: 4.88 ng
RT: 6.831 min Scan# 407
Delta R.T. 0.009 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 357861
Ion Ratio Lower Upper
99 100
42 16.5 13.4 20.2
71 29.8 24.0 36.0



#6
bis(2-Chloroethyl)ether
Concen: 4.50 ng
RT: 7.080 min Scan# 434
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion: 93 Resp: 320660
Ion Ratio Lower Upper
93 100
63 72.5 59.0 88.6
95 32.7 26.4 39.6









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.406 min Scan# 733
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:136 Resp: 104416




Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.9	13.3
54	8.0	6.5	9.7
68	6.6	5.3	7.9




#8
Nitrobenzene-d5
Concen: 5.78 ng
RT: 8.784 min Scan# 605
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion: 82 Resp: 393432

Ion	Ratio	Lower	Upper
82	100		
128	44.2	33.8	50.6
54	45.7	38.5	57.7









#9
Naphthalene
Concen: 4.70 ng
RT: 10.457 min Scan# 737
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 1334255
Ion Ratio Lower Upper
128 100
129 11.1 8.7 13.1
127 13.0 10.3 15.5



#10
Hexachlorobutadiene
Concen: 4.78 ng
RT: 10.749 min Scan# 760
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion:225 Resp: 254482
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.2 51.1 76.7









#11
2-Methylnaphthalene-d10
Concen: 4.82 ng
RT: 12.007 min Scan# 932
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 743966
Ion Ratio Lower Upper
152 100
151 20.1 16.2 24.4



#12
2-Methylnaphthalene
Concen: 4.65 ng
RT: 12.082 min Scan# 949
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion:142 Resp: 842208
Ion Ratio Lower Upper
142 100
141 87.2 70.6 106.0
115 32.0 26.1 39.1









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.268 min Scan# 1183
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 55509
Ion Ratio Lower Upper
164 100
162 104.0 82.6 124.0
160 47.8 38.2 57.2



#14
2,4,6-Tribromophenol
Concen: 6.19 ng
RT: 15.778 min Scan# 1302
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion:330 Resp: 156460
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 30.6 24.2 36.2









#15
2-Fluorobiphenyl
Concen: 4.63 ng
RT: 12.898 min Scan# 1075
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:172 Resp: 1039924




Ion	Ratio	Lower	Upper
172	100		
171	33.8	26.9	40.3
170	22.0	17.4	26.0




#16
Acenaphthylene
Concen: 5.28 ng
RT: 13.989 min Scan# 1161
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion:152 Resp: 1282665

Ion	Ratio	Lower	Upper
152	100		
151	19.4	15.5	23.3
153	13.2	10.4	15.6







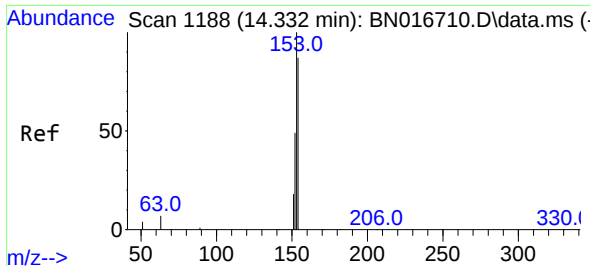

#17
Acenaphthene
Concen: 4.86 ng
RT: 14.332 min Scan# 1188
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 794277
Ion Ratio Lower Upper
154 100
153 110.9 90.1 135.1
152 52.6 43.6 65.4

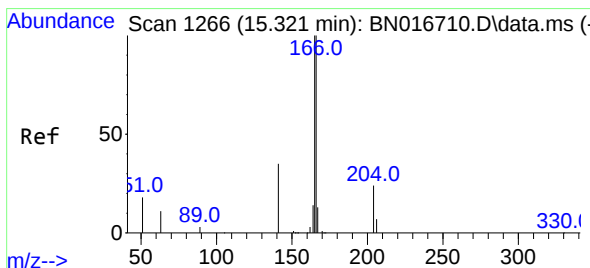

#18
Fluorene
Concen: 5.00 ng
RT: 15.334 min Scan# 1267
Delta R.T. 0.013 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion:166 Resp: 966155
Ion Ratio Lower Upper
166 100
165 96.0 78.1 117.1
167 13.5 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.029 min Scan# 1404
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 103378
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.8 5.8 8.8



#20
4,6-Dinitro-2-methylphenol
Concen: 8.03 ng
RT: 15.410 min Scan# 1273
Delta R.T. -0.013 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion:198 Resp: 96187
Ion Ratio Lower Upper
198 100
182 6.8 26.2 39.2#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 5.15 ng
RT: 16.226 min Scan# 1338
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:248 Resp: 330472
Ion Ratio Lower Upper
248 100
250 93.9 76.2 114.4
141 57.5 45.6 68.4



#22
Hexachlorobenzene
Concen: 4.74 ng
RT: 16.336 min Scan# 1347
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion:284 Resp: 352433
Ion Ratio Lower Upper
284 100
142 32.2 25.8 38.6
249 29.2 23.3 34.9







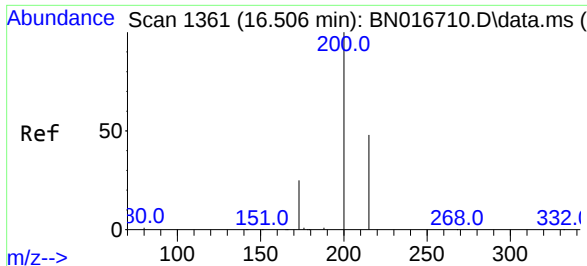

#23
Atrazine
Concen: 6.08 ng
RT: 16.506 min Scan# 1361
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:200 Resp: 283830
Ion Ratio Lower Upper
200 100
173 28.4 20.1 30.1
215 47.3 38.8 58.2

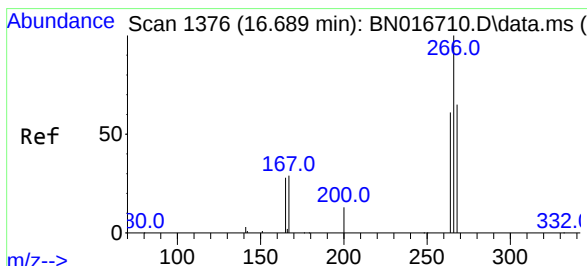

#24
Pentachlorophenol
Concen: 6.71 ng
RT: 16.676 min Scan# 1375
Delta R.T. -0.012 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion:266 Resp: 164978
Ion Ratio Lower Upper
266 100
264 62.4 49.3 73.9
268 64.1 51.8 77.8









#25
Phenanthrene
Concen: 4.77 ng
RT: 17.066 min Scan# 1407
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 1484243
Ion Ratio Lower Upper
178 100
176 18.8 15.0 22.6
179 15.5 12.4 18.6



#26
Anthracene
Concen: 5.21 ng
RT: 17.163 min Scan# 1415
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion:178 Resp: 1399986
Ion Ratio Lower Upper
178 100
176 18.2 14.5 21.7
179 15.6 12.2 18.4









#27
Fluoranthene-d10
Concen: 5.15 ng
RT: 19.073 min Scan# 1698
Delta R.T. 0.005 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 1414721
Ion Ratio Lower Upper
212 100
106 13.4 10.6 16.0
104 7.4 5.8 8.8



#28
Fluoranthene
Concen: 4.81 ng
RT: 19.102 min Scan# 1704
Delta R.T. 0.005 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion:202 Resp: 1613927
Ion Ratio Lower Upper
202 100
101 11.3 8.9 13.3
203 17.6 13.8 20.8









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.238 min Scan# 2002
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 100292
Ion Ratio Lower Upper
240 100
120 10.6 6.6 10.0#
236 26.6 20.7 31.1



#30
Pyrene
Concen: 5.25 ng
RT: 19.465 min Scan# 1777
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion:202 Resp: 1703602
Ion Ratio Lower Upper
202 100
200 20.6 16.5 24.7
203 17.8 13.9 20.9









#31
 Terphenyl-d14
 Concen: 5.27 ng
 RT: 19.683 min Scan# 1821
 Delta R.T. 0.000 min
 Lab File: BN016714.D
 Acq: 04 Oct 2021 17:07

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:244 Resp: 1149843




Ion	Ratio	Lower	Upper
244	100		
212	7.2	5.8	8.6
122	11.8	8.9	13.3




#32
 Benzo(a)anthracene
 Concen: 5.49 ng
 RT: 21.227 min Scan# 2001
 Delta R.T. 0.011 min
 Lab File: BN016714.D
 Acq: 04 Oct 2021 17:07

Tgt Ion:228 Resp: 1691139

Ion	Ratio	Lower	Upper
228	100		
226	25.8	22.3	33.5
229	20.6	15.4	23.0









#33
Chrysene
Concen: 5.27 ng
RT: 21.280 min Scan# 2006
Delta R.T. 0.011 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:228 Resp: 1641777




Ion	Ratio	Lower	Upper
228	100		
226	28.4	24.2	36.4
229	20.3	15.4	23.0




#34
Bis(2-ethylhexyl)phthalate
Concen: 9.17 ng
RT: 21.174 min Scan# 1996
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion:149 Resp: 1125157


Ion	Ratio	Lower	Upper
149	100		
167	28.3	22.2	33.4
279	4.3	3.4	5.2







#35
Perylene-d12
Concen: 0.40 ng
RT: 23.494 min Scan# 2430
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0





Tgt Ion:264 Resp: 106341
Ion Ratio Lower Upper
264 100
260 24.6 19.8 29.6
265 24.7 20.3 30.5




#36
Indeno(1,2,3-cd)pyrene
Concen: 5.12 ng
RT: 25.781 min Scan# 3098
Delta R.T. 0.000 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07



Tgt Ion:276 Resp: 1944096
Ion Ratio Lower Upper
276 100
138 24.3 19.2 28.8
277 25.2 20.0 30.0









#37
Benzo(b)fluoranthene
Concen: 5.19 ng
RT: 22.817 min Scan# 2232
Delta R.T. 0.003 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 1773448
Ion Ratio Lower Upper
252 100
253 22.2 17.8 26.8
125 9.8 8.3 12.5



#38
Benzo(k)fluoranthene
Concen: 5.01 ng
RT: 22.865 min Scan# 2246
Delta R.T. 0.003 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion:252 Resp: 1691114
Ion Ratio Lower Upper
252 100
253 22.3 17.8 26.8
125 9.8 8.5 12.7









#39
Benzo(a)pyrene
Concen: 5.37 ng
RT: 23.395 min Scan# 2401
Delta R.T. 0.003 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 1634338
Ion Ratio Lower Upper
252 100
253 22.0 17.9 26.9
125 10.9 9.4 14.2



#40
Dibenzo(a,h)anthracene
Concen: 5.19 ng
RT: 25.805 min Scan# 3105
Delta R.T. 0.007 min
Lab File: BN016714.D
Acq: 04 Oct 2021 17:07

Tgt Ion:278 Resp: 1588140
Ion Ratio Lower Upper
278 100
139 15.9 13.1 19.7
279 23.9 19.3 28.9



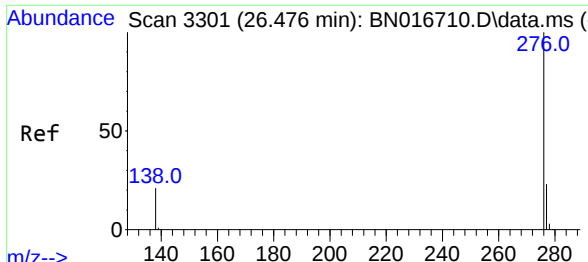

#41
 Benzo(g,h,i)perylene
 Concen: 5.09 ng
 RT: 26.483 min Scan# 3303
 Delta R.T. 0.007 min
 Lab File: BN016714.D
 Acq: 04 Oct 2021 17:07

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:276 Resp: 1706452
 Ion Ratio Lower Upper
 276 100
 277 24.0 19.0 28.4
 138 20.9 17.0 25.6

