

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
 Data File : BN016723.D
 Acq On : 04 Oct 2021 23:12
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Oct 05 03:35:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 04 17:52:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.642	152	26109	0.40	ng	0.00
7) Naphthalene-d8	10.407	136	116210	0.40	ng	0.00
13) Acenaphthene-d10	14.269	164	61216	0.40	ng	0.00
19) Phenanthrene-d10	17.030	188	115894	0.40	ng	0.00
29) Chrysene-d12	21.238	240	115135	0.40	ng	0.00
35) Perylene-d12	23.495	264	121122	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.254	112	25490	0.38	ng	0.00
5) Phenol-d6	6.822	99	28426	0.38	ng	0.00
8) Nitrobenzene-d5	8.784	82	28112	0.35	ng	0.00
11) 2-Methylnaphthalene-d10	12.007	152	65640	0.38	ng	0.00
14) 2,4,6-Tribromophenol	15.779	330	10159	0.40	ng	0.00
15) 2-Fluorobiphenyl	12.898	172	91700	0.37	ng	0.00
27) Fluoranthene-d10	19.068	212	118452	0.37	ng	0.00
31) Terphenyl-d14	19.683	244	99887	0.39	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.253	88	4532	0.37	ng	# 65
3) n-Nitrosodimethylamine	3.594	42	7368	0.37	ng	# 99
6) bis(2-Chloroethyl)ether	7.080	93	27851	0.39	ng	99
9) Naphthalene	10.457	128	119531	0.38	ng	100
10) Hexachlorobutadiene	10.749	225	22610	0.38	ng	# 100
12) 2-Methylnaphthalene	12.078	142	77888	0.39	ng	99
16) Acenaphthylene	13.990	152	99472	0.37	ng	100
17) Acenaphthene	14.332	154	67474	0.38	ng	100
18) Fluorene	15.322	166	82262	0.38	ng	100
20) 4,6-Dinitro-2-methylph...	15.423	198	2377	0.51	ng	# 69
21) 4-Bromophenyl-phenylether	16.226	248	26268	0.37	ng	98
22) Hexachlorobenzene	16.336	284	30337	0.38	ng	100
23) Atrazine	16.506	200	19013	0.34	ng	99
24) Pentachlorophenol	16.689	266	8231	0.55	ng	99
25) Phenanthrene	17.066	178	129125	0.38	ng	100
26) Anthracene	17.164	178	111018	0.36	ng	100
28) Fluoranthene	19.098	202	146341	0.39	ng	100
30) Pyrene	19.465	202	146985	0.39	ng	100
32) Benzo(a)anthracene	21.217	228	139389	0.39	ng	100
33) Chrysene	21.270	228	146208	0.40	ng	100
34) Bis(2-ethylhexyl)phtha...	21.174	149	68331	0.32	ng	100
36) Indeno(1,2,3-cd)pyrene	25.774	276	174036	0.45	ng	99
37) Benzo(b)fluoranthene	22.814	252	152224	0.39	ng	100
38) Benzo(k)fluoranthene	22.858	252	151102	0.40	ng	98
39) Benzo(a)pyrene	23.392	252	138785	0.40	ng	99
40) Dibenzo(a,h)anthracene	25.798	278	139294	0.46	ng	98
41) Benzo(g,h,i)perylene	26.473	276	151830	0.44	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016723.D
Acq On : 04 Oct 2021 23:12
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Quant Time: Oct 05 03:35:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 04 17:52:33 2021
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.642 min Scan# 495
 Delta R.T. 0.000 min
 Lab File: BN016723.D
 Acq: 04 Oct 2021 23:12




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:152 Resp: 26109
 Ion Ratio Lower Upper
 152 100
 150 154.5 123.3 184.9
 115 58.2 47.0 70.6



#2
 1,4-Dioxane
 Concen: 0.37 ng
 RT: 3.253 min Scan# 19
 Delta R.T. 0.000 min
 Lab File: BN016723.D
 Acq: 04 Oct 2021 23:12

Tgt Ion: 88 Resp: 4532
 Ion Ratio Lower Upper
 88 100
 43 28.5 61.7 92.5#
 58 65.2 62.2 93.2









#3
n-Nitrosodimethylamine
Concen: 0.37 ng
RT: 3.594 min Scan# 56
Delta R.T. 0.019 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 42 Resp: 7368
Ion Ratio Lower Upper
42 100
74 154.7 124.0 186.0
44 0.0 5.6 8.4#



#4
2-Fluorophenol
Concen: 0.38 ng
RT: 5.254 min Scan# 236
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion: 112 Resp: 25490
Ion Ratio Lower Upper
112 100
64 54.0 42.9 64.3
63 27.2 21.5 32.3









#5
Phenol-d6
Concen: 0.38 ng
RT: 6.822 min Scan# 406
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 99 Resp: 28426
Ion Ratio Lower Upper
99 100
42 16.7 13.4 20.2
71 29.9 24.0 36.0



#6
bis(2-Chloroethyl)ether
Concen: 0.39 ng
RT: 7.080 min Scan# 434
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion: 93 Resp: 27851
Ion Ratio Lower Upper
93 100
63 73.1 59.0 88.6
95 32.9 26.4 39.6









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.407 min Scan# 733
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	136	Resp:	116210
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.9	13.3
54	7.2	6.5	9.7
68	6.1	5.3	7.9



#8
Nitrobenzene-d5
Concen: 0.35 ng
RT: 8.784 min Scan# 605
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:	82	Resp:	28112
Ion	Ratio	Lower	Upper
82	100		
128	42.6	33.8	50.6
54	47.3	38.5	57.7









#9
Naphthalene
Concen: 0.38 ng
RT: 10.457 min Scan# 737
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:128 Resp: 119531
Ion Ratio Lower Upper
128 100
129 11.1 8.7 13.1
127 13.0 10.3 15.5



#10
Hexachlorobutadiene
Concen: 0.38 ng
RT: 10.749 min Scan# 760
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:225 Resp: 22610
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.0 51.1 76.7







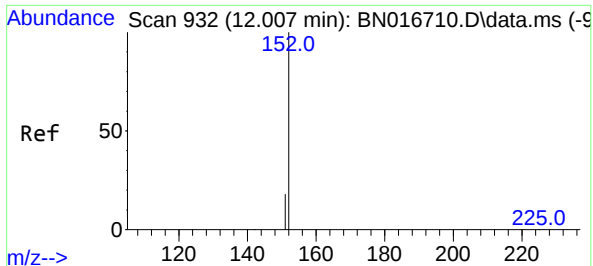

#11
2-Methylnaphthalene-d10
Concen: 0.38 ng
RT: 12.007 min Scan# 932
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 65640
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.4



#12
2-Methylnaphthalene
Concen: 0.39 ng
RT: 12.078 min Scan# 948
Delta R.T. -0.004 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:142 Resp: 77888
Ion Ratio Lower Upper
142 100
141 89.1 70.6 106.0
115 33.1 26.1 39.1









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.269 min Scan# 1183
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:164 Resp: 61216
Ion Ratio Lower Upper
164 100
162 103.6 82.6 124.0
160 47.8 38.2 57.2



#14
2,4,6-Tribromophenol
Concen: 0.40 ng
RT: 15.779 min Scan# 1302
Delta R.T. 0.001 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:330 Resp: 10159
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 30.2 24.2 36.2









#15
2-Fluorobiphenyl
Concen: 0.37 ng
RT: 12.898 min Scan# 1075
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:172	Resp:	91700
Ion Ratio	Lower	Upper
172	100	
171	34.0	26.9 40.3
170	21.9	17.4 26.0



#16
Acenaphthylene
Concen: 0.37 ng
RT: 13.990 min Scan# 1161
Delta R.T. 0.001 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:152	Resp:	99472
Ion Ratio	Lower	Upper
152	100	
151	19.4	15.5 23.3
153	13.0	10.4 15.6







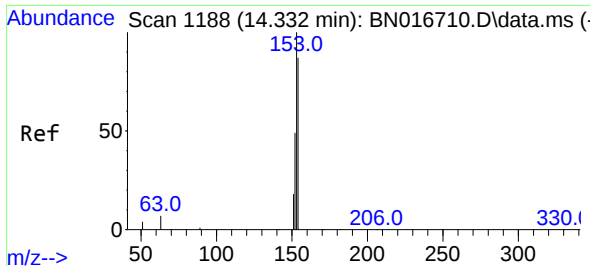

#17
Acenaphthene
Concen: 0.38 ng
RT: 14.332 min Scan# 1188
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:154 Resp: 67474
Ion Ratio Lower Upper
154 100
153 112.4 90.1 135.1
152 54.4 43.6 65.4

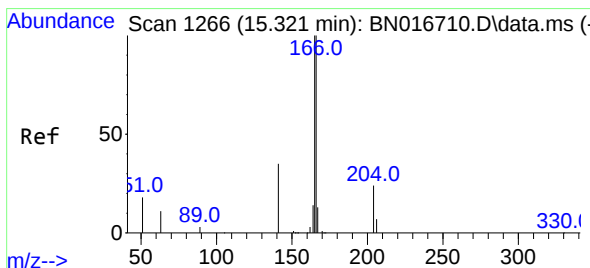

#18
Fluorene
Concen: 0.38 ng
RT: 15.322 min Scan# 1266
Delta R.T. 0.001 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:166 Resp: 82262
Ion Ratio Lower Upper
166 100
165 97.4 78.1 117.1
167 13.4 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.030 min Scan# 1404
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:188 Resp: 115894




Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	6.9	5.8	8.8




#20
4,6-Dinitro-2-methylphenol
Concen: 0.51 ng
RT: 15.423 min Scan# 1274
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:198 Resp: 2377

Ion	Ratio	Lower	Upper
198	100		
182	15.4	26.2	39.2#
77	0.0	0.0	0.0









#21
4-Bromophenyl-phenylether
Concen: 0.37 ng
RT: 16.226 min Scan# 1338
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:248 Resp: 26268
Ion Ratio Lower Upper
248 100
250 95.8 76.2 114.4
141 53.3 45.6 68.4



#22
Hexachlorobenzene
Concen: 0.38 ng
RT: 16.336 min Scan# 1347
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:284 Resp: 30337
Ion Ratio Lower Upper
284 100
142 32.3 25.8 38.6
249 28.8 23.3 34.9







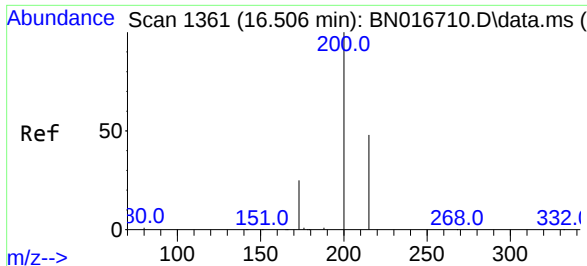

#23
Atrazine
Concen: 0.34 ng
RT: 16.506 min Scan# 1361
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:200 Resp: 19013
Ion Ratio Lower Upper
200 100
173 24.0 20.1 30.1
215 48.8 38.8 58.2

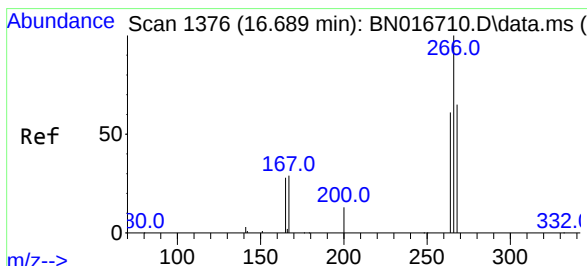

#24
Pentachlorophenol
Concen: 0.55 ng
RT: 16.689 min Scan# 1376
Delta R.T. -0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:266 Resp: 8231
Ion Ratio Lower Upper
266 100
264 62.5 49.3 73.9
268 64.1 51.8 77.8









#25
Phenanthrene
Concen: 0.38 ng
RT: 17.066 min Scan# 1407
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:178 Resp: 129125
Ion Ratio Lower Upper
178 100
176 18.9 15.0 22.6
179 15.5 12.4 18.6



#26
Anthracene
Concen: 0.36 ng
RT: 17.164 min Scan# 1415
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:178 Resp: 111018
Ion Ratio Lower Upper
178 100
176 18.2 14.5 21.7
179 15.3 12.2 18.4









#27
Fluoranthene-d10
Concen: 0.37 ng
RT: 19.068 min Scan# 1697
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 118452
Ion Ratio Lower Upper
212 100
106 13.4 10.6 16.0
104 7.3 5.8 8.8



#28
Fluoranthene
Concen: 0.39 ng
RT: 19.098 min Scan# 1703
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:202 Resp: 146341
Ion Ratio Lower Upper
202 100
101 11.2 8.9 13.3
203 17.3 13.8 20.8









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.238 min Scan# 2002
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:240 Resp: 115135
Ion Ratio Lower Upper
240 100
120 7.7 6.6 10.0
236 25.7 20.7 31.1



#30
Pyrene
Concen: 0.39 ng
RT: 19.465 min Scan# 1777
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:202 Resp: 146985
Ion Ratio Lower Upper
202 100
200 20.6 16.5 24.7
203 17.5 13.9 20.9









#31
Terphenyl-d14
Concen: 0.39 ng
RT: 19.683 min Scan# 1821
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:244 Resp: 99887
Ion Ratio Lower Upper
244 100
212 7.0 5.8 8.6
122 10.7 8.9 13.3



#32
Benzo(a)anthracene
Concen: 0.39 ng
RT: 21.217 min Scan# 2000
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:228 Resp: 139389
Ion Ratio Lower Upper
228 100
226 27.6 22.3 33.5
229 19.1 15.4 23.0









#33
Chrysene
Concen: 0.40 ng
RT: 21.270 min Scan# 2005
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:228 Resp: 146208
Ion Ratio Lower Upper
228 100
226 30.2 24.2 36.4
229 19.4 15.4 23.0



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.32 ng
RT: 21.174 min Scan# 1996
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12


Tgt Ion:149 Resp: 68331
Ion Ratio Lower Upper
149 100
167 27.6 22.2 33.4
279 4.2 3.4 5.2







#35
Perylene-d12
Concen: 0.40 ng
RT: 23.495 min Scan# 2430
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC





Tgt Ion:264 Resp: 121122
Ion Ratio Lower Upper
264 100
260 24.3 19.8 29.6
265 23.5 20.3 30.5




#36
Indeno(1,2,3-cd)pyrene
Concen: 0.45 ng
RT: 25.774 min Scan# 3096
Delta R.T. -0.007 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12



Tgt Ion:276 Resp: 174036
Ion Ratio Lower Upper
276 100
138 25.2 19.2 28.8
277 25.1 20.0 30.0









#37
Benzo(b)fluoranthene
Concen: 0.39 ng
RT: 22.814 min Scan# 2231
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:252 Resp: 152224
Ion Ratio Lower Upper
252 100
253 22.2 17.8 26.8
125 10.1 8.3 12.5



#38
Benzo(k)fluoranthene
Concen: 0.40 ng
RT: 22.858 min Scan# 2244
Delta R.T. -0.003 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:252 Resp: 151102
Ion Ratio Lower Upper
252 100
253 22.3 17.8 26.8
125 12.4 8.5 12.7









#39
Benzo(a)pyrene
Concen: 0.40 ng
RT: 23.392 min Scan# 2400
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:252 Resp: 138785
Ion Ratio Lower Upper
252 100
253 22.4 17.9 26.9
125 11.2 9.4 14.2



#40
Dibenzo(a,h)anthracene
Concen: 0.46 ng
RT: 25.798 min Scan# 3103
Delta R.T. 0.000 min
Lab File: BN016723.D
Acq: 04 Oct 2021 23:12

Tgt Ion:278 Resp: 139294
Ion Ratio Lower Upper
278 100
139 17.7 13.1 19.7
279 23.8 19.3 28.9





#41
 Benzo(g,h,i)perylene
 Concen: 0.44 ng
 RT: 26.473 min Scan# 3300
 Delta R.T. -0.003 min
 Lab File: BN016723.D
 Acq: 04 Oct 2021 23:12

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:276 Resp: 151830
 Ion Ratio Lower Upper
 276 100
 277 23.7 19.0 28.4
 138 20.7 17.0 25.6

