
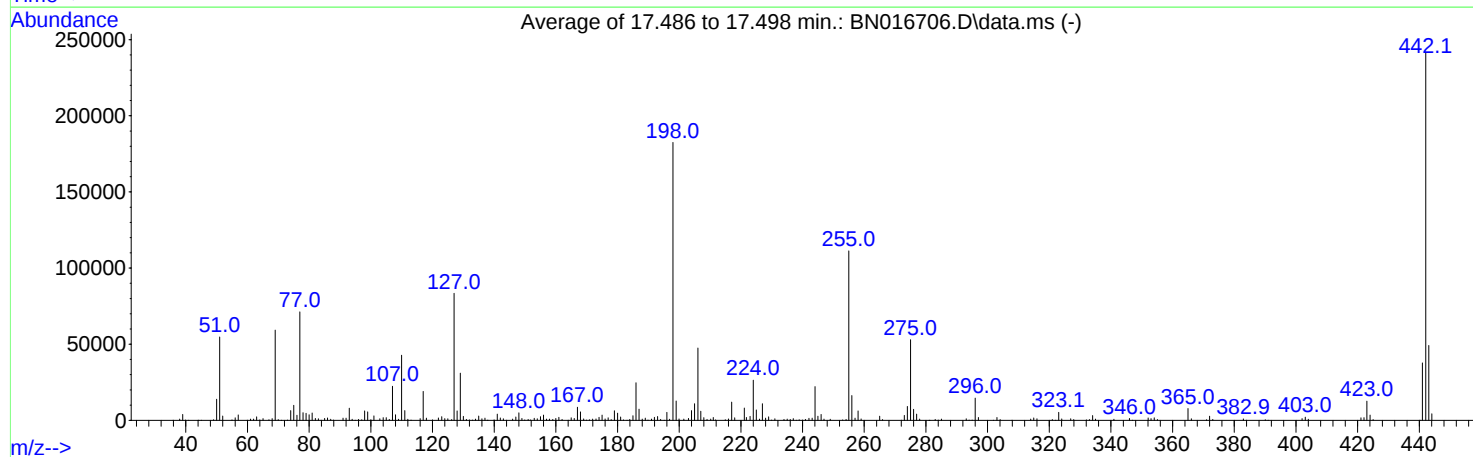


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
 Data File : BN016706.D
 Acq On : 04 Oct 2021 12:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 04 17:52:33 2021

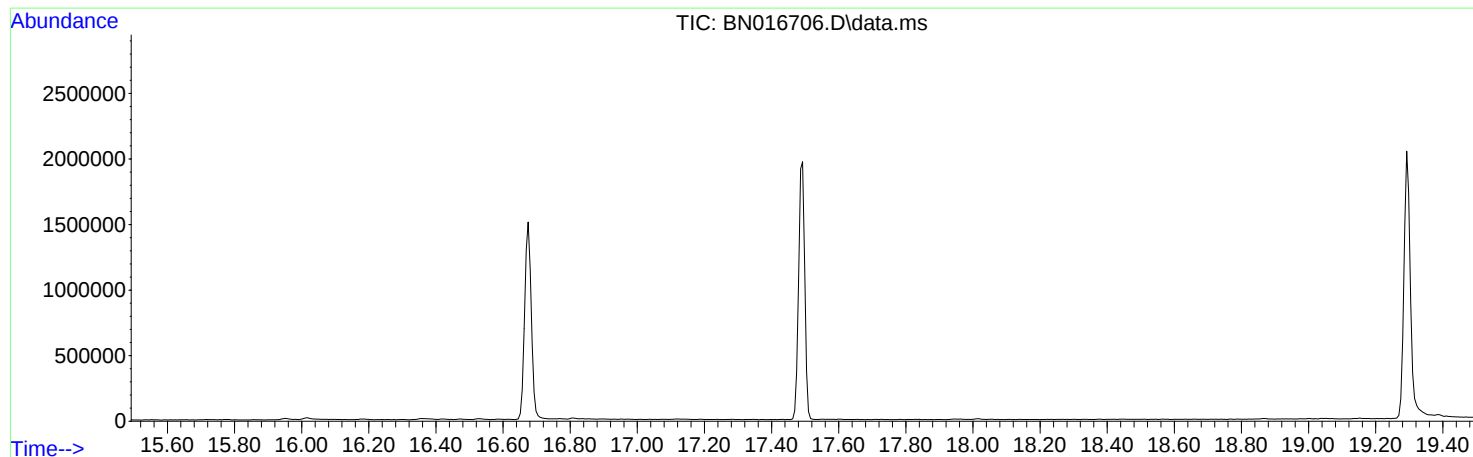




AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	54701	PASS
68	69	0.00	2	2.0	1160	PASS
69	198	0.00	100	32.5	59284	PASS
70	69	0.00	2	0.9	521	PASS
127	198	10	80	45.7	83411	PASS
197	198	0.00	2	0.4	753	PASS
198	198	100	100	100.0	182461	PASS
199	198	5	9	7.0	12743	PASS
275	198	10	60	29.0	52915	PASS
365	198	1	100	4.3	7809	PASS
441	198	0.01	100	20.7	37763	PASS
442	442	50	100	100.0	241557	PASS
443	442	15	24	20.3	49149	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016706.D
Acq On : 04 Oct 2021 12:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 04 14:31:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

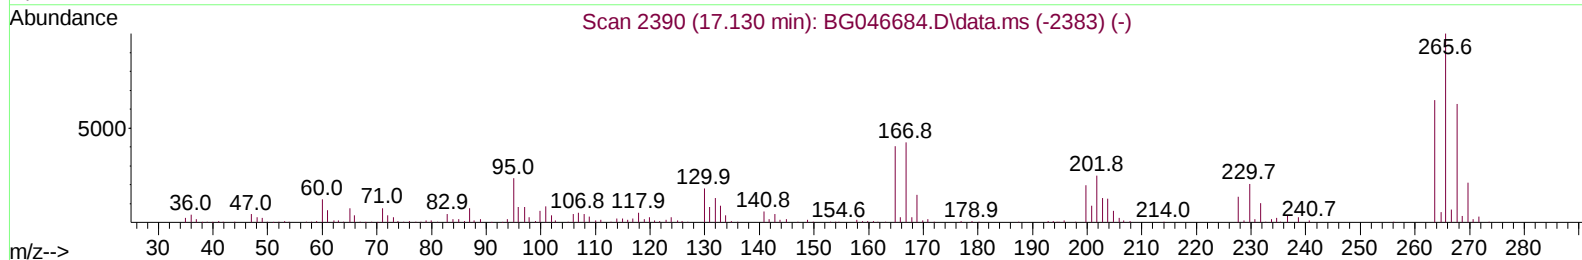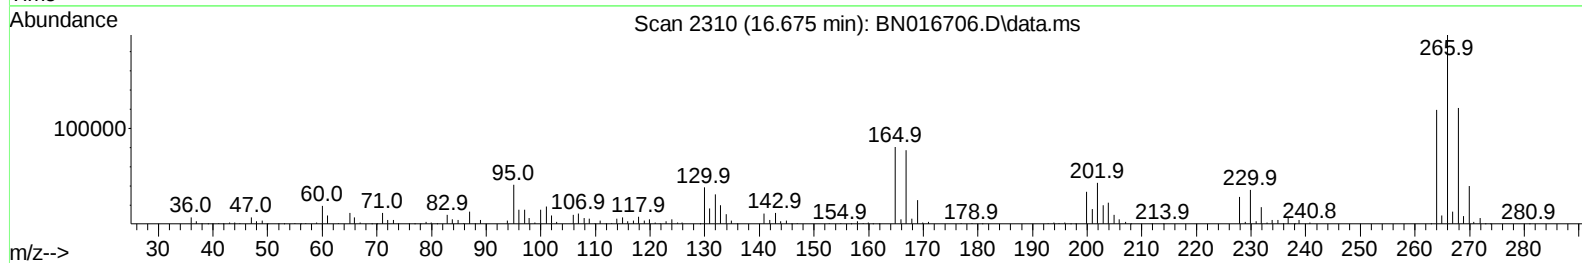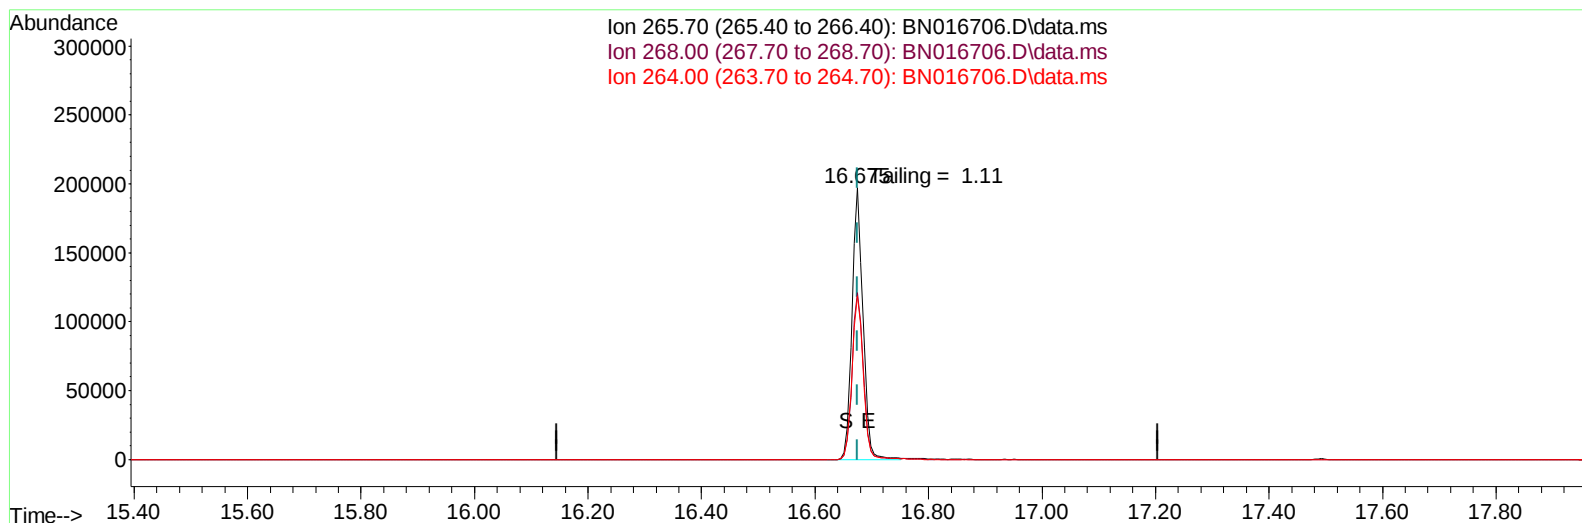

TIC: BN016706.D\data.ms

(70) Pentachlorophenol (C)

16.675min (+ 0.000) 31125.43 ng




response 265027

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.38
264.00	61.60	60.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016706.D
Acq On : 04 Oct 2021 12:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 04 14:31:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

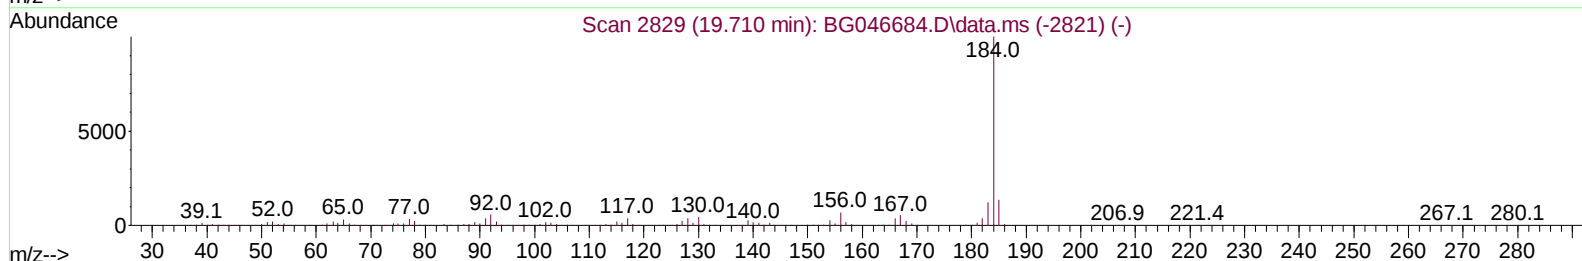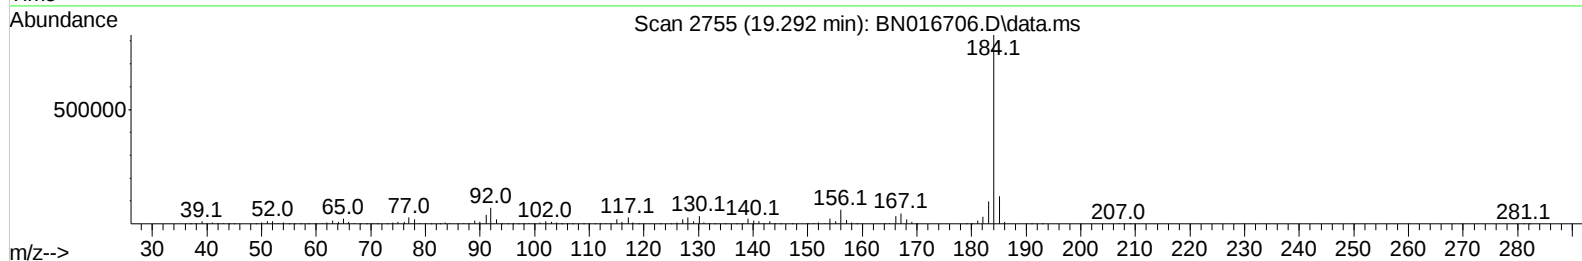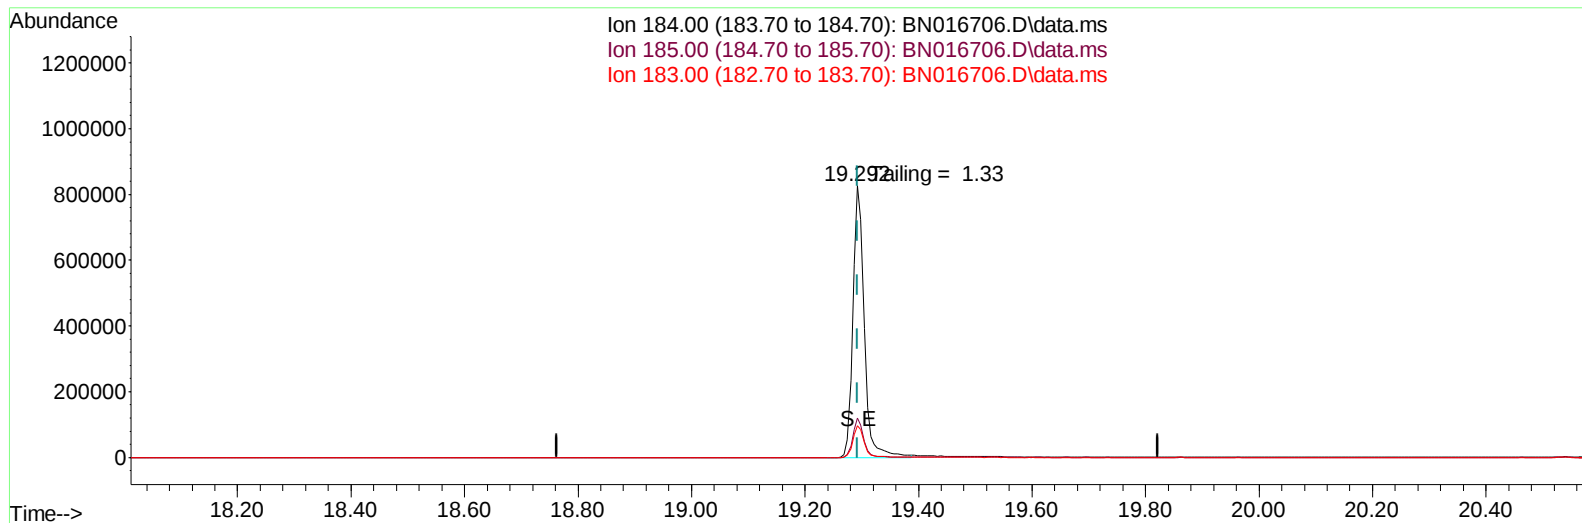

TIC: BN016706.D\data.ms

(77) Benzidine

19.292min (+ 0.000) 0.00 ng

response 1172195

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.48
183.00	13.20	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/4/2021	BNA_N	<u>BN016706.D</u>
Compound Name	Response	Retention Time
DDT	681349	20.539
DDD	8225	20.098
DDE	680	19.586
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8905	690254	1.29