
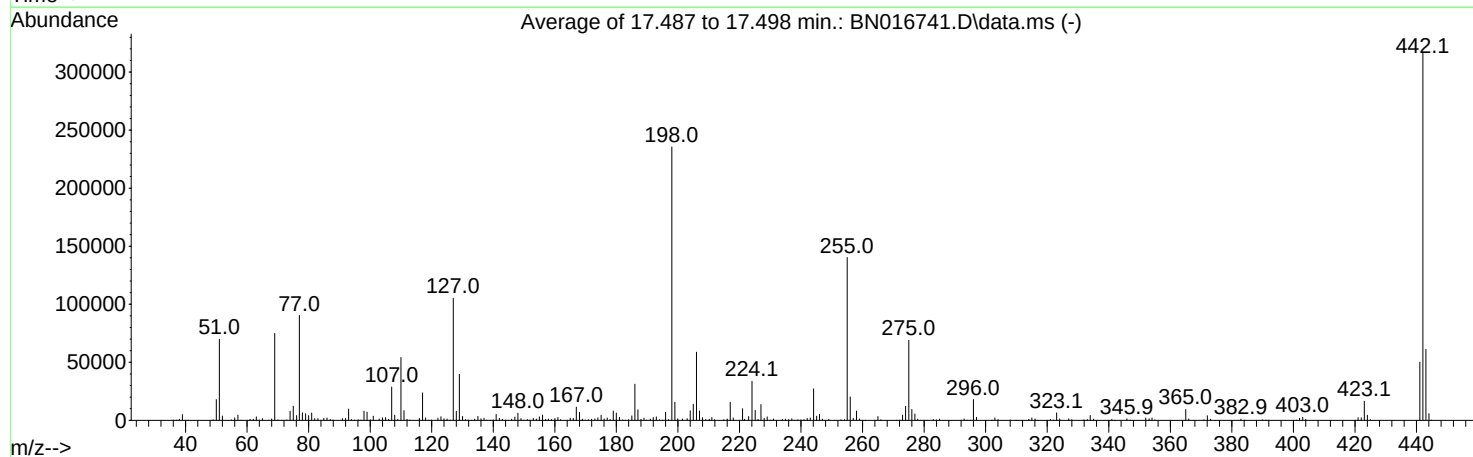


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
 Data File : BN016741.D
 Acq On : 05 Oct 2021 11:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 04 17:52:33 2021

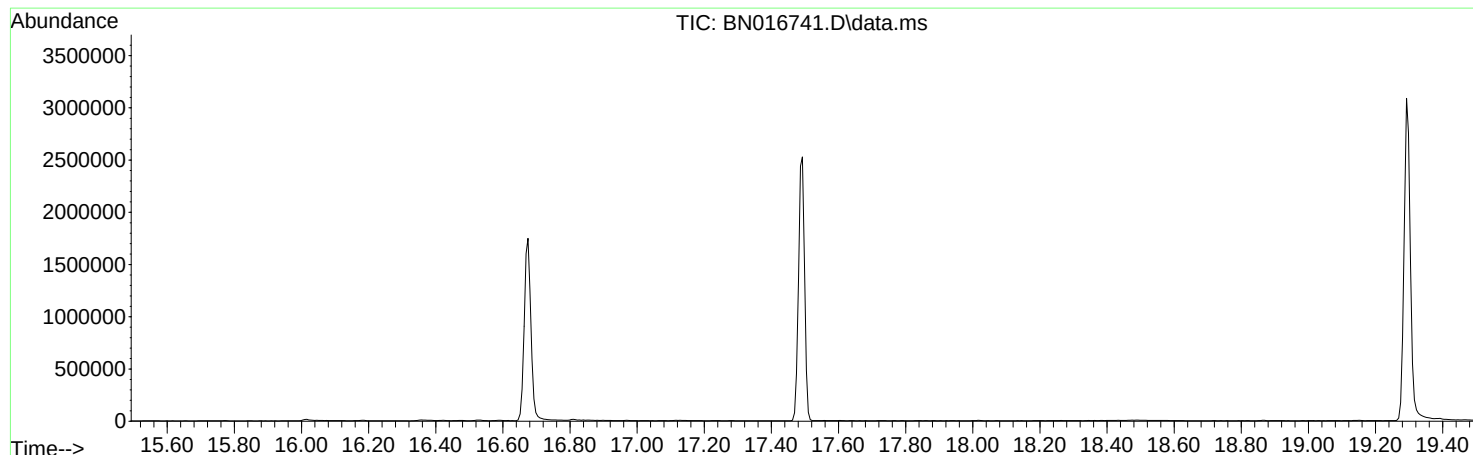

AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	69893	PASS
68	69	0.00	2	1.7	1277	PASS
69	198	0.00	100	31.8	74819	PASS
70	69	0.00	2	0.5	365	PASS
127	198	10	80	44.7	105227	PASS
197	198	0.00	2	0.3	729	PASS
198	198	100	100	100.0	235584	PASS
199	198	5	9	6.7	15701	PASS
275	198	10	60	29.3	68936	PASS
365	198	1	100	4.0	9408	PASS
441	198	0.01	100	21.3	50205	PASS
442	442	50	100	100.0	316885	PASS
443	442	15	24	19.3	61275	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/4/2021	BNA_N	<u>BN016741.D</u>
Compound Name	Response	Retention Time
DDT	861320	20.53
DDD	10735	20.09
DDE	0	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10735	872055	1.23

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016741.D
Acq On : 05 Oct 2021 11:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 05 11:58:05 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

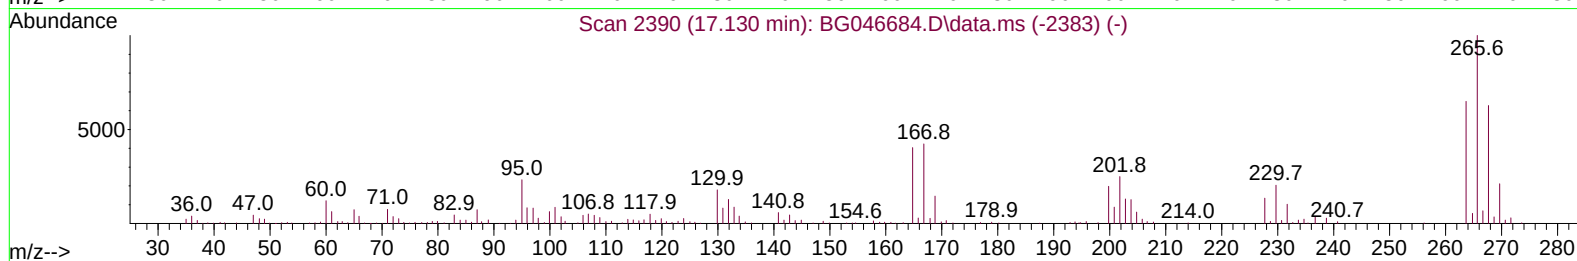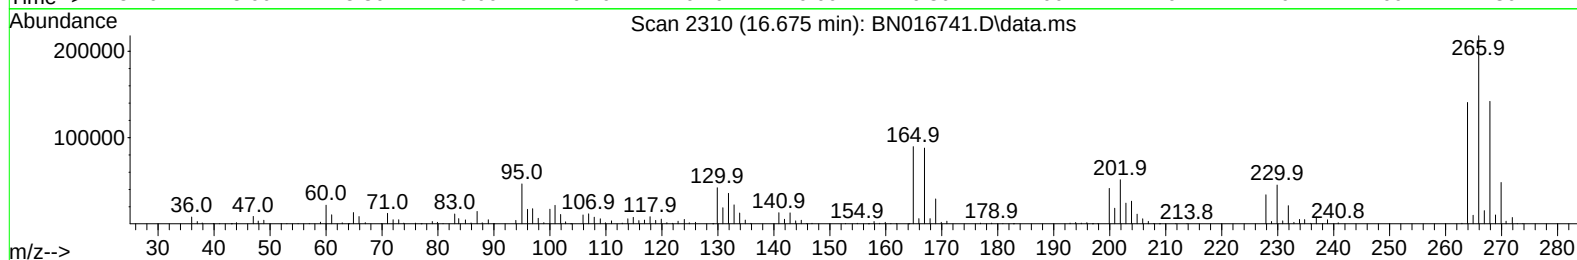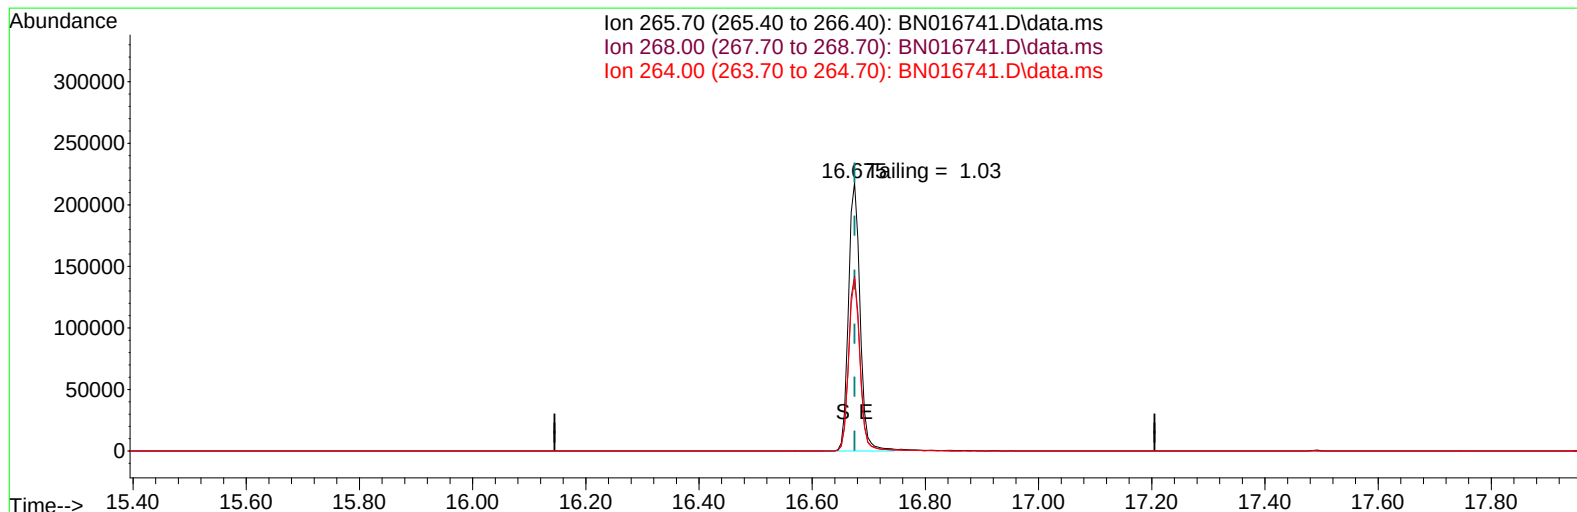

TIC: BN016741.D\data.ms

(70) Pentachlorophenol (C)

16.675min (+ 0.000) 30955.19 ng




response 312649

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.13
264.00	61.60	64.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016741.D
Acq On : 05 Oct 2021 11:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 05 11:58:05 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

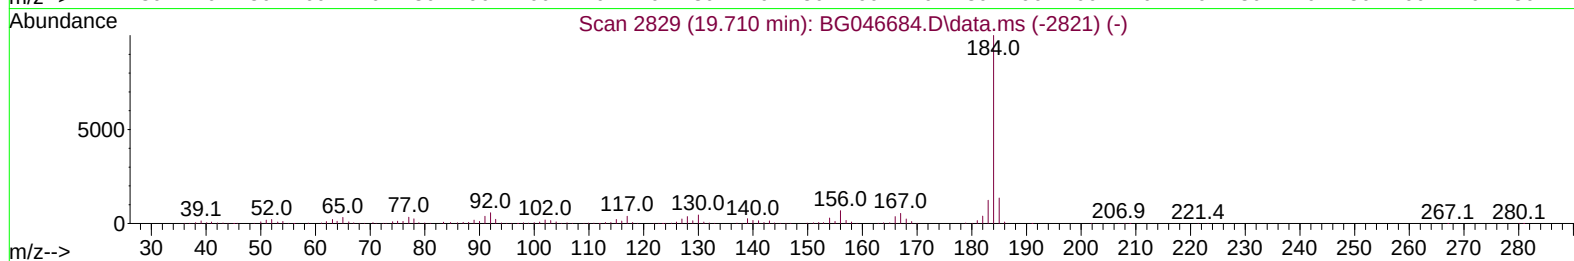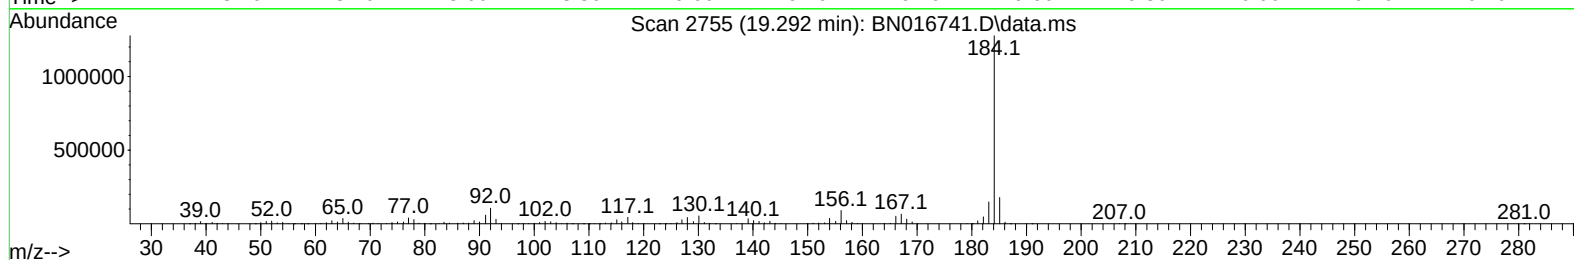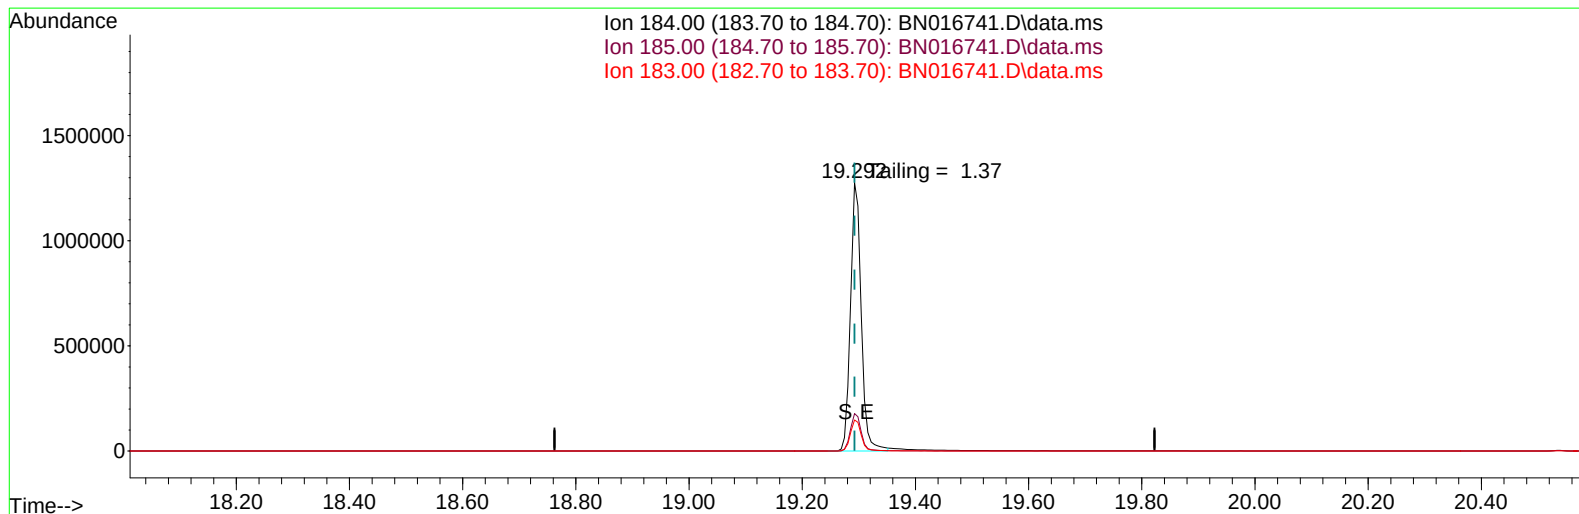

TIC: BN016741.D\data.ms

(77) Benzidine

19.292min (+ 0.000) 0.00 ng

response 1721522

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.99
183.00	13.20	11.61
0.00	0.00	0.00