
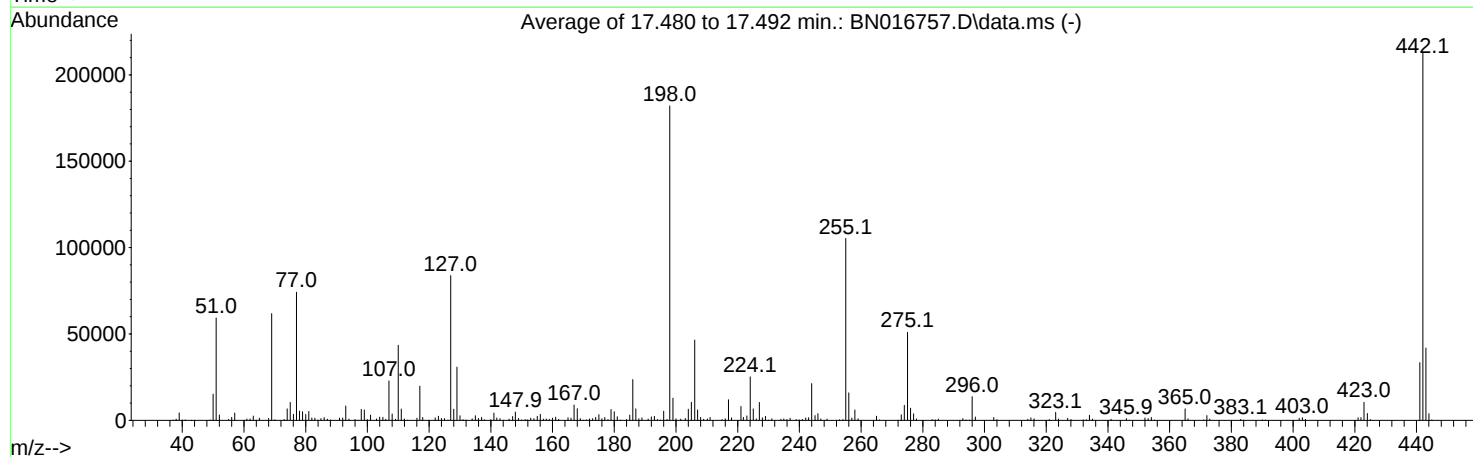


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
 Data File : BN016757.D
 Acq On : 06 Oct 2021 00:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 04 17:52:33 2021

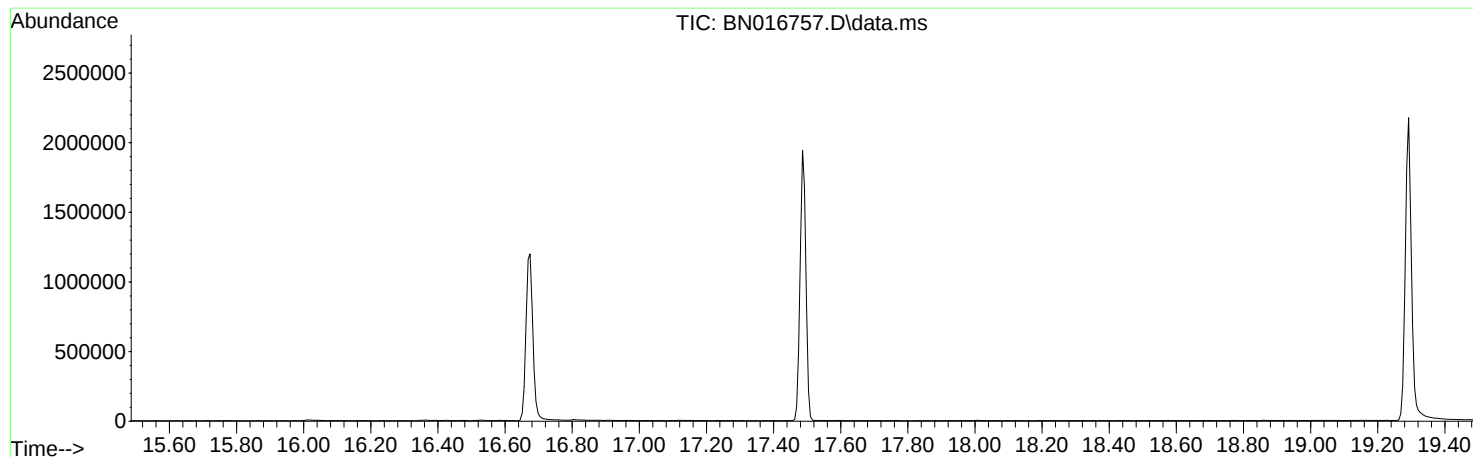

AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	59248	PASS
68	69	0.00	2	1.9	1152	PASS
69	198	0.00	100	33.9	61763	PASS
70	69	0.00	2	0.7	412	PASS
127	198	10	80	46.1	83853	PASS
197	198	0.00	2	0.3	604	PASS
198	198	100	100	100.0	182016	PASS
199	198	5	9	7.1	12914	PASS
275	198	10	60	28.0	50965	PASS
365	198	1	100	3.6	6638	PASS
441	198	0.01	100	18.4	33429	PASS
442	442	50	100	100.0	212936	PASS
443	442	15	24	19.7	41864	PASS

Instrument :
BNA_N
ClientSampleId :
DFTPP

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/4/2021	BNA_N	<u>BN016757.D</u>
Compound Name	Response	Retention Time
DDT	605303	20.533
DDD	27653	20.098
DDE	0	19.581
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27653	632956	4.37

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016757.D
Acq On : 06 Oct 2021 00:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 06 04:41:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

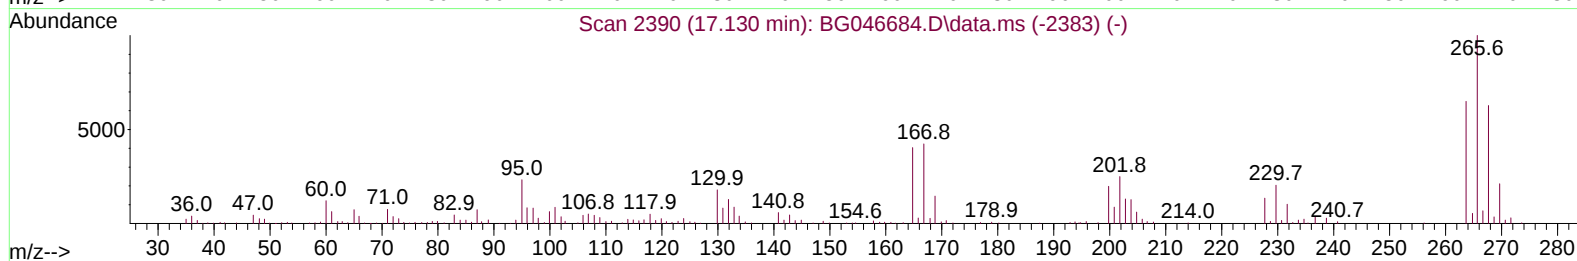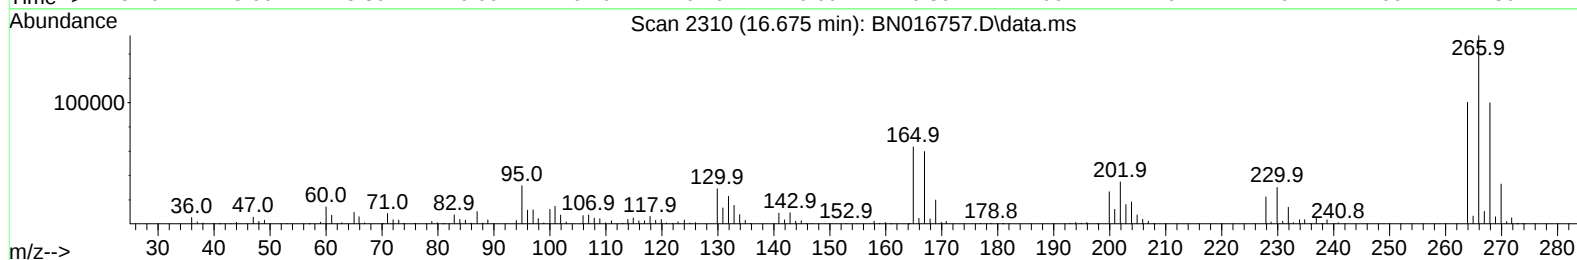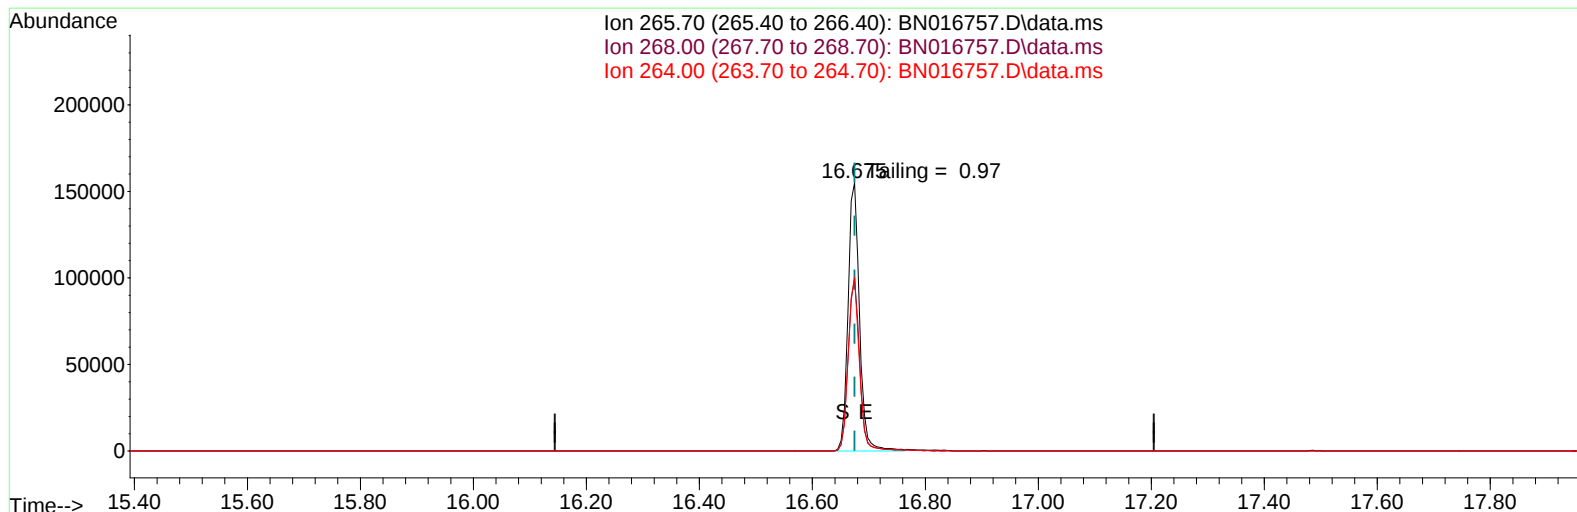

TIC: BN016757.D\data.ms

(70) Pentachlorophenol (C)

16.675min (-0.000) 22795.26 ng




response 220931

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.40
264.00	61.60	64.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016757.D
Acq On : 06 Oct 2021 00:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 06 04:41:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

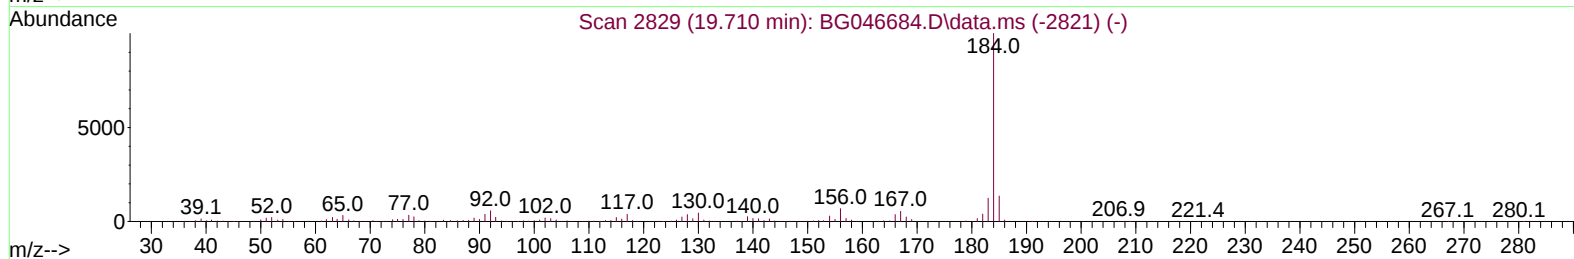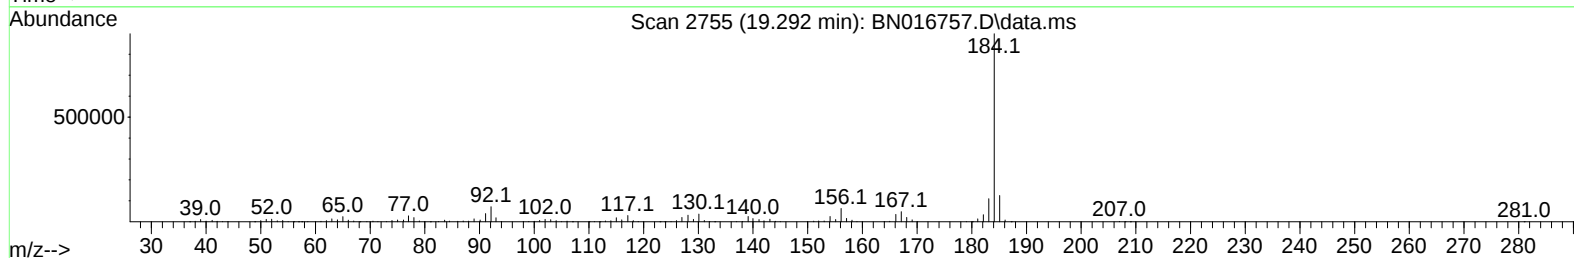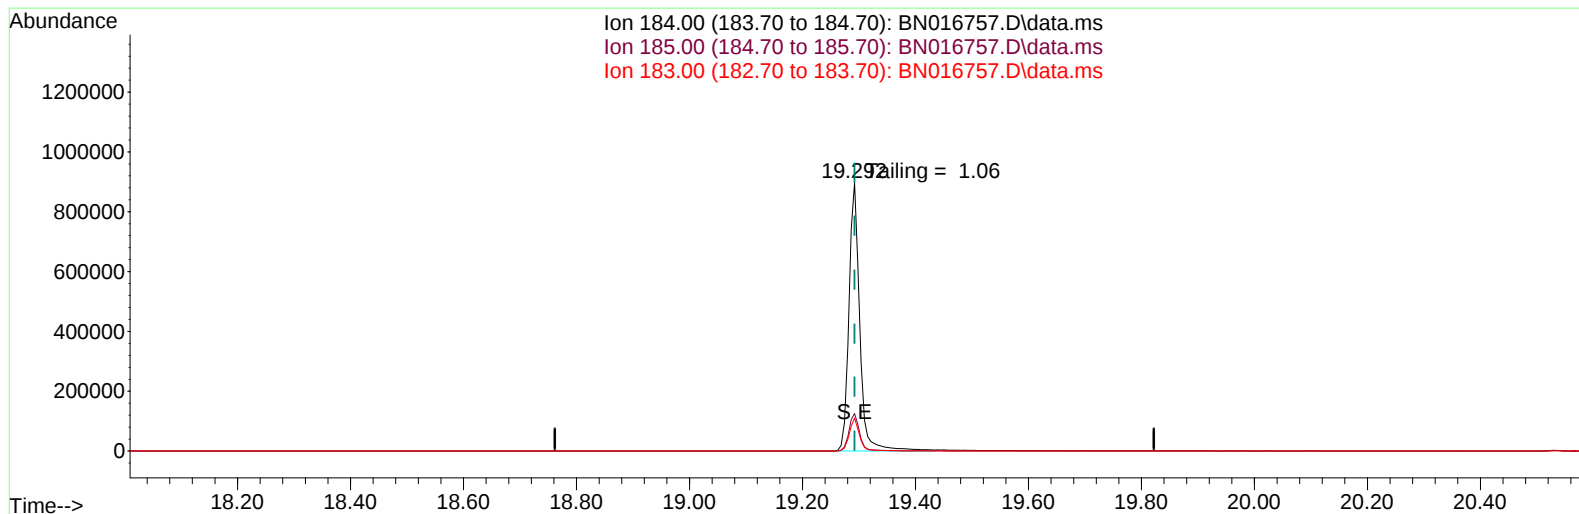

TIC: BN016757.D\data.ms

(77) Benzidine

19.292min (-0.000) 0.00 ng

response 1203109

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.99
183.00	13.20	12.28
0.00	0.00	0.00