

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100518\
 Data File : BN002929.D
 Acq On : 04 Oct 2018 13:09
 Operator : MJ/SJ
 Sample : J5183-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 05 02:01:36 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 05 02:00:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	123883	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	562270	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	340235	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	780558	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	735076	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	597204	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	8995	3.35	ng/uL	0.00
5) Phenol-d5	6.82	99	208175	19.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	135899	20.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	176257	20.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	172493	21.17	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	87871	20.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	101324	20.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	172249	19.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	245040	23.80	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	614780	23.08	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	752657	21.64	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	75599	17.17	ng/ul	0.00
57) Fluorene-d10	15.26	176	542825	23.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.41	200	81617	16.72	ng/ul	0.00
70) Anthracene-d10	17.11	188	852739	22.88	ng/ul	0.00
78) Pyrene-d10	19.42	212	914709	23.58	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	725452	23.08	ng/ul	0.00


Target Compounds				Ovalue		
6) Phenol	6.84	94	21915	2.066	ng/ul#	87
44) Dimethylphthalate	13.72	163	319169	12.279	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100518\
Data File : BN002929.D
Acq On : 04 Oct 2018 13:09
Operator : MJ/SJ
Sample : J5183-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 05 02:01:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 05 02:00:32 2018
Response via : Initial Calibration

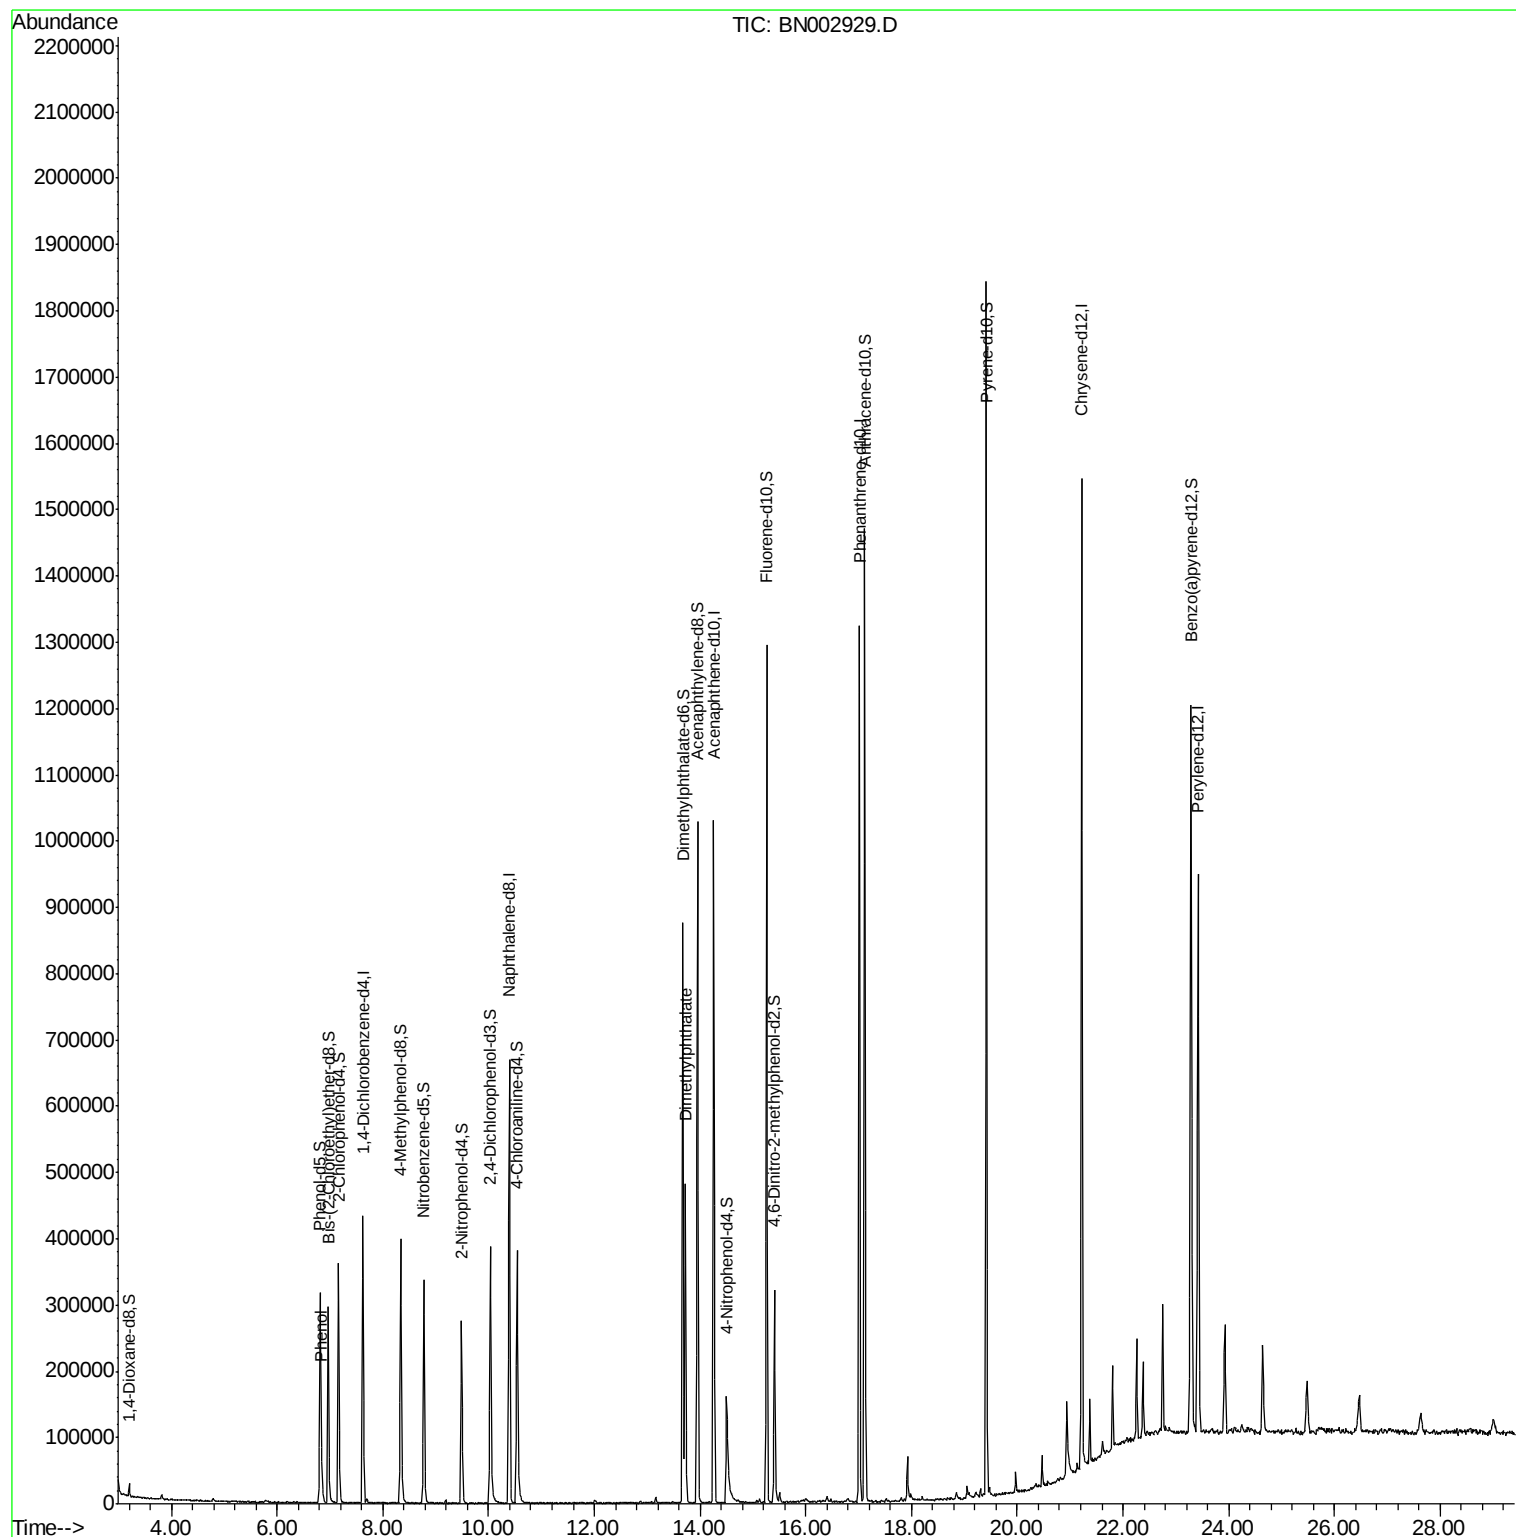

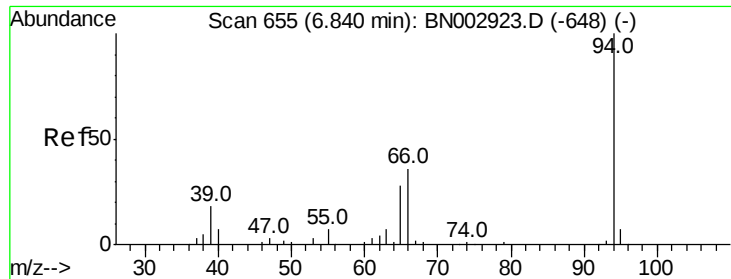

#6

Phenol

Concen: 2.066 ng/ul

RT: 6.84 min Scan# 655

Delta R.T. -0.00 min

Lab File: BN002929.D

Acq: 04 Oct 2018 13:09

Instrument :

BNA_N

ClientSampled :


Tot Ion: 94 Resp: 21915

Ion Ratio Lower Upper

94 100

65 32.0 23.1 34.7




66 48.6 29.8 44.6#

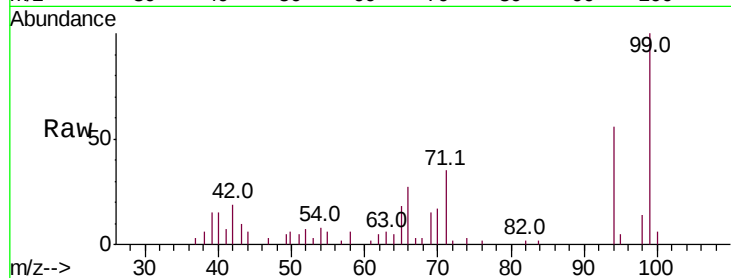

Abundance Ion 94.00 (93.70 to 94.70): BN002923.D (-648) (-)

Ion 65.00 (64.70 to 65.70): BN002923.D (-648) (-)

Ion 66.00 (65.70 to 66.70): BN002923.D (-648) (-)

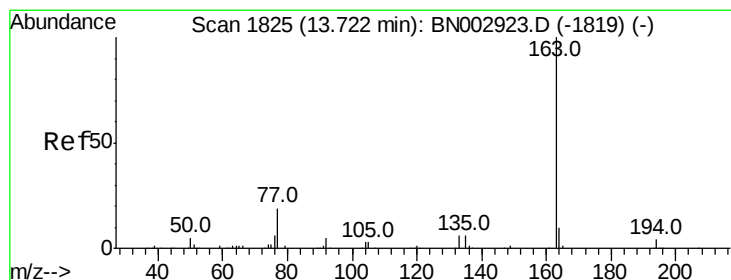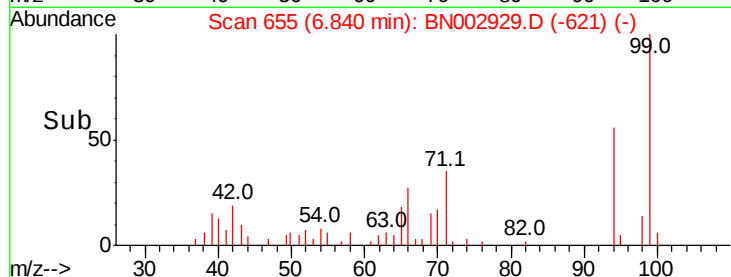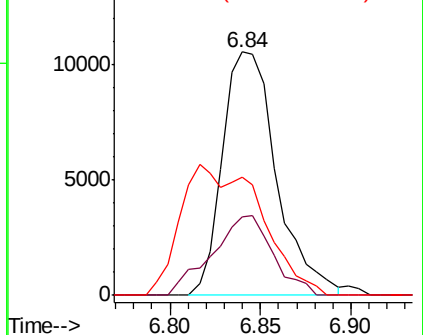

#44

Dimethylphthalate

Concen: 12.279 ng/ul

RT: 13.72 min Scan# 1825

Delta R.T. -0.00 min

Lab File: BN002929.D

Acq: 04 Oct 2018 13:09


Tgt Ion:163 Resp: 319169

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 10.3 8.1 12.1

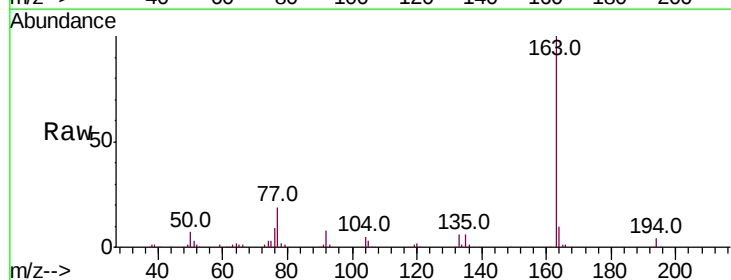

Abundance Ion 163.00 (162.70 to 163.70): BN002923.D (-1819) (-)

Ion 194.00 (193.70 to 194.70): BN002923.D (-1819) (-)

Ion 164.00 (163.70 to 164.70): BN002923.D (-1819) (-)

