

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100518\
 Data File : BN002939.D
 Acq On : 04 Oct 2018 19:01
 Operator : MJ/SJ
 Sample : J5184-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 05 02:27:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 05 02:27:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	130991	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	610048	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	375832	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	820739	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	727484	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	610140	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	9599	3.38	ng/uL	0.00
5) Phenol-d5	6.81	99	214042	19.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	141483	20.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	182720	19.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	185245	21.50	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	94134	19.92	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	109958	20.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	185987	19.27	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	260077	23.28	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	681985	23.18	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	849960	22.13	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	80771	16.60	ng/ul	0.00
57) Fluorene-d10	15.26	176	602013	23.36	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	91960	17.91	ng/ul	0.00
70) Anthracene-d10	17.11	188	909457	23.21	ng/ul	0.00
78) Pyrene-d10	19.42	212	934528	24.34	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	748698	23.31	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.84	94	24776	2.209	ng/ul 95
44) Dimethylphthalate	13.72	163	331285	11.538	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100518\
Data File : BN002939.D
Acq On : 04 Oct 2018 19:01
Operator : MJ/SJ
Sample : J5184-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 05 02:27:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 05 02:27:06 2018
Response via : Initial Calibration

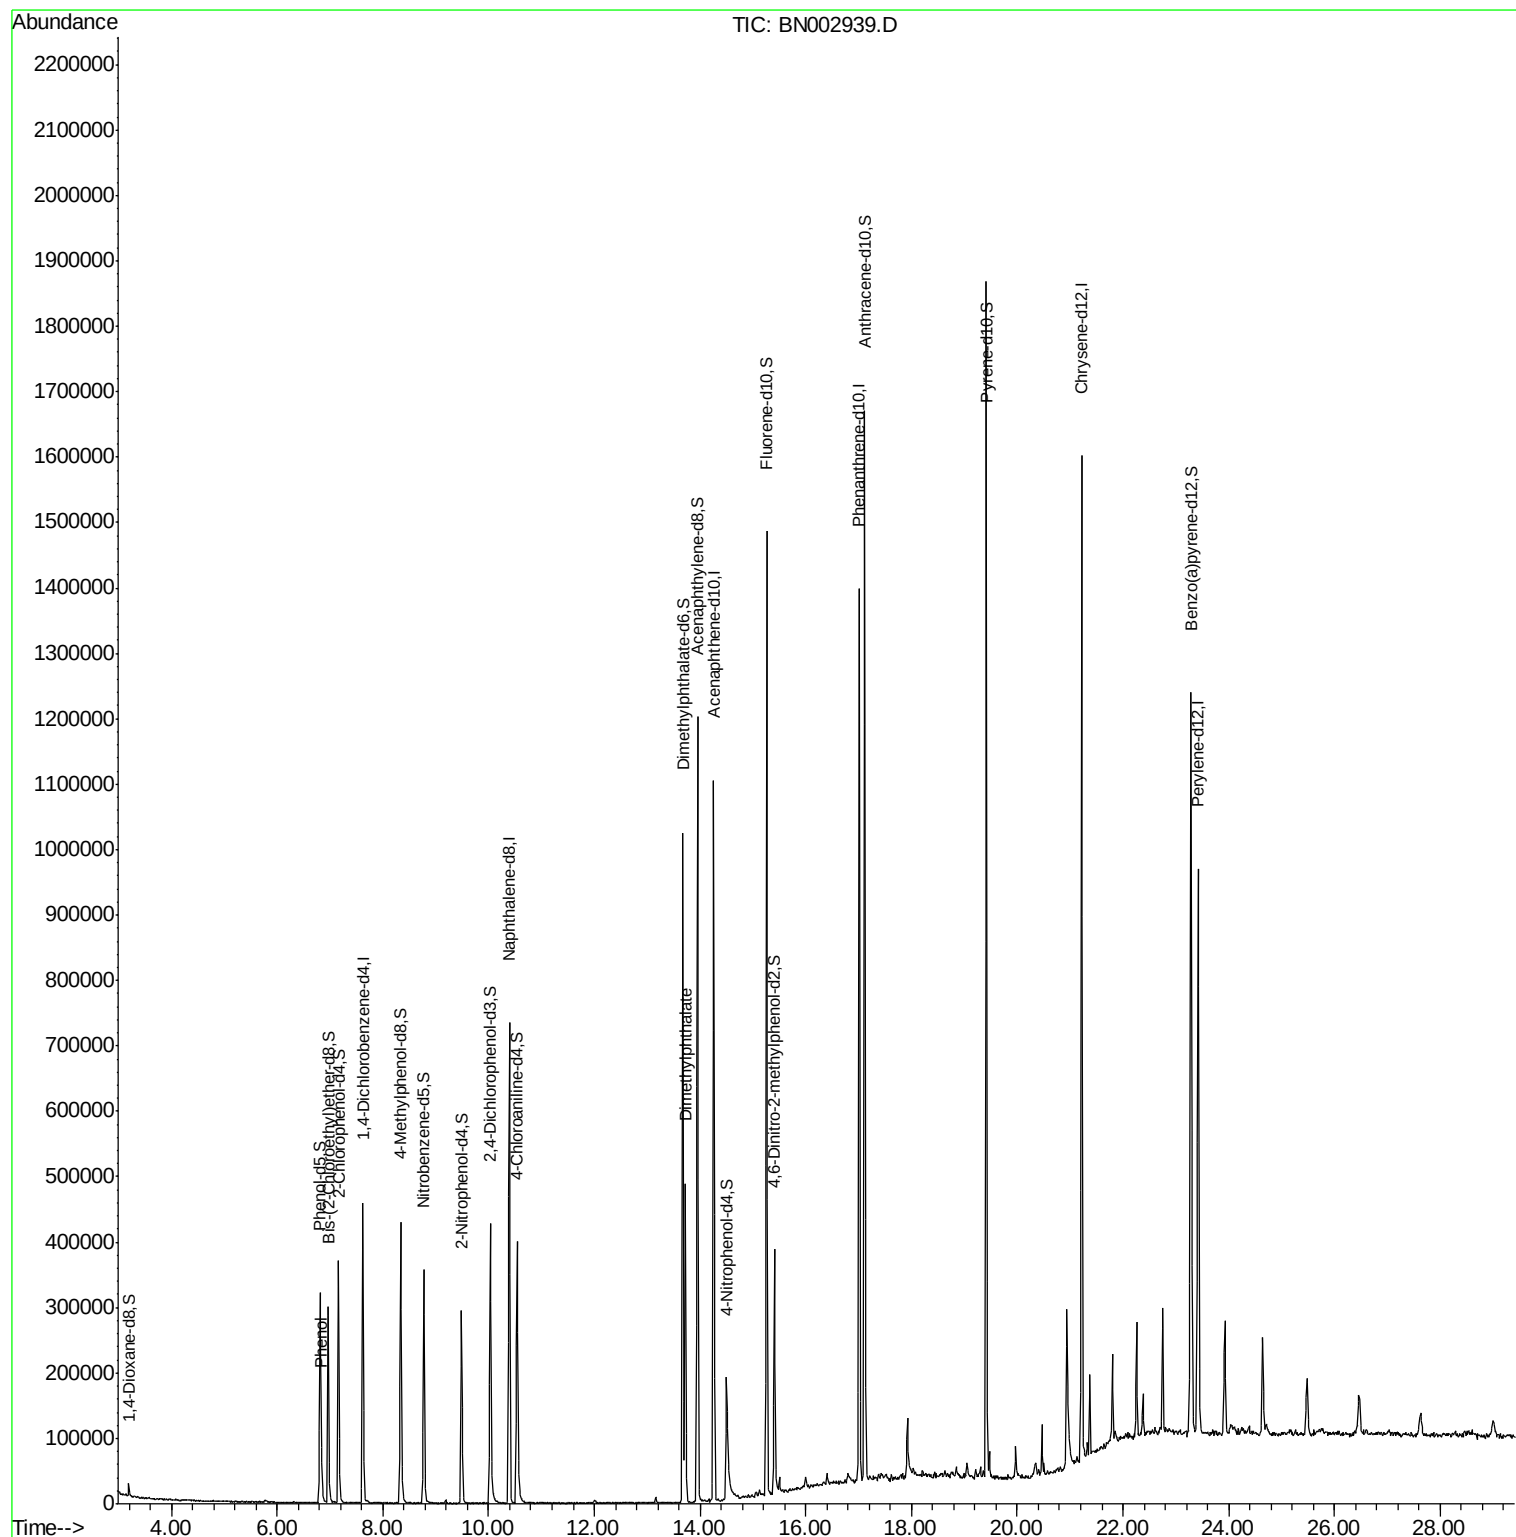

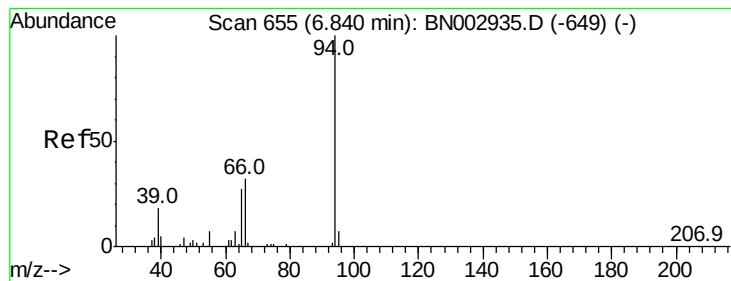

#6

Phenol

Concen: 2.209 ng/ul

RT: 6.84 min Scan# 655

Delta R.T. -0.00 min

Lab File: BN002939.D

Acq: 04 Oct 2018 19:01

Instrument :

BNA_N

ClientSampleId :





Tot Ion: 94 Resp: 24776

Ion Ratio Lower Upper

94 100

65 29.7 23.1 34.7

66 41.9 29.8 44.6

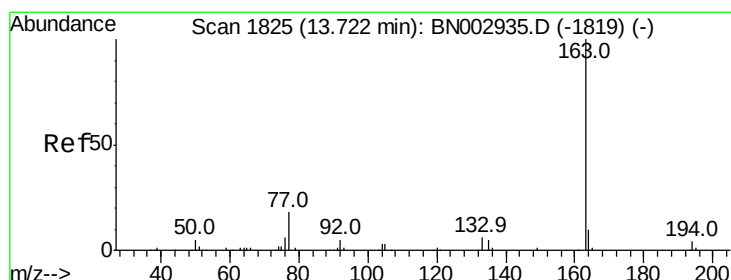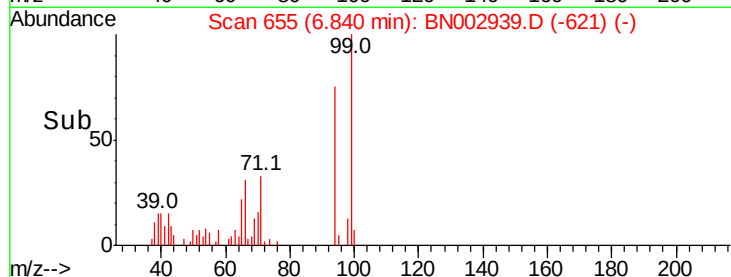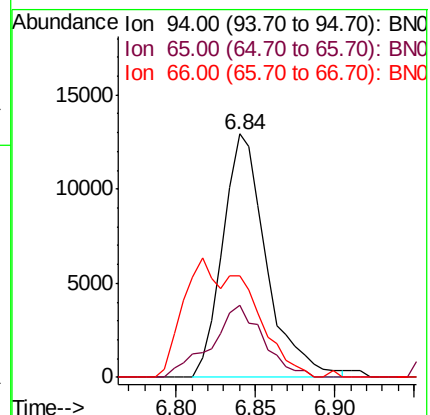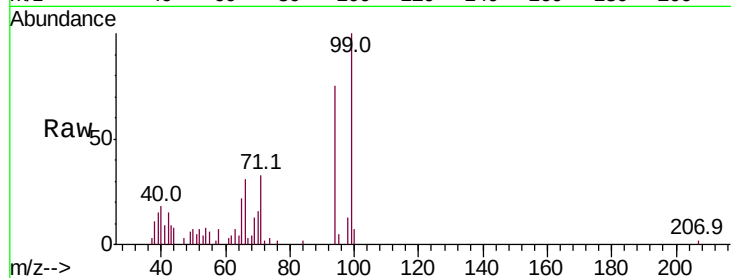

#44

Dimethylphthalate

Concen: 11.538 ng/ul

RT: 13.72 min Scan# 1825

Delta R.T. -0.00 min

Lab File: BN002939.D

Acq: 04 Oct 2018 19:01

Tgt Ion: 163 Resp: 331285

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 10.3 8.1 12.1

