


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100518\
Data File : BN002952.D
Acq On : 05 Oct 2018 03:21
Operator : MJ/SJ
Sample : J5116-04DL 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC55DL

Manual Integrations
APPROVED

Sohil
10/5/2018 5:30:17 PM

Quant Time: Oct 05 07:18:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 05 05:51:15 2018
Response via : Initial Calibration

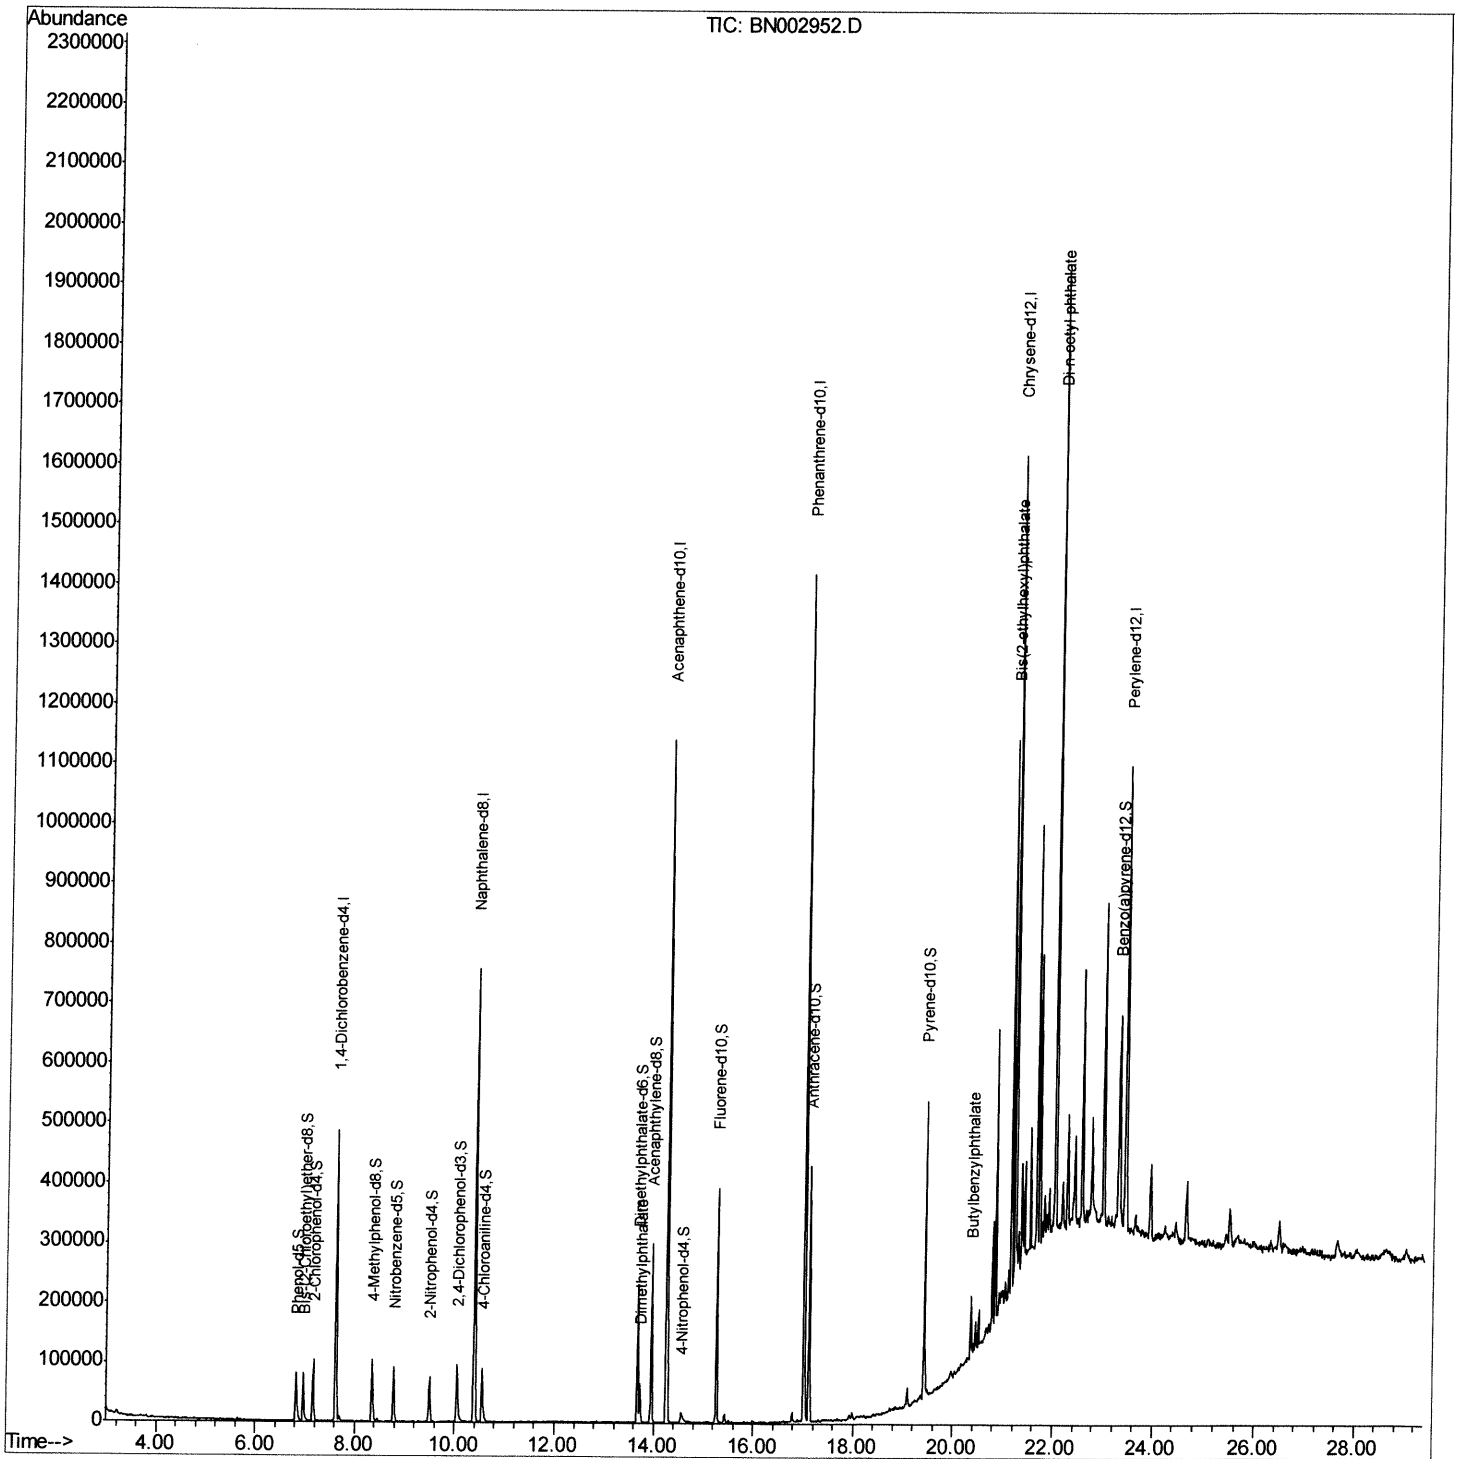

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100518\
Data File : BN002952.D
Acq On : 05 Oct 2018 03:21
Operator : MJ/SJ
Sample : J5116-04DL 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC55DL

Manual Integrations
APPROVED

Sohil
10/5/2018 5:30:17 PM

Quant Time: Oct 05 05:51:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 05 05:51:15 2018
Response via : Initial Calibration

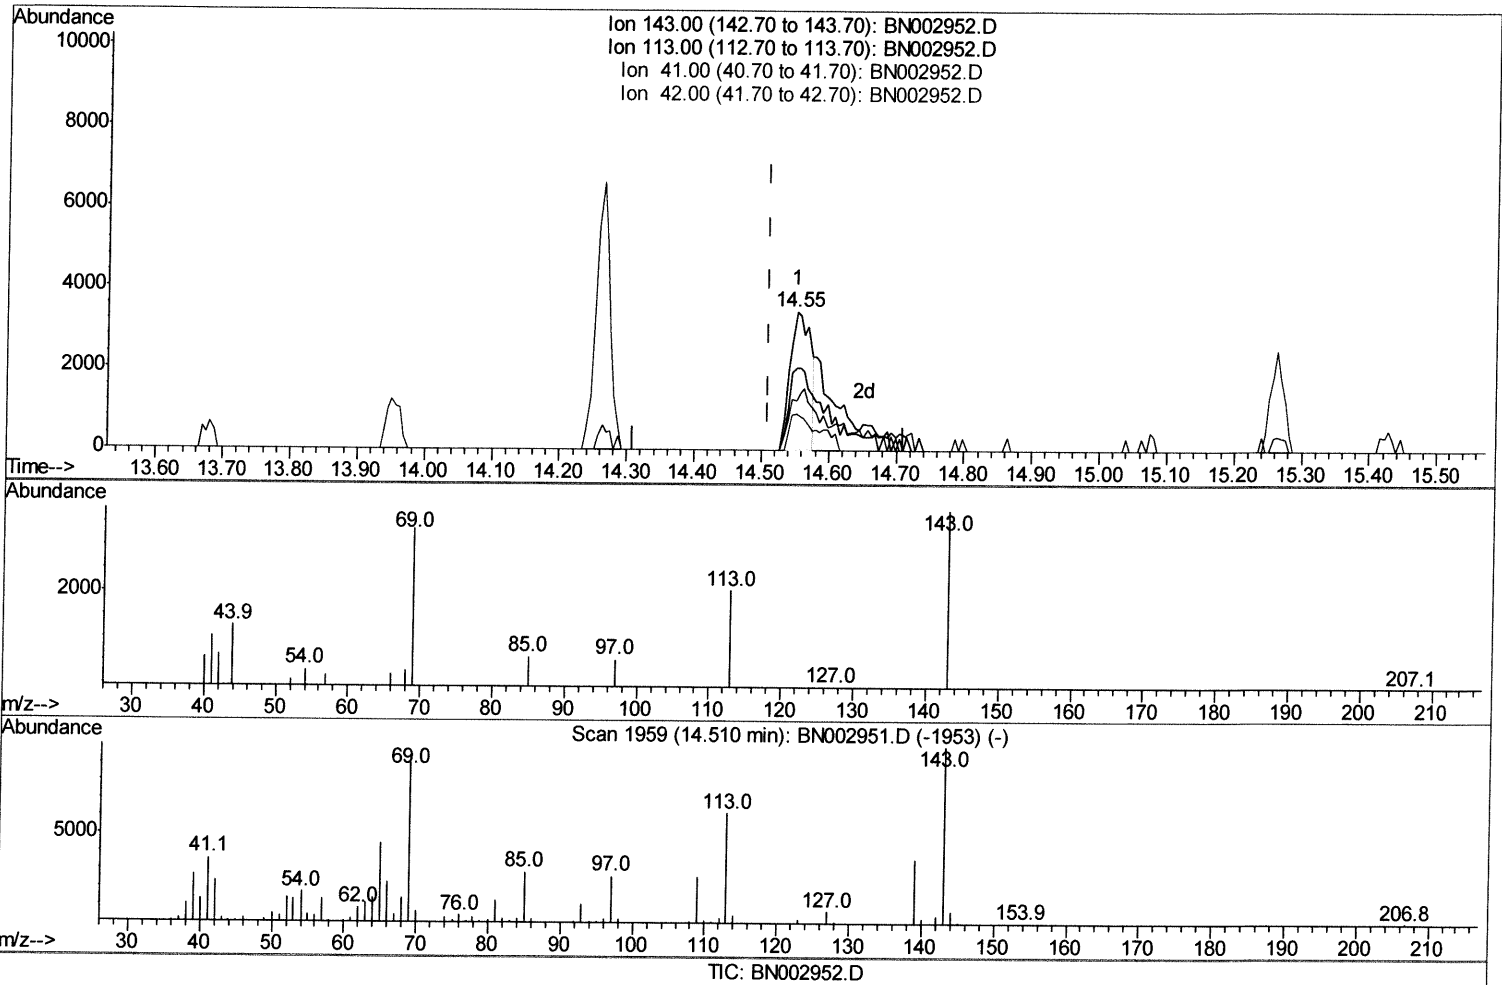

(51) 4-Nitrophenol-d4 (S)

14.551min (+0.041) 1.46ng/ul

response 7175

Ion	Exp%	Act%
143.00	100	100
113.00	66.10	59.54
41.00	39.90	35.67
42.00	25.80	26.42

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100518\
Data File : BN002952.D
Acq On : 05 Oct 2018 03:21
Operator : MJ/SJ
Sample : J5116-04DL 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC55DL

Manual Integrations
APPROVED

Sohil
10/5/2018 5:30:17 PM

Quant Time: Oct 05 05:51:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 05 05:51:15 2018
Response via : Initial Calibration

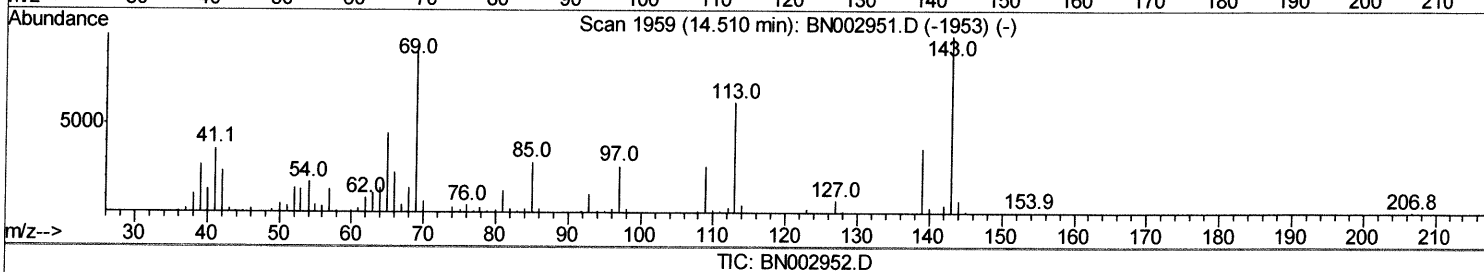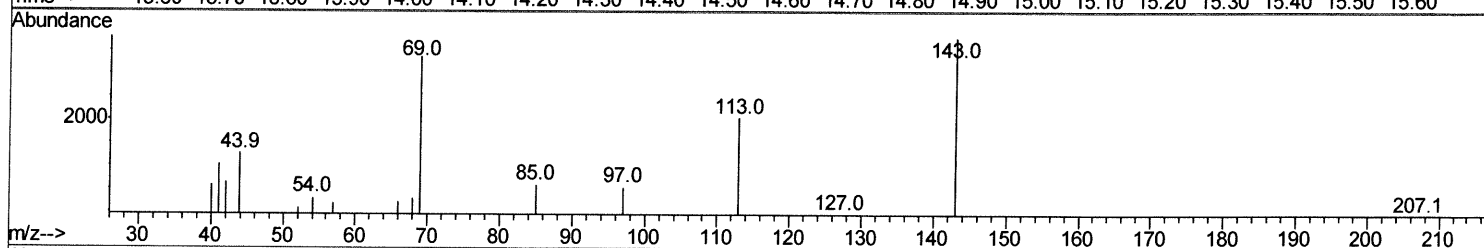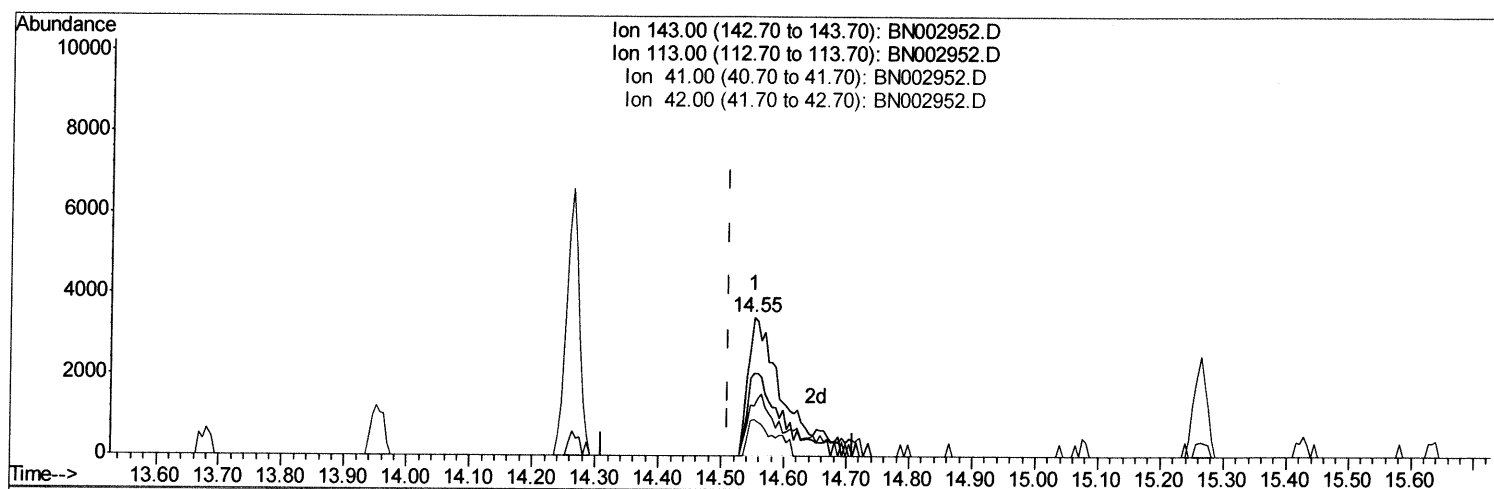

TIC: BN002952.D

(51) 4-Nitrophenol-d4 (S)

14.551min (+0.041) 2.88ng/ul m

SJ 10/10/18

response 14119

Ion	Exp%	Act%
143.00	100	100
113.00	66.10	59.54
41.00	39.90	35.67
42.00	25.80	26.42

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100518\
 Data File : BN002952.D
 Acq On : 05 Oct 2018 03:21
 Operator : MJ/SJ
 Sample : J5116-04DL 5X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleID :
 JLC55DL

Manual Integrations
 APPROVED

Sohil
 10/5/2018 5:30:17 PM

Quant Time: Oct 05 07:18:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 05 05:51:15 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	138176	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	636173	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	378555	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	838715	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	622246	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	538280	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	2877	0.96	ng/uL	0.00
5) Phenol-d5	6.82	99	62869	5.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	41525	5.70	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	55328	5.73	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	49779	5.48	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	26314	5.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	29494	5.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	51866	5.15	ng/ul	0.01
29) 4-Chloroaniline-d4	10.55	131	67301	5.78	ng/ul	0.01
43) Dimethylphthalate-d6	13.67	166	173420	5.85	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	227258	5.87	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	14119m	2.88	ng/ul	0.04
57) Fluorene-d10	15.26	176	164770	6.35	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	5212	0.99	ng/ul	0.02
70) Anthracene-d10	17.12	188	241875	6.04	ng/ul	0.00
78) Pyrene-d10	19.42	212	244634	7.45	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	178797	6.31	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	13.73	163	47193	1.632	ng/ul	99
80) Butylbenzylphthalate	20.36	149	33560	1.960	ng/ul	98
83) Bis(2-ethylhexyl)phthalate	21.16	149	581421	23.393	ng/ul#	55
86) Di-n-octyl phthalate	22.02	149	1066876	29.986	ng/ul	99

5/10/10/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed