

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100518\
 Data File : BN002934.D
 Acq On : 04 Oct 2018 16:06
 Operator : MJ/SJ
 Sample : J5184-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC21

Quant Time: Oct 05 02:02:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 05 02:00:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	123518	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	567217	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	345020	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	773965	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	714903	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	564020	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	11784	4.40	ng/uL	0.00
5) Phenol-d5	6.81	99	246860	23.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	160330	24.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	208491	24.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	208186	25.63	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	106008	24.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	122532	24.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	213745	23.81	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	299225	28.81	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	712378	26.38	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	897771	25.46	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	85847	19.22	ng/ul	0.00
57) Fluorene-d10	15.26	176	630850	26.66	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	89494	18.49	ng/ul	0.00
70) Anthracene-d10	17.11	188	959573	25.97	ng/ul	0.00
78) Pyrene-d10	19.42	212	1014339	26.89	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	775167	26.11	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.84	94	18302	1.730	ng/ul#	91
44) Dimethylphthalate	13.72	163	412572	15.652	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100518\
Data File : BN002934.D
Acq On : 04 Oct 2018 16:06
Operator : MJ/SJ
Sample : J5184-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC21

Quant Time: Oct 05 02:02:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 05 02:00:32 2018
Response via : Initial Calibration

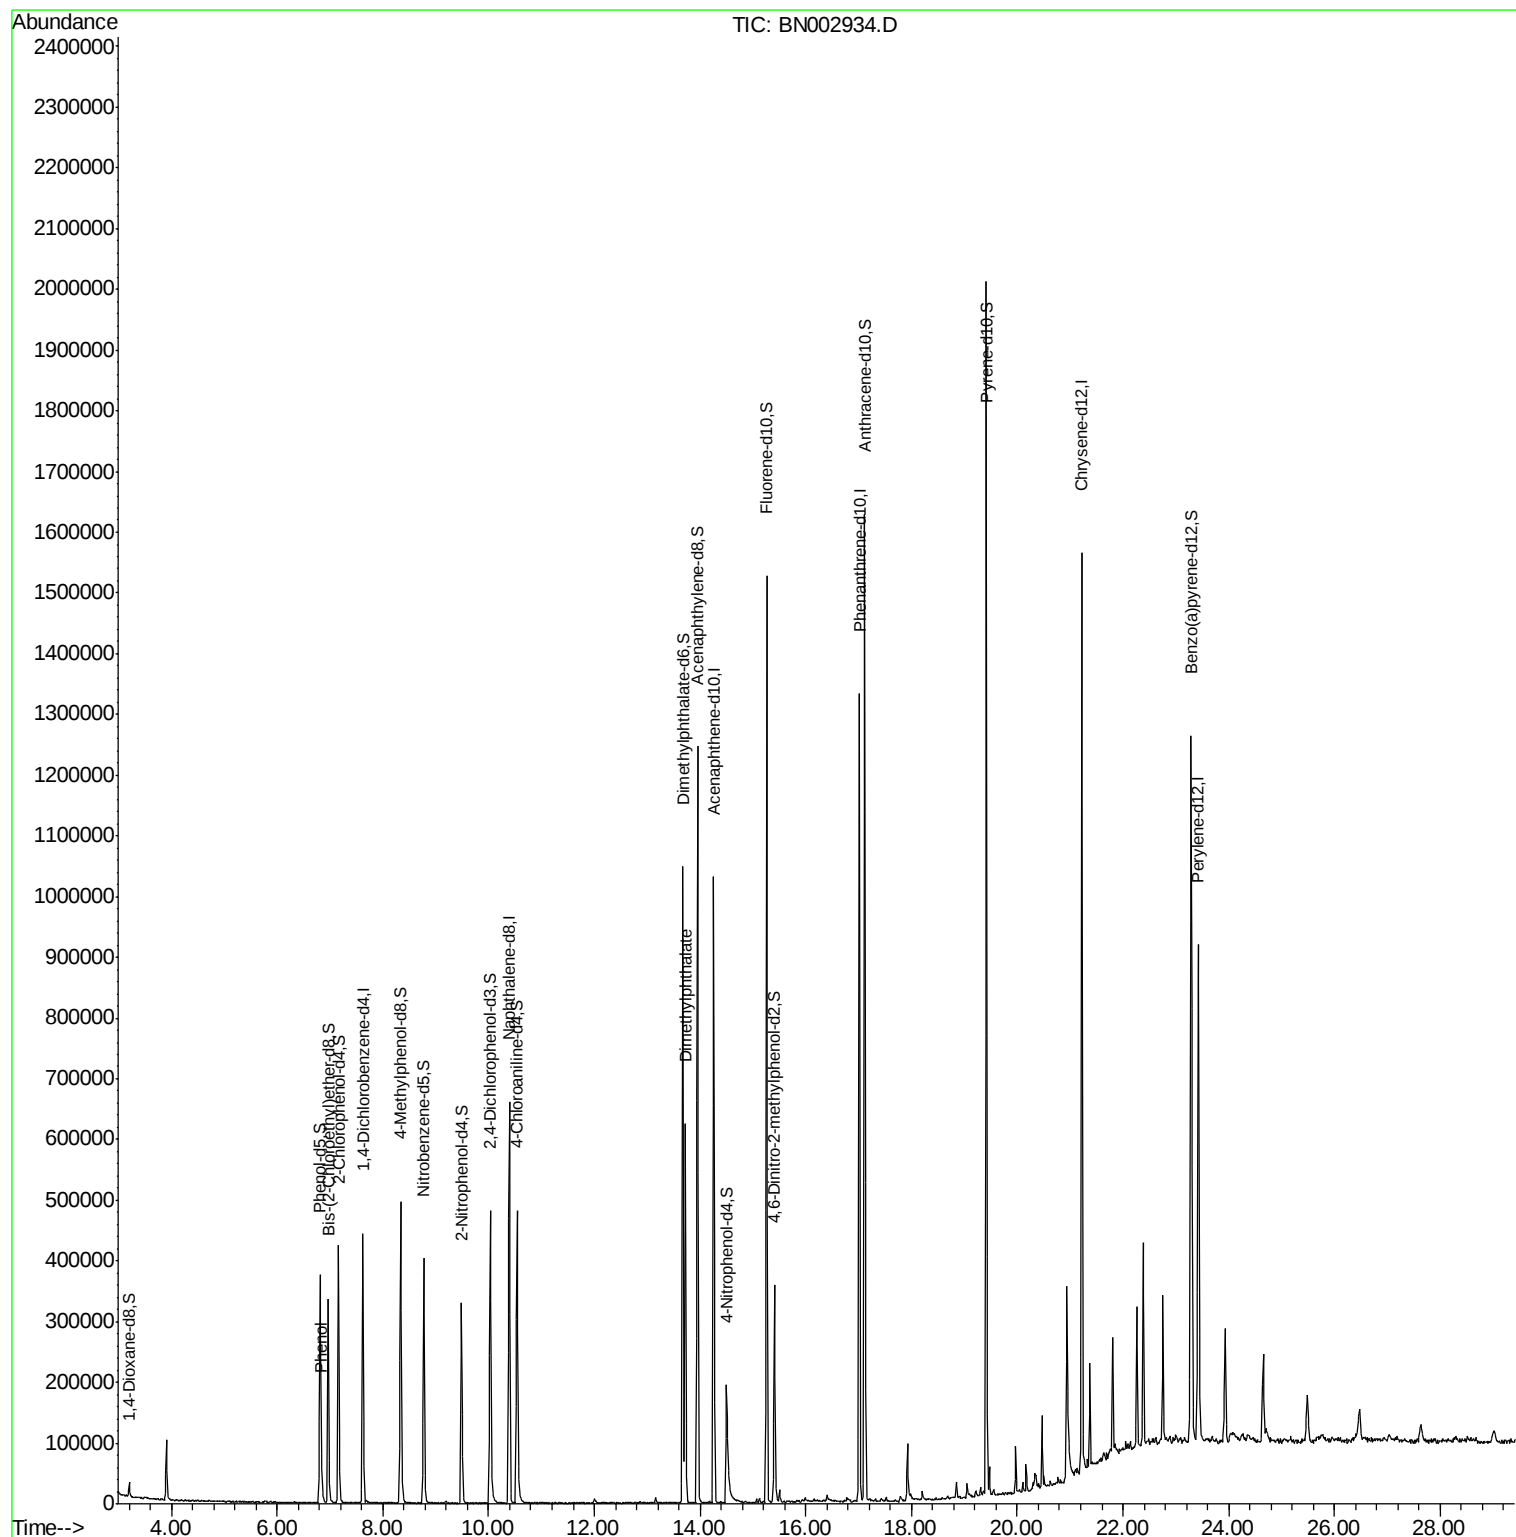

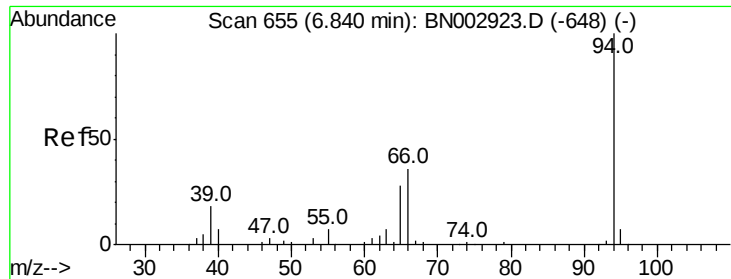





#6

Phenol

Concen: 1.730 ng/ul
 RT: 6.84 min Scan# 655
 Delta R.T. -0.00 min
 Lab File: BN002934.D
 Acq: 04 Oct 2018 16:06

Instrument :
 BNA_N
 ClientSampleId :
 JLC21

Tot Ion: 94 Resp: 18302
 Ion Ratio Lower Upper
 94 100
 65 28.3 23.1 34.7
 66 45.9 29.8 44.6#

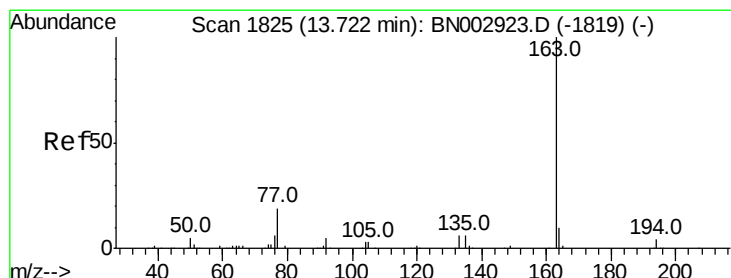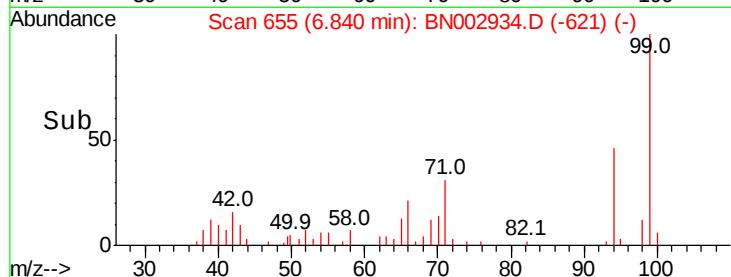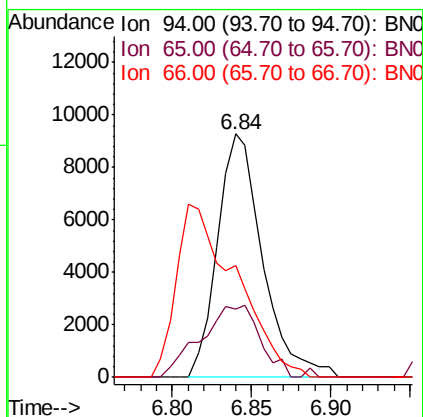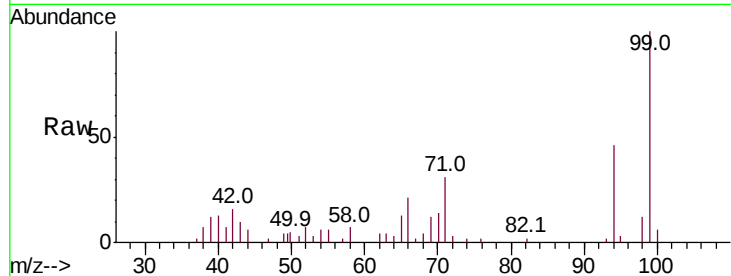

#44

Dimethylphthalate

Concen: 15.652 ng/ul
 RT: 13.72 min Scan# 1825
 Delta R.T. -0.00 min
 Lab File: BN002934.D
 Acq: 04 Oct 2018 16:06

Tgt Ion:163 Resp: 412572
 Ion Ratio Lower Upper
 163 100
 194 4.1 3.5 5.3
 164 10.2 8.1 12.1

