

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100520\
 Data File : BN012056.D
 Acq On : 05 Oct 2020 15:08
 Operator : CG/JU
 Sample : PB132074BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK74

Quant Time: Oct 05 15:45:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 16:22:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	251177	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	945659	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	550772	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	1090314	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	1057232	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	1171556	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	41756	7.23	ng/uL	0.00
5) Phenol-d5	6.83	99	624276	29.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	394377	30.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	516316	30.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	491543	29.79	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	227362	30.28	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	247350	30.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	450044	28.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	626011	34.10	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	1391998	32.22	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	1687040	32.72	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	193915	24.37	ng/ul	0.00
58) Fluorene-d10	15.29	176	1150006	30.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	173315	24.91	ng/ul	0.00
71) Anthracene-d10	17.14	188	1766819	33.42	ng/ul	0.00
79) Pyrene-d10	19.45	212	1819529	32.72	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.32	264	2062671	31.37	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.36	70	13916	1.054	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100520\
Data File : BN012056.D
Acq On : 05 Oct 2020 15:08
Operator : CG/JU
Sample : PB132074BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK74

Quant Time: Oct 05 15:45:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 16:22:43 2020
Response via : Initial Calibration

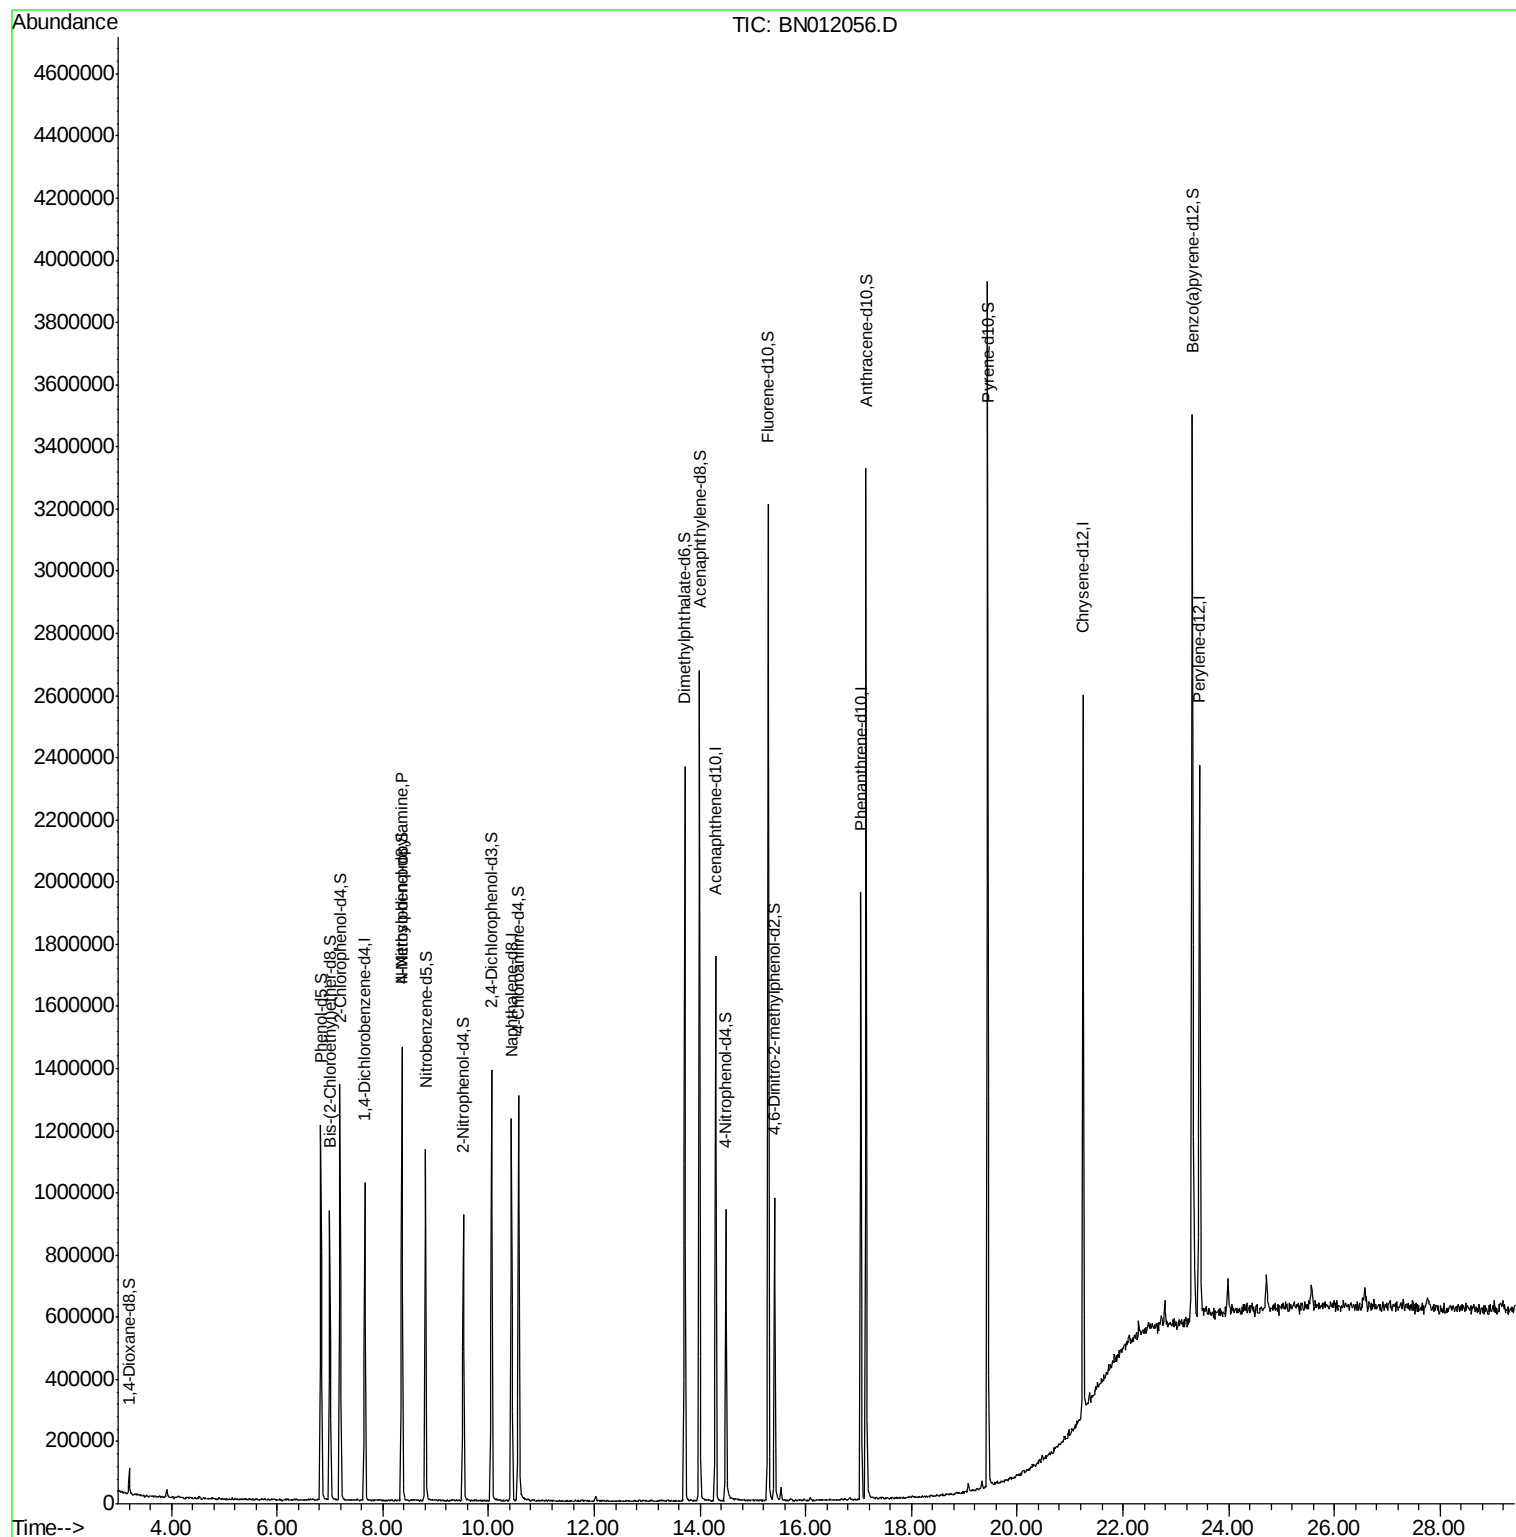

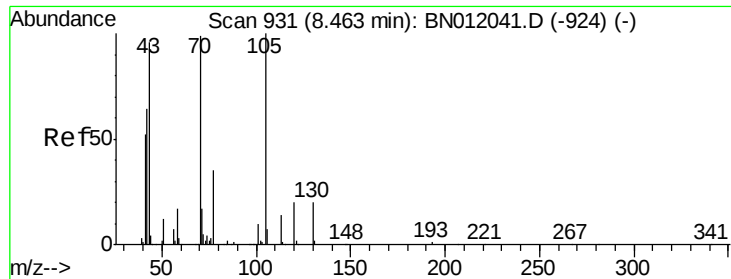

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.054 ng/ul
 RT: 8.36 min Scan# 913
 Delta R.T. -0.11 min
 Lab File: BN012056.D
 Acq: 05 Oct 2020 15:08

Instrument :
 BNA_N
 ClientSampleId :
 SBLK74

Tot Ion: 70 Resp: 13916
 Ion Ratio Lower Upper
 70 100
 42 359.2 50.0 75.0#
 101 0.0 7.6 11.4#
 130 0.0 16.4 24.6#

