

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100520\
 Data File : BN012058.D
 Acq On : 05 Oct 2020 16:20
 Operator : CG/JU
 Sample : L4185-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AR2

Quant Time: Oct 05 16:59:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 16:22:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	245401	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	927977	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	555186	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	1168354	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	1181815	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	1352241	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	35429	6.28	ng/uL	0.00
5) Phenol-d5	6.83	99	112840	5.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	311059	24.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	342851	20.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	214958	13.33	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	194142	26.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	205883	25.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	397039	25.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	35165	1.95	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	1413067	32.45	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	1603640	30.85	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	37149	4.63	ng/ul	0.00
58) Fluorene-d10	15.29	176	1166919	30.70	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	211828	28.41	ng/ul	0.00
71) Anthracene-d10	17.14	188	1927434	34.02	ng/ul	0.00
79) Pyrene-d10	19.45	212	2157640	34.71	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.32	264	2578699	33.98	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.76	163	86149	1.920	ng/ul# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100520\
Data File : BN012058.D
Acq On : 05 Oct 2020 16:20
Operator : CG/JU
Sample : L4185-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AR2

Quant Time: Oct 05 16:59:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 16:22:43 2020
Response via : Initial Calibration

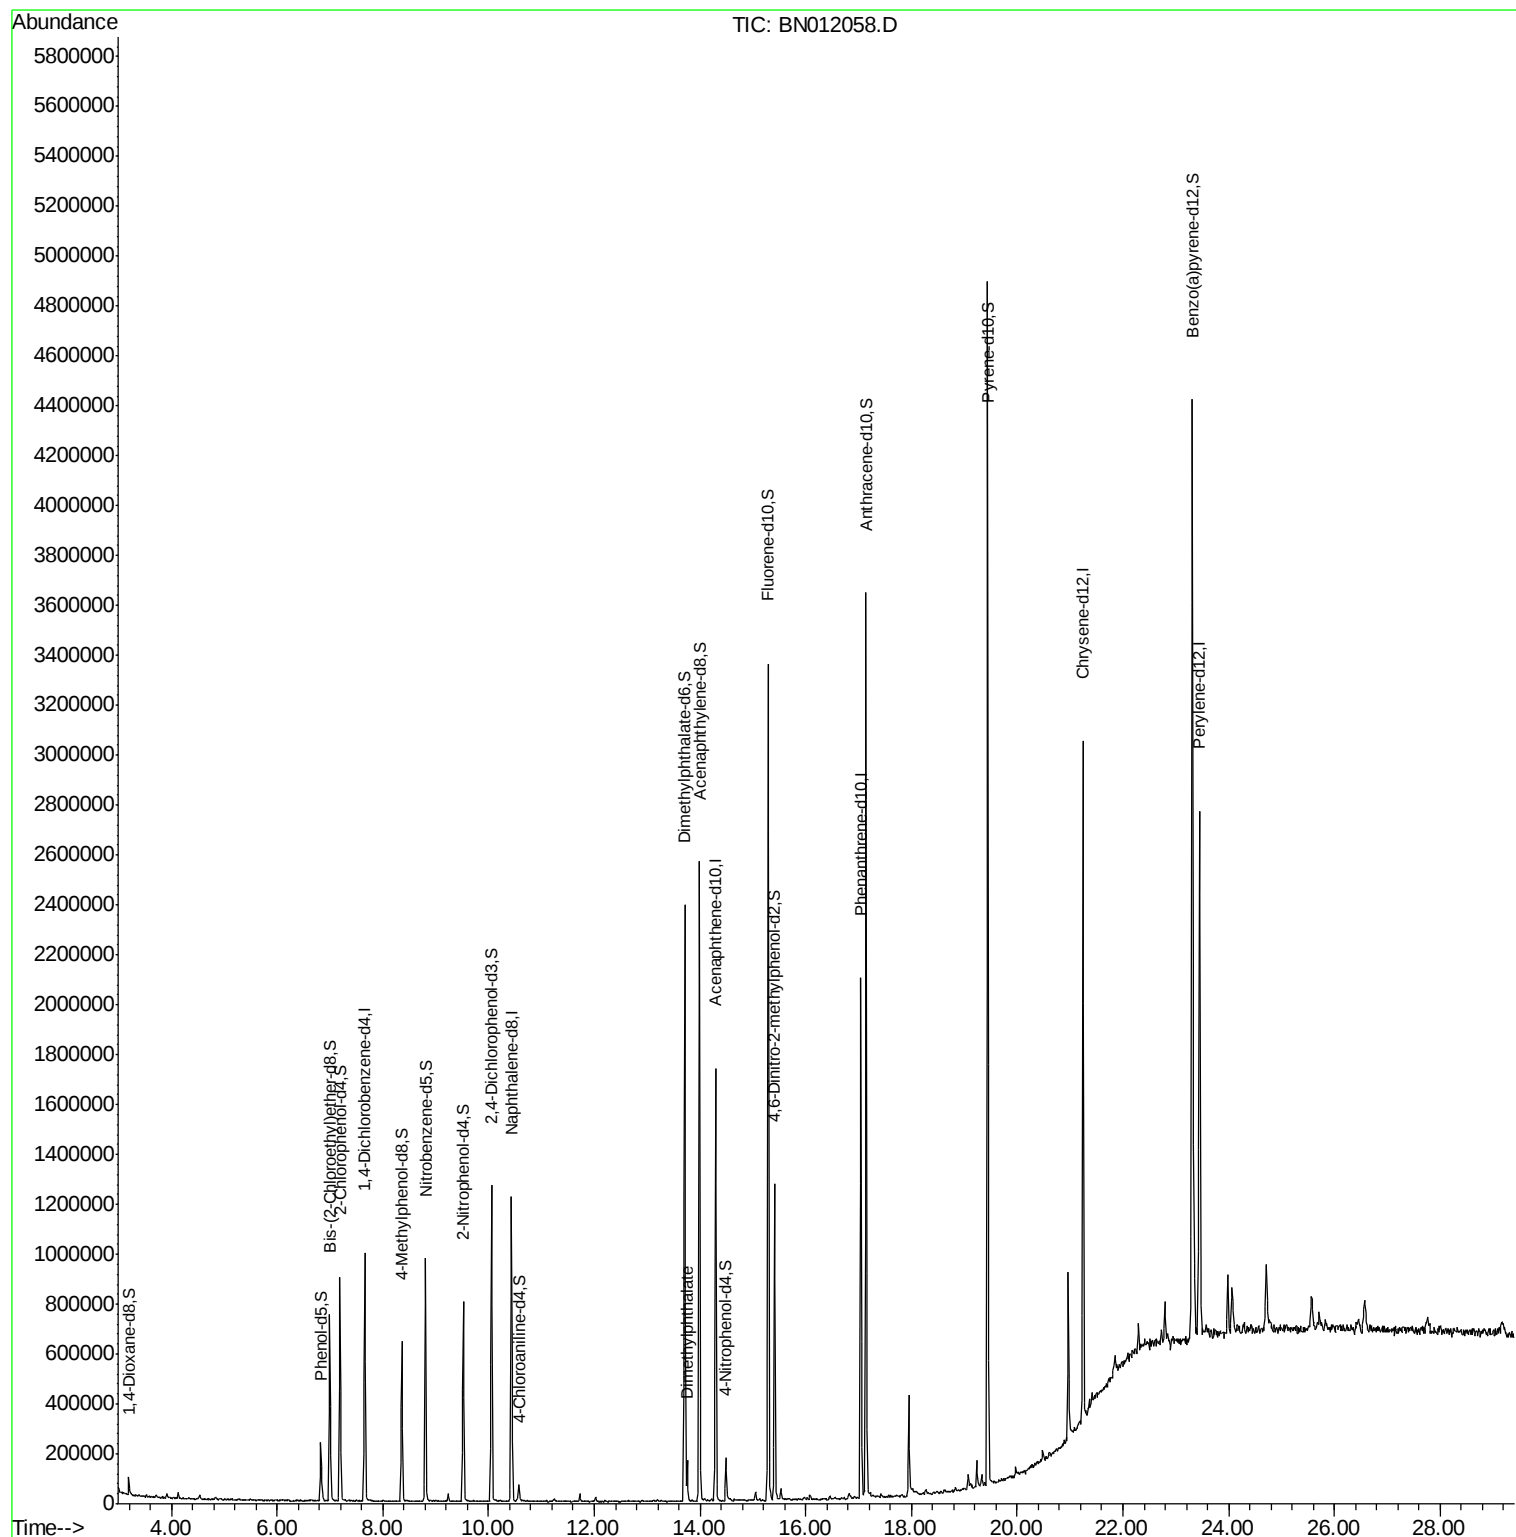

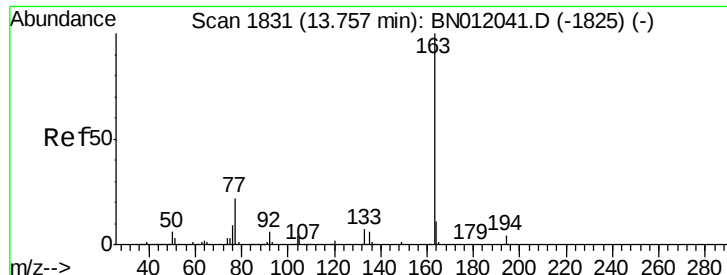

#45

Dimethylphthalate

Concen: 1.920 ng/ul

RT: 13.76 min Scan# 1831

Delta R.T. -0.01 min

Lab File: BN012058.D

Acq: 05 Oct 2020 16:20

Instrument :

BNA_N

ClientSampleId :

C0AR2


Tot Ion:163 Resp: 86149

Ion Ratio Lower Upper

163 100

194 5.9 3.4 5.0#

164 11.3 7.8 11.8

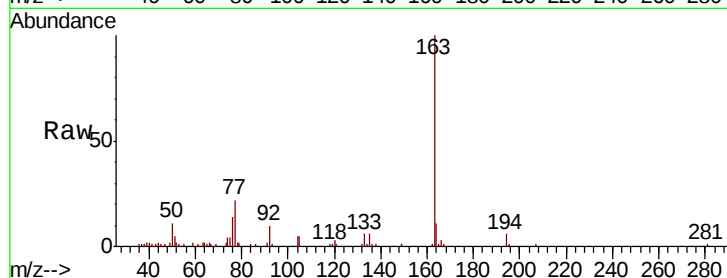

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

