

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100520\
 Data File : BN012061.D
 Acq On : 05 Oct 2020 18:09
 Operator : CG/JU
 Sample : L4185-14
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AR6

Quant Time: Oct 05 18:51:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 05 17:32:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	249616	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	980765	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	580325	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	1181947	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	1154171	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	1294332	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	29914	5.21	ng/uL	0.00
5) Phenol-d5	6.83	99	107711	5.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	331566	25.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	352997	20.95	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	215173	13.12	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	202455	26.00	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	221934	26.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	411136	25.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	168264	8.84	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	1466591	32.22	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	1682148	30.96	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	29289	3.49	ng/ul	-0.01
58) Fluorene-d10	15.29	176	1213567	30.55	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	198783	26.35	ng/ul	0.00
71) Anthracene-d10	17.14	188	1898420	33.12	ng/ul	0.00
79) Pyrene-d10	19.45	212	2135752	35.18	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	2358790	32.47	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.76	163	83336	1.777	ng/ul# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100520\
Data File : BN012061.D
Acq On : 05 Oct 2020 18:09
Operator : CG/JU
Sample : L4185-14
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AR6

Quant Time: Oct 05 18:51:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 05 17:32:05 2020
Response via : Initial Calibration

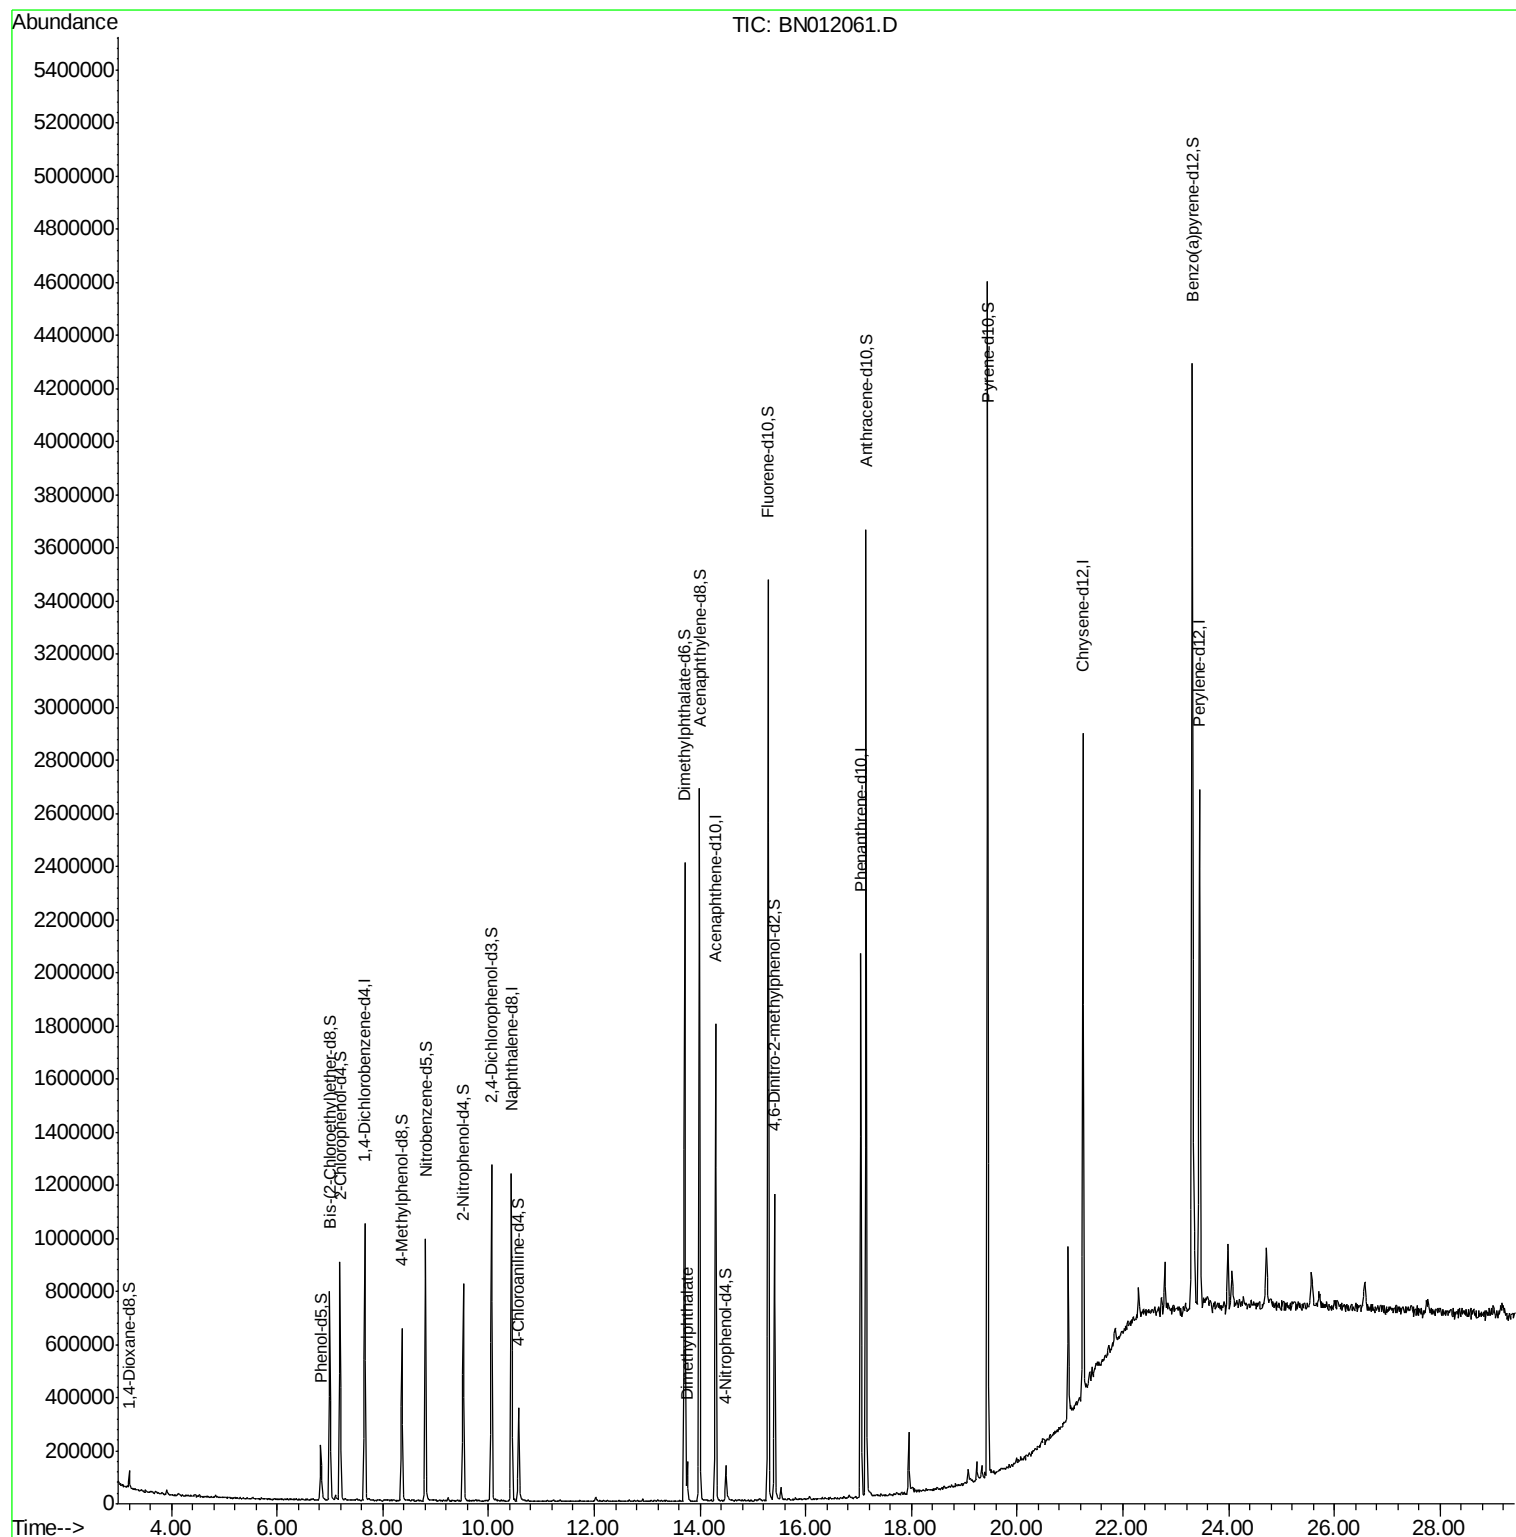

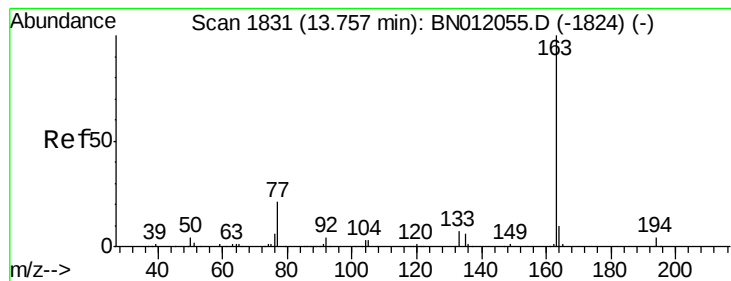

#45
 Dimethylphthalate
 Concen: 1.777 ng/ul
 RT: 13.76 min Scan# 1831
 Delta R.T. -0.01 min
 Lab File: BN012061.D
 Acq: 05 Oct 2020 18:09

Instrument :
 BNA_N
 ClientSampleId :
 C0AR6

Tot Ion	Ratio	Lower	Upper
163	100		
194	5.7	3.4	5.0#
164	8.8	7.8	11.8

