

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100520\
 Data File : BN012062.D
 Acq On : 05 Oct 2020 18:45
 Operator : CG/JU
 Sample : L4185-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AR5

Quant Time: Oct 06 00:25:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 16:22:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	269182	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1025756	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	617307	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	1289541	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	1287197	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	1461845	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	44399	7.18	ng/uL	0.00
5) Phenol-d5	6.83	99	205511	9.15	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	459164	33.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	537131	29.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	355750	20.12	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	290077	35.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	329234	37.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	617375	36.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	78440	3.94	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	2039891	42.13	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	2467196	42.69	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	64189	7.20	ng/ul	0.00
58) Fluorene-d10	15.29	176	1709210	40.45	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	304753	37.03	ng/ul	0.00
71) Anthracene-d10	17.14	188	2632261	42.09	ng/ul	0.00
79) Pyrene-d10	19.45	212	3057081	45.16	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	3625907	44.20	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.76	163	138438	2.774	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100520\
Data File : BN012062.D
Acq On : 05 Oct 2020 18:45
Operator : CG/JU
Sample : L4185-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AR5

Quant Time: Oct 06 00:25:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 16:22:43 2020
Response via : Initial Calibration

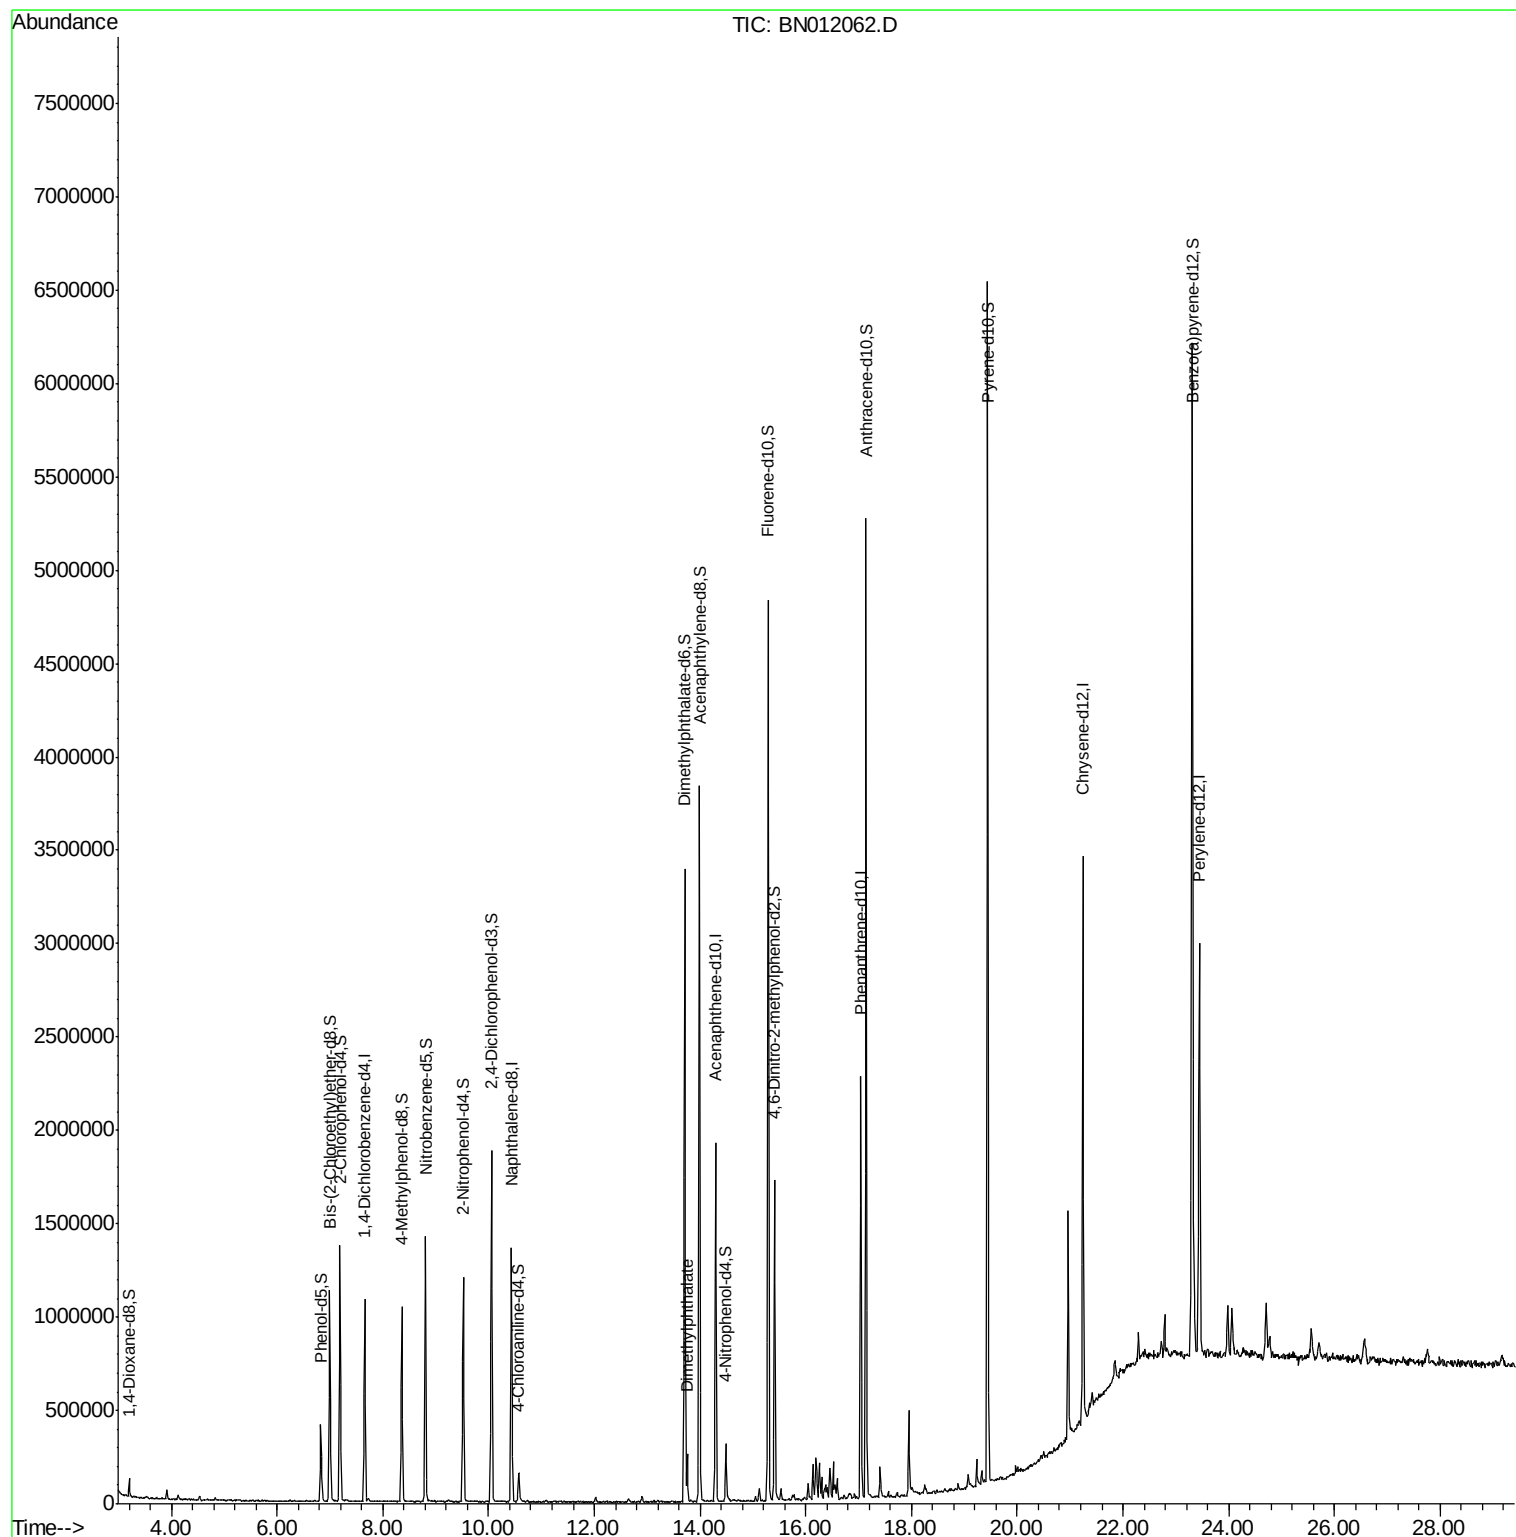

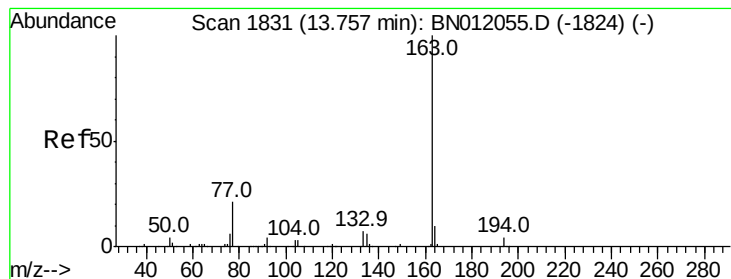

#45

Dimethylphthalate

Concen: 2.774 ng/ul

RT: 13.76 min Scan# 1831

Delta R.T. -0.01 min

Lab File: BN012062.D

Acq: 05 Oct 2020 18:45

Instrument :

BNA_N

ClientSampleId :

C0AR5


Tot Ion:163 Resp: 138438

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 10.0 7.8 11.8

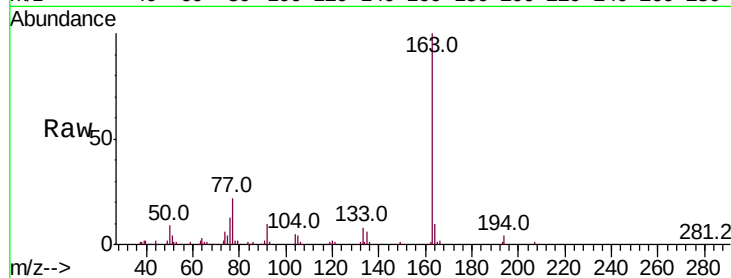

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

