

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100520\
 Data File : BN012073.D
 Acq On : 06 Oct 2020 02:01
 Operator : CG/JU
 Sample : L4184-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AP0

Quant Time: Oct 06 04:07:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 06 00:53:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	342026	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1403490	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	803138	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	1677163	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	1590405	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	1718300	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	34837	4.43	ng/uL	0.00
5) Phenol-d5	6.83	99	571198	20.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	365569	20.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	481613	20.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	436956	19.45	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	219563	19.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	249083	20.67	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	453515	19.62	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	583518	21.41	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	1354195	21.50	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	1701576	22.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	187076	16.13	ng/ul	0.00
58) Fluorene-d10	15.29	176	1160810	21.11	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	163384	15.26	ng/ul	0.00
71) Anthracene-d10	17.14	188	1687222	20.75	ng/ul	0.00
79) Pyrene-d10	19.44	212	1817495	21.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	1975494	20.49	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.76	163	637892	9.826	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100520\
Data File : BN012073.D
Acq On : 06 Oct 2020 02:01
Operator : CG/JU
Sample : L4184-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP0

Quant Time: Oct 06 04:07:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 06 00:53:35 2020
Response via : Initial Calibration

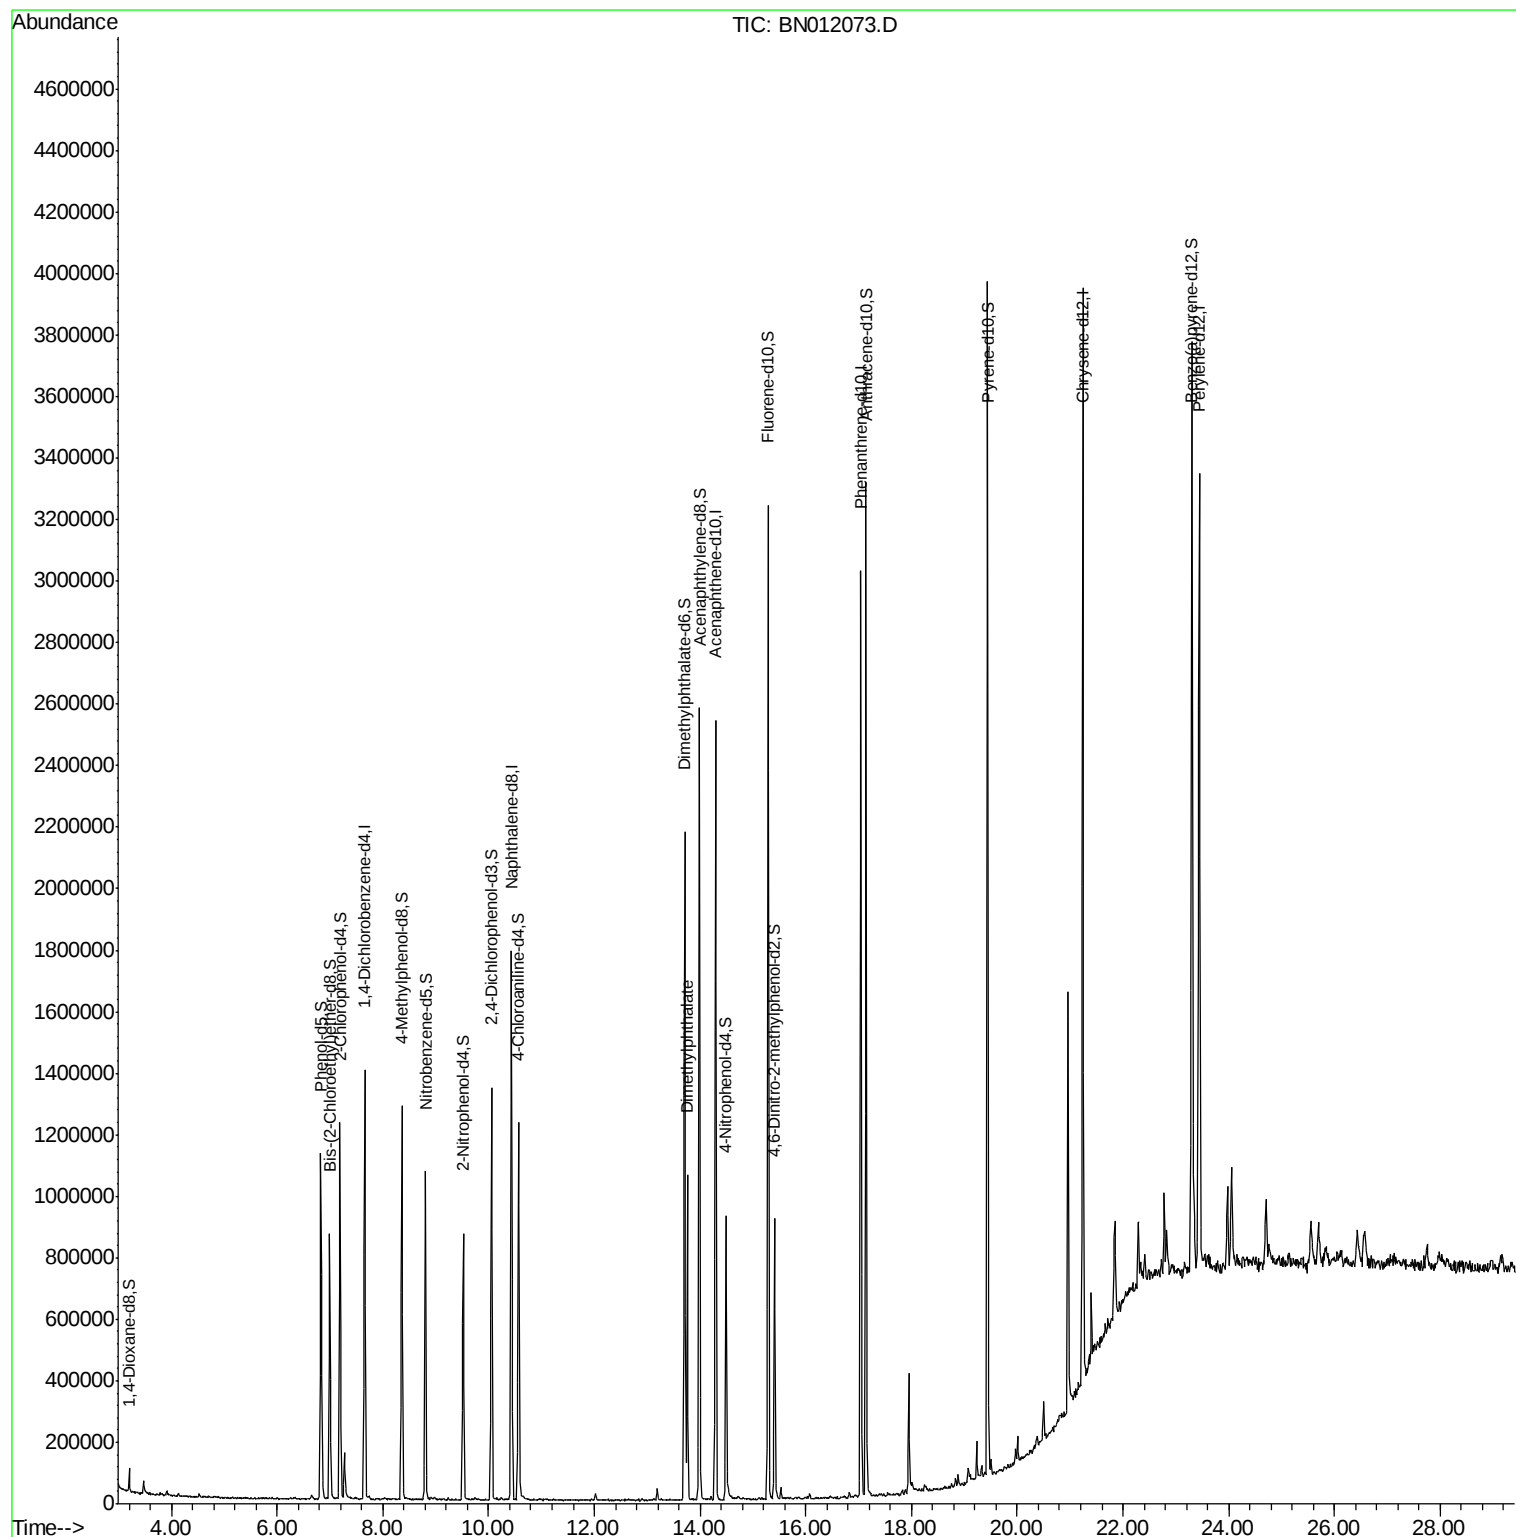

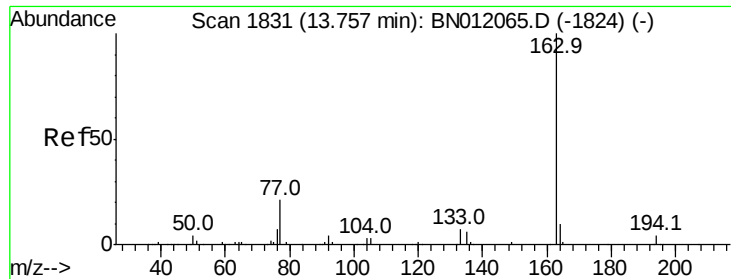

#45

Dimethylphthalate

Concen: 9.826 ng/ul

RT: 13.76 min Scan# 1831

Delta R.T. 0.00 min

Lab File: BN012073.D

Acq: 06 Oct 2020 02:01

Instrument :

BNA_N

ClientSampleId :

C0AP0


Tot Ion:163 Resp: 637892

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.0

164 9.2 7.8 11.8

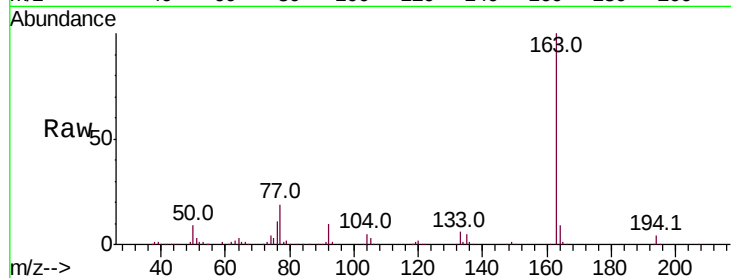

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

