

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100520\
 Data File : BN012077.D
 Acq On : 06 Oct 2020 04:26
 Operator : CG/JU
 Sample : L4184-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AM2

Quant Time: Oct 06 05:18:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 06 00:53:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	288236	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1131423	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	679425	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	1349077	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	1312462	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	1464149	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	31386	4.74	ng/uL	0.00
5) Phenol-d5	6.83	99	556076	23.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	344145	23.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	454275	23.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	437972	23.13	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	212866	23.69	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	217657	22.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	420145	22.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	409182	18.63	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	1247778	23.41	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	1600997	25.17	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	164814	16.79	ng/ul	0.00
58) Fluorene-d10	15.29	176	1077008	23.16	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	135141	15.70	ng/ul	0.00
71) Anthracene-d10	17.14	188	1605367	24.54	ng/ul	0.00
79) Pyrene-d10	19.44	212	1711819	24.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	1894337	23.05	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.76	163	479055	8.723	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100520\
Data File : BN012077.D
Acq On : 06 Oct 2020 04:26
Operator : CG/JU
Sample : L4184-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AM2

Quant Time: Oct 06 05:18:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 06 00:53:35 2020
Response via : Initial Calibration

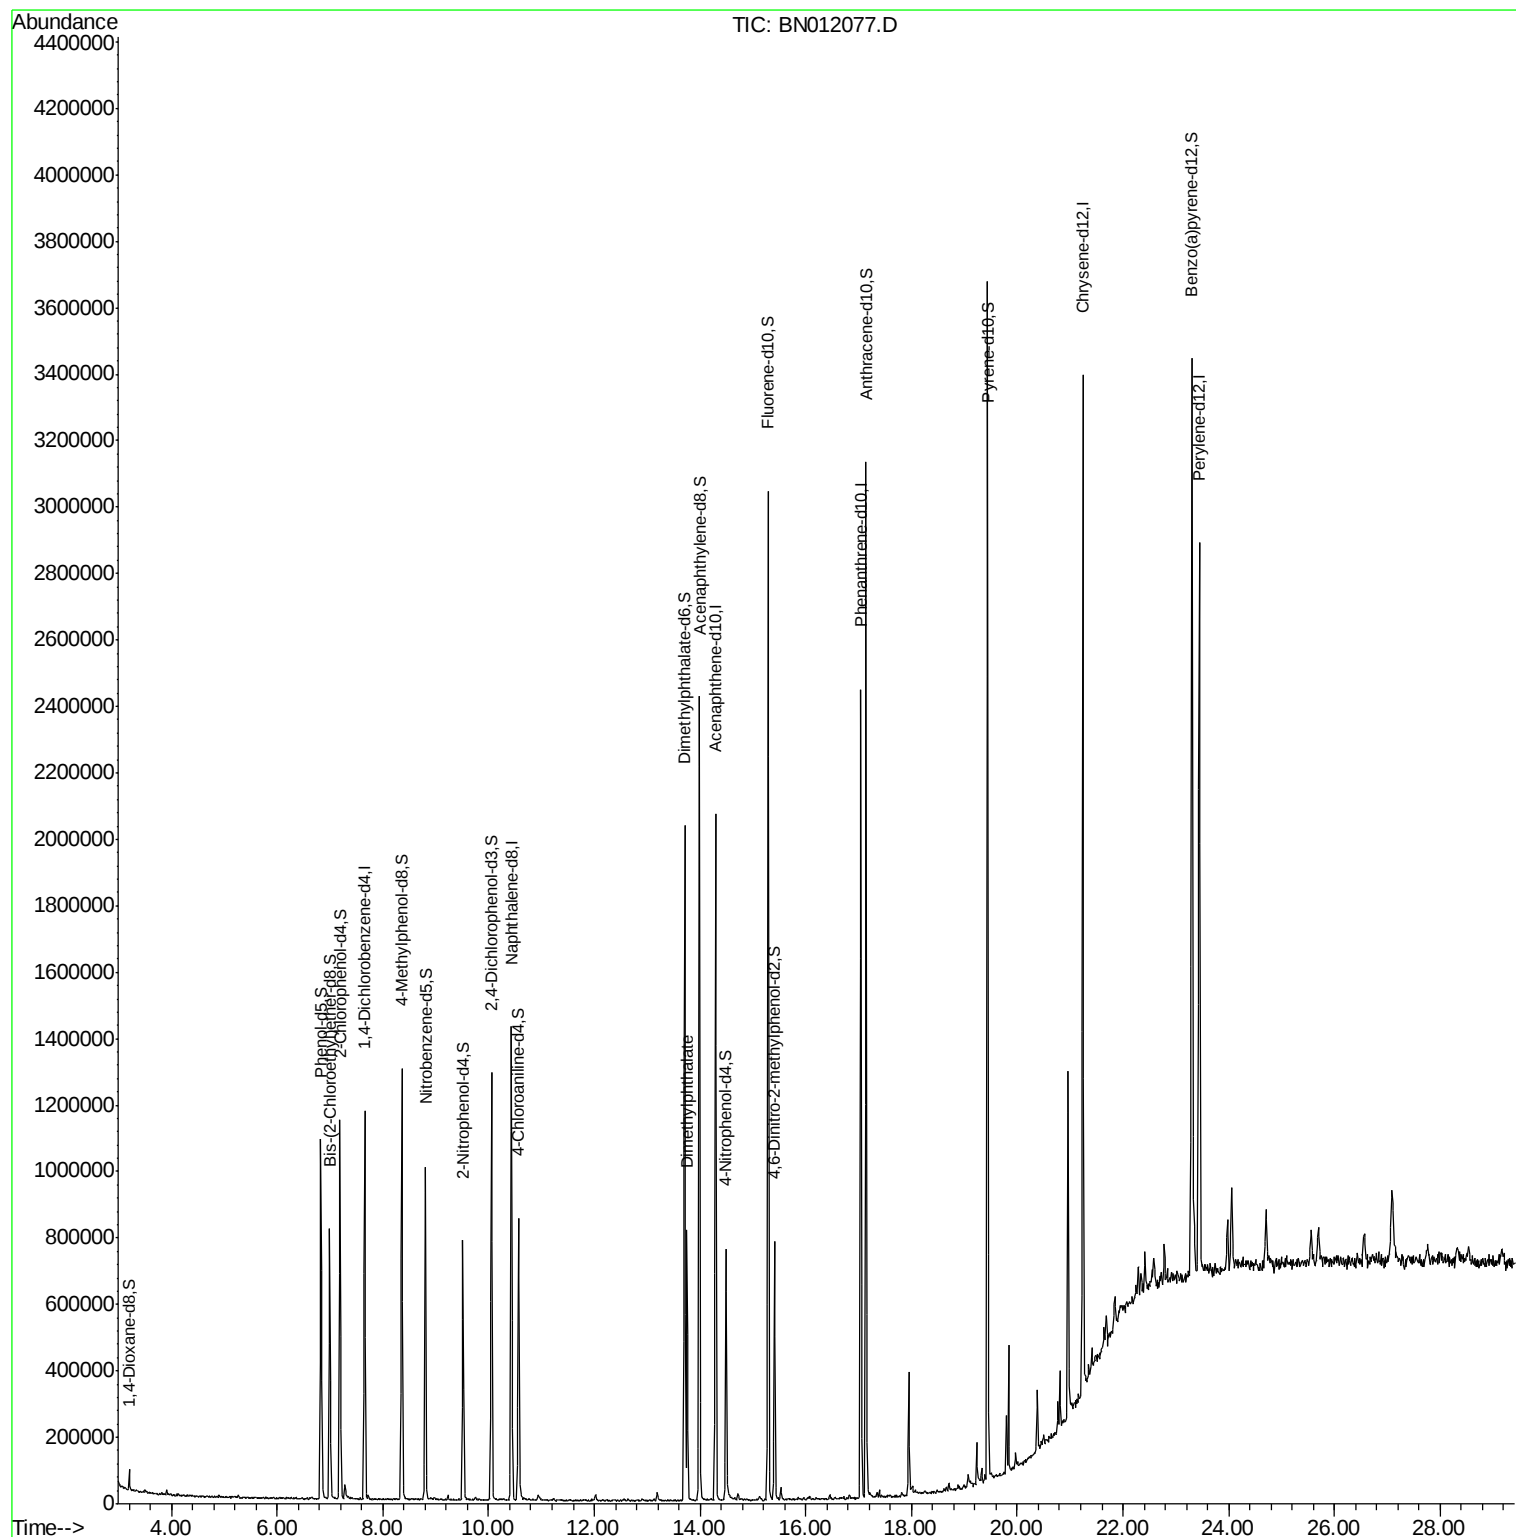

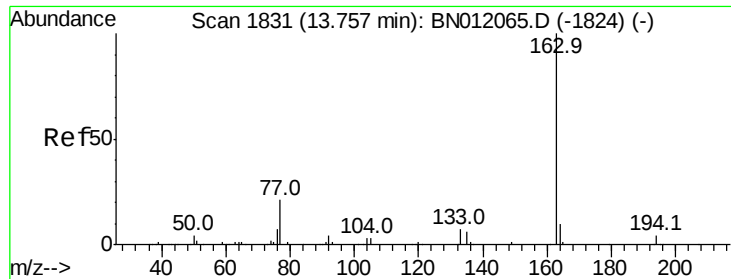

#45

Dimethylphthalate

Concen: 8.723 ng/ul

RT: 13.76 min Scan# 1831

Delta R.T. -0.00 min

Lab File: BN012077.D

Acq: 06 Oct 2020 04:26

Instrument :

BNA_N

ClientSampleId :

C0AM2


Tot Ion:163 Resp: 479055

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 10.0 7.8 11.8

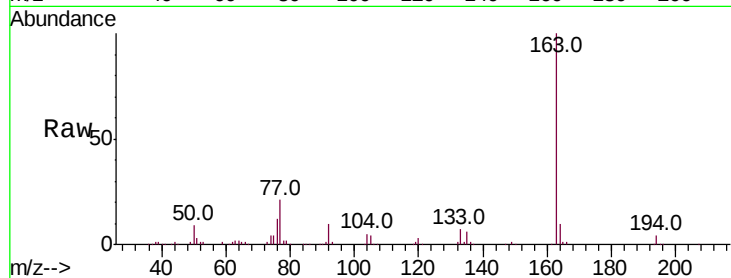

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

