

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100520\
 Data File : BN012059.D
 Acq On : 05 Oct 2020 16:57
 Operator : CG/JU
 Sample : L4185-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AR1

Quant Time: Oct 05 17:29:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 16:22:43 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.658	152	251515	20.00	ng/ul	0.00
18) Naphthalene-d8	10.434	136	1020038	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.298	164	622494	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.045	188	1299071	20.00	ng/ul	0.00
78) Chrysene-d12	21.245	240	1306116	20.00	ng/ul	0.00
86) Perylene-d12	23.451	264	1419672	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	32858	5.68	ng/uL	0.00
5) Phenol-d5	6.828	99	119705	5.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	6.999	67	358453	27.79	ng/ul	0.00
9) 2-Chlorophenol-d4	7.193	132	383814	22.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.358	113	233371	14.12	ng/ul	0.00
19) Nitrobenzene-d5	8.805	128	226431	27.96	ng/ul	0.00
22) 2-Nitrophenol-d4	9.522	143	248334	28.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.052	165	452634	26.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.575	131	34652	1.75	ng/ul	0.00
44) Dimethylphthalate-d6	13.710	166	1639779	33.58	ng/ul	0.00
47) Acenaphthylene-d8	13.987	160	1837802	31.53	ng/ul	0.00
52) 4-Nitrophenol-d4	14.493	143	40105	4.46	ng/ul	0.00
58) Fluorene-d10	15.292	176	1386143	32.53	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.410	200	260097	31.37	ng/ul	0.00
71) Anthracene-d10	17.145	188	2315879	36.76	ng/ul	0.00
79) Pyrene-d10	19.445	212	2564285	37.33	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.310	264	3015501	37.85	ng/ul	0.00
Target Compounds						Qvalue
45) Dimethylphthalate	13.757	163	130652	2.60	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100520\
Data File : BN012059.D
Acq On : 05 Oct 2020 16:57
Operator : CG/JU
Sample : L4185-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AR1


Quant Time: Oct 05 17:29:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 16:22:43 2020
Response via : Initial Calibration

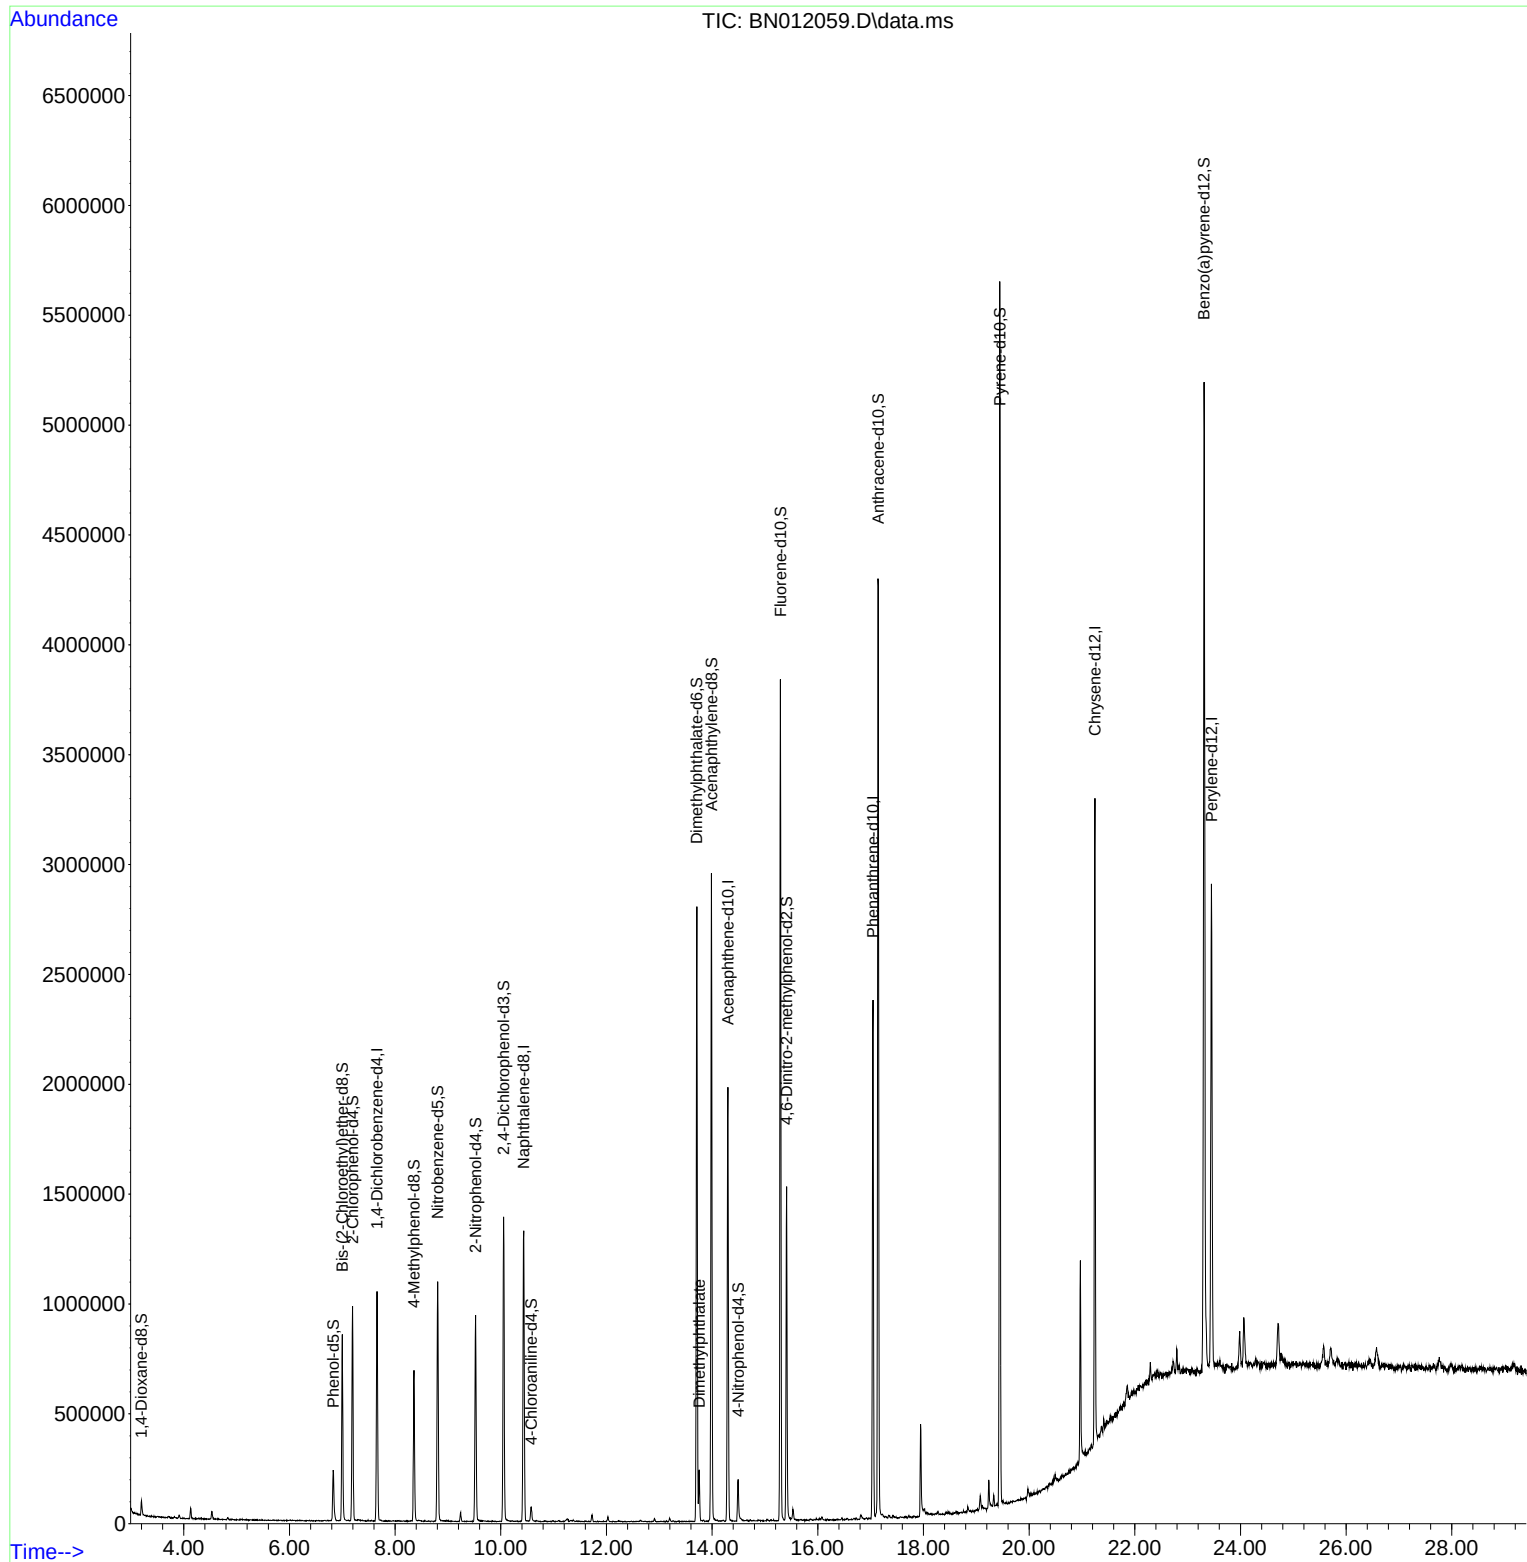

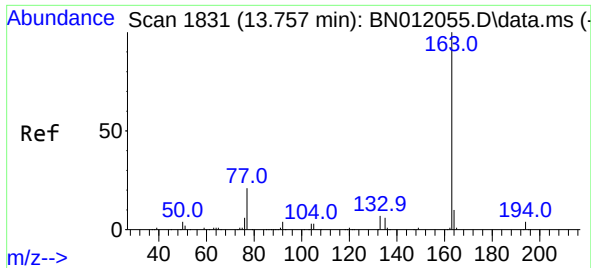

#45
 Dimethylphthalate
 Concen: 2.60 ng/ul
 RT: 13.757 min Scan# 1831
 Delta R.T. -0.005 min
 Lab File: BN012059.D
 Acq: 05 Oct 2020 16:57

Instrument :
 BNA_N
 ClientSampleId :
 C0AR1

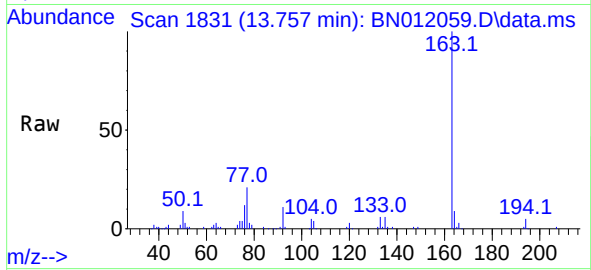

Tgt Ion:163 Resp: 130652

Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.4	5.0
164	9.5	7.8	11.8

