

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100520\
 Data File : BN012064.D
 Acq On : 05 Oct 2020 19:58
 Operator : CG/JU
 Sample : L4209-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLWS8

Quant Time: Oct 06 00:24:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 16:22:43 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.658	152	230901	20.00	ng/ul	0.00
18) Naphthalene-d8	10.428	136	912375	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.298	164	581538	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.039	188	1241099	20.00	ng/ul	0.00
78) Chrysene-d12	21.239	240	1183936	20.00	ng/ul	0.00
86) Perylene-d12	23.451	264	1352859	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	27689	5.22	ng/uL	0.00
5) Phenol-d5	6.828	99	61690	3.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	6.999	67	341568	28.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.193	132	175726	11.28	ng/ul	0.00
13) 4-Methylphenol-d8	8.358	113	125501	8.27	ng/ul	0.00
19) Nitrobenzene-d5	8.805	128	209355	28.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.522	143	203131	25.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.052	165	286901	19.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.575	131	41703	2.35	ng/ul	0.00
44) Dimethylphthalate-d6	13.710	166	1566116	34.33	ng/ul	0.00
47) Acenaphthylene-d8	13.987	160	790081	14.51	ng/ul	0.00
52) 4-Nitrophenol-d4	14.493	143	38092	4.53	ng/ul	0.00
58) Fluorene-d10	15.292	176	1308208	32.86	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.410	200	252326	31.85	ng/ul	0.00
71) Anthracene-d10	17.139	188	2088290	34.70	ng/ul	0.00
79) Pyrene-d10	19.445	212	2415714	38.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.310	264	2697155	35.53	ng/ul	0.00
Target Compounds						Qvalue
45) Dimethylphthalate	13.751	163	98688	2.10	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100520\
Data File : BN012064.D
Acq On : 05 Oct 2020 19:58
Operator : CG/JU
Sample : L4209-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLWS8


Quant Time: Oct 06 00:24:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 16:22:43 2020
Response via : Initial Calibration

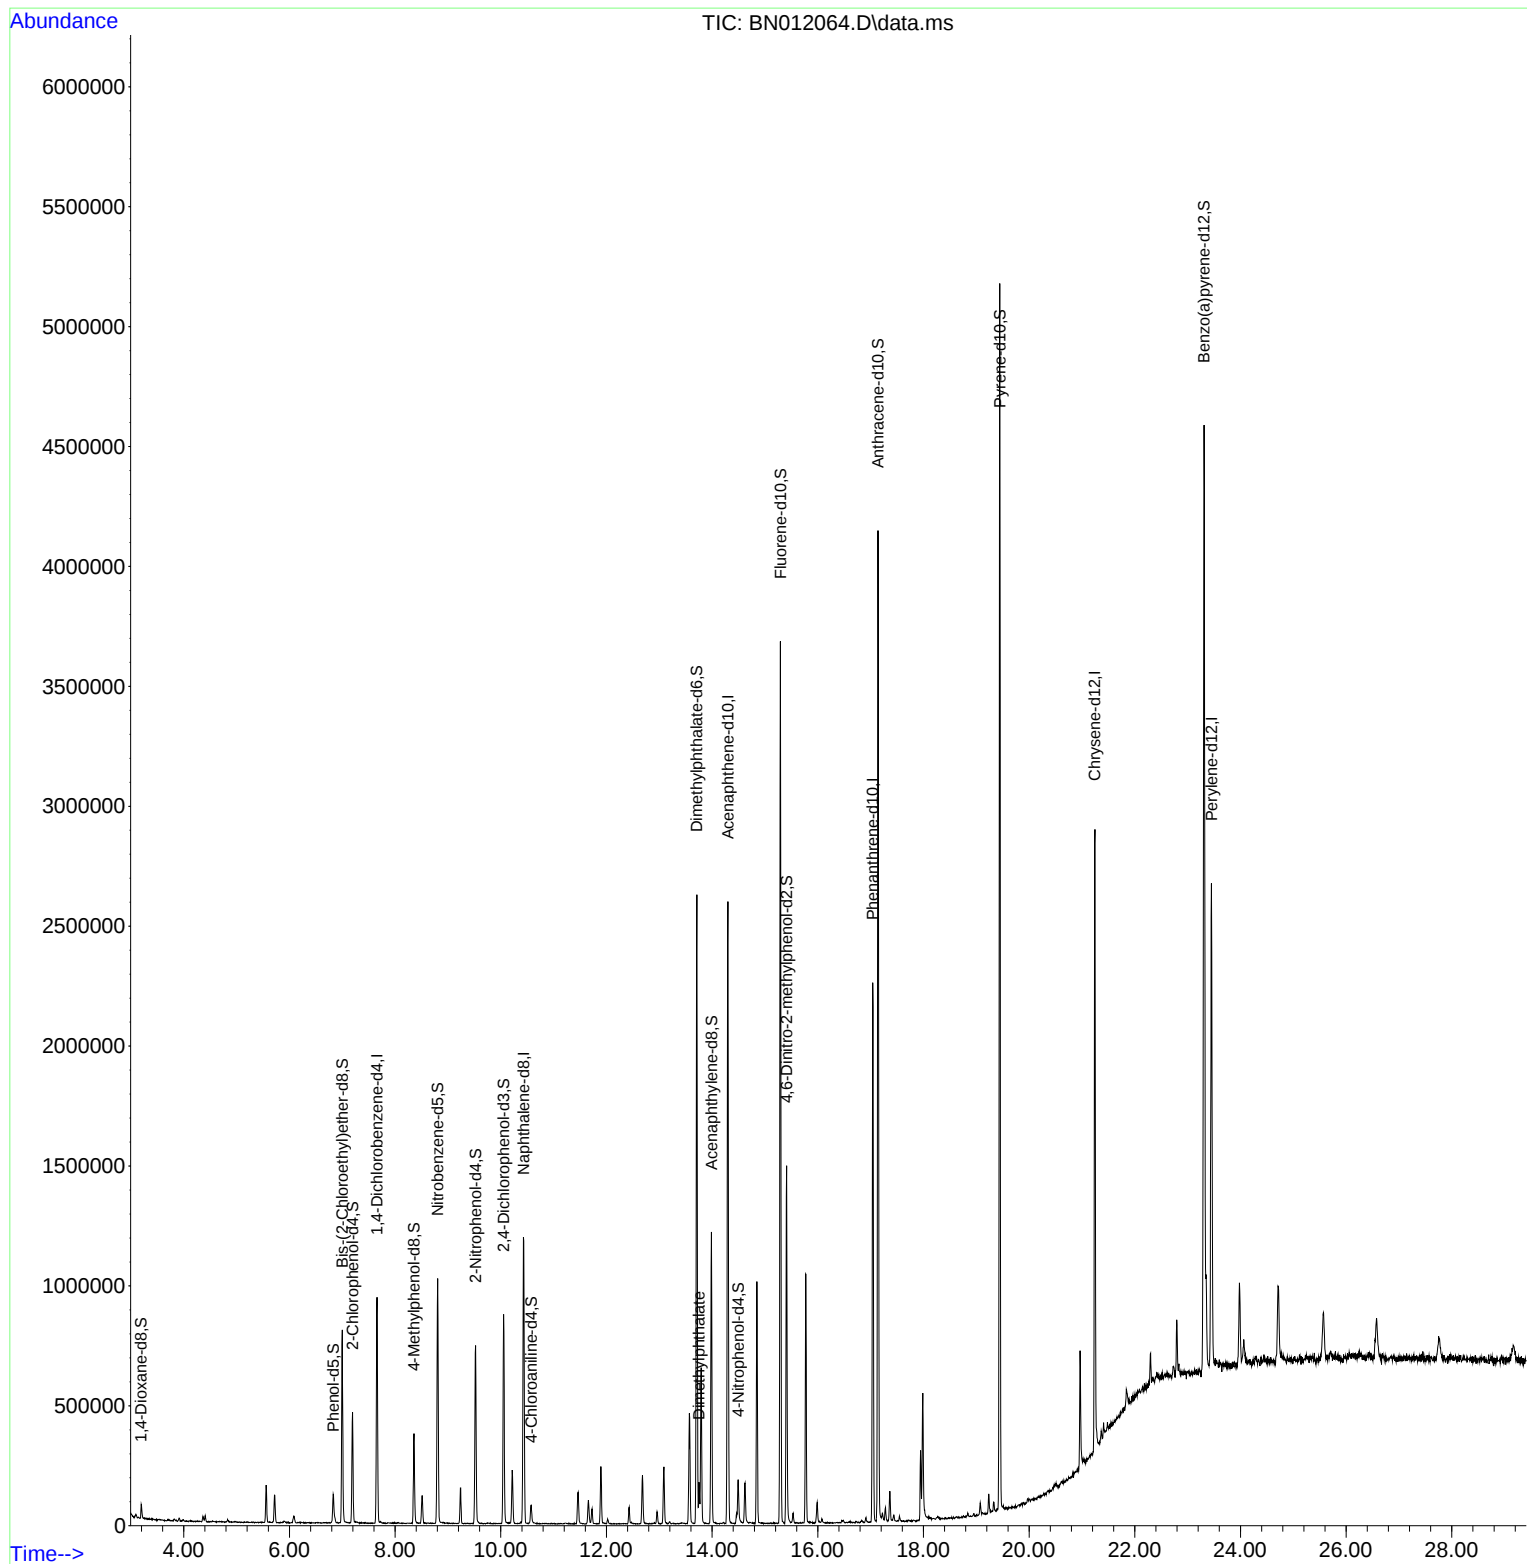

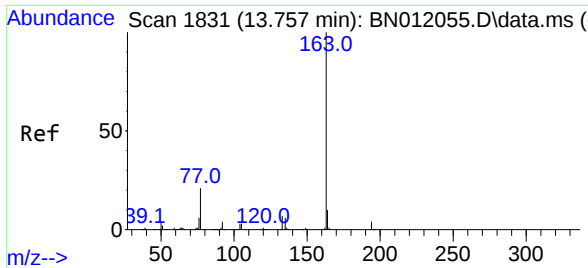

#45
 Dimethylphthalate
 Concen: 2.10 ng/ul
 RT: 13.751 min Scan# 1830
 Delta R.T. -0.011 min
 Lab File: BN012064.D
 Acq: 05 Oct 2020 19:58

Instrument :
 BNA_N
 ClientSampleId :
 JLWS8

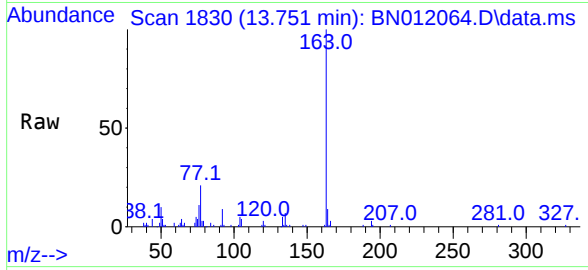

Tgt Ion:163	Resp:	98688
Ion	Ratio	Lower Upper
163	100	
194	3.3	3.4 5.0#
164	8.7	7.8 11.8

