

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100520\
 Data File : BN012070.D
 Acq On : 06 Oct 2020 00:12
 Operator : CG/JU
 Sample : L4184-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL2

Quant Time: Oct 06 00:54:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 06 00:53:35 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.658	152	284168	20.00	ng/ul	0.00
18) Naphthalene-d8	10.428	136	1123312	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.298	164	683248	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.039	188	1381881	20.00	ng/ul	0.00
78) Chrysene-d12	21.239	240	1297070	20.00	ng/ul	0.00
86) Perylene-d12	23.445	264	1432115	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	13046	2.00	ng/uL	0.00
5) Phenol-d5	6.828	99	186632	7.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	6.999	67	151220	10.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.193	132	163707	8.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.358	113	115678	6.20	ng/ul	0.00
19) Nitrobenzene-d5	8.805	128	84343	9.46	ng/ul	0.00
22) 2-Nitrophenol-d4	9.522	143	76210	7.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.057	165	137940	7.46	ng/ul	0.00
29) 4-Chloroaniline-d4	10.569	131	96352	4.42	ng/ul	0.00
44) Dimethylphthalate-d6	13.710	166	531901	9.92	ng/ul	0.00
47) Acenaphthylene-d8	13.987	160	567291	8.87	ng/ul	0.00
52) 4-Nitrophenol-d4	14.493	143	34185	3.46	ng/ul	0.00
58) Fluorene-d10	15.292	176	454704	9.72	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.410	200	41261	4.68	ng/ul	0.00
71) Anthracene-d10	17.139	188	635680	9.49	ng/ul	0.00
79) Pyrene-d10	19.439	212	639746	9.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.304	264	587299	7.31	ng/ul	0.00
Target Compounds						
						Qvalue
14) Acetophenone	8.475	105	31932	1.07	ng/ul	97
45) Dimethylphthalate	13.757	163	192538	3.49	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100520\
Data File : BN012070.D
Acq On : 06 Oct 2020 00:12
Operator : CG/JU
Sample : L4184-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL2

Quant Time: Oct 06 00:54:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 06 00:53:35 2020
Response via : Initial Calibration




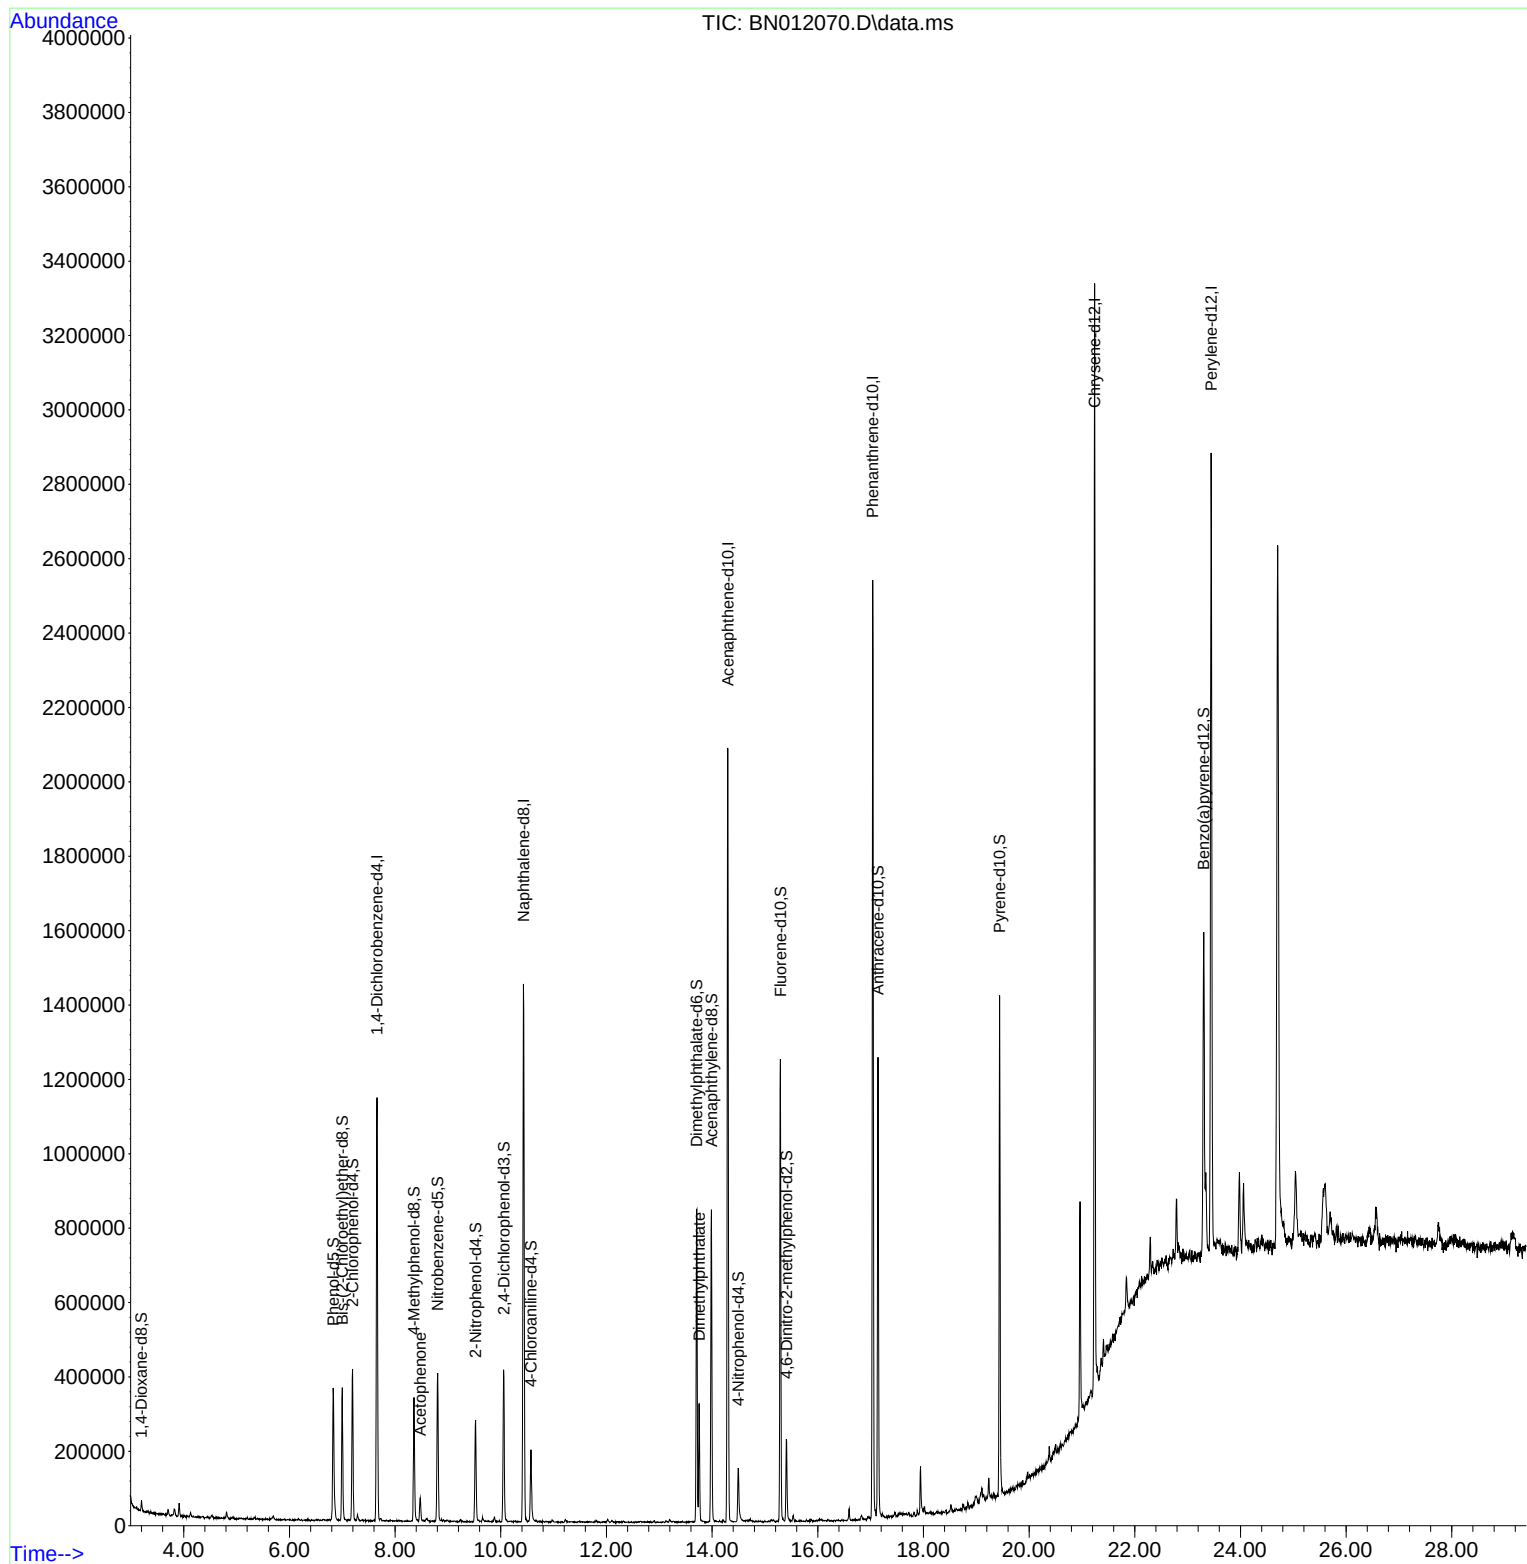


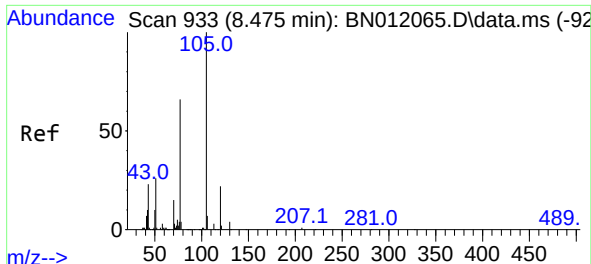

#14
Acetophenone
Concen: 1.07 ng/ul
RT: 8.475 min Scan# 933
Delta R.T. 0.000 min
Lab File: BN012070.D
Acq: 06 Oct 2020 00:12

Instrument :
BNA_N
ClientSampled :
C0AL2

Tgt Ion:105 Resp: 31932
Ion Ratio Lower Upper
105 100
77 82.1 66.9 100.3
51 34.6 24.3 36.5

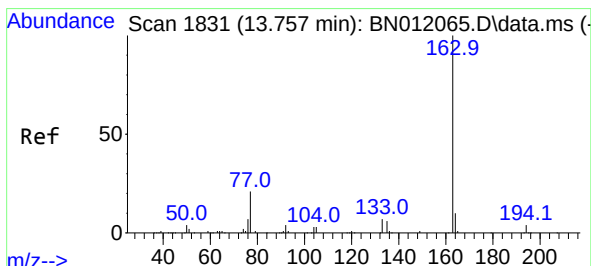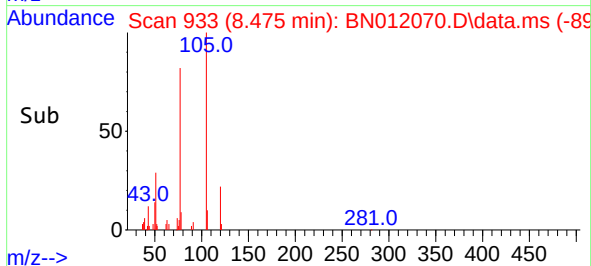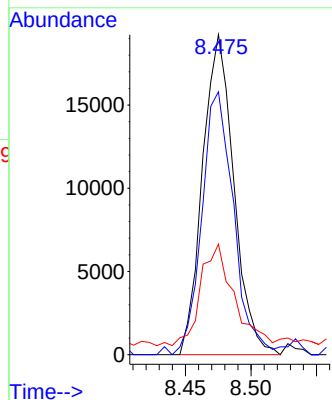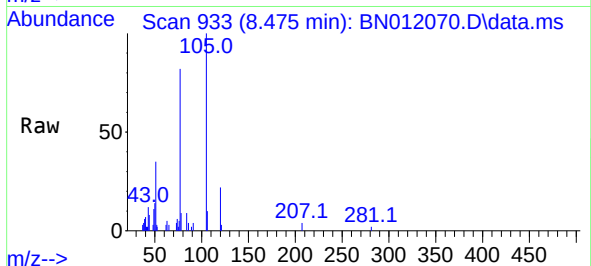

#45
Dimethylphthalate
Concen: 3.49 ng/ul
RT: 13.757 min Scan# 1831
Delta R.T. 0.000 min
Lab File: BN012070.D
Acq: 06 Oct 2020 00:12

Tgt Ion:163 Resp: 192538
Ion Ratio Lower Upper
163 100
194 4.6 3.4 5.0
164 9.6 7.8 11.8

