

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100520\
 Data File : BN012075.D
 Acq On : 06 Oct 2020 03:13
 Operator : CG/JU
 Sample : L4184-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AM5

Quant Time: Oct 06 04:07:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 06 00:53:35 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.658	152	294407	20.00	ng/ul	0.00
18) Naphthalene-d8	10.428	136	1144676	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.293	164	695248	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.040	188	1365012	20.00	ng/ul	0.00
78) Chrysene-d12	21.239	240	1345061	20.00	ng/ul	0.00
86) Perylene-d12	23.439	264	1377932	20.00	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	42608	6.30	ng/uL	0.00
5) Phenol-d5	6.828	99	708079	28.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	6.999	67	441530	29.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.193	132	589392	29.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.358	113	557442	28.82	ng/ul	0.00
19) Nitrobenzene-d5	8.805	128	274180	30.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.522	143	300220	30.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.052	165	538894	28.59	ng/ul	0.00
29) 4-Chloroaniline-d4	10.569	131	682918	30.73	ng/ul	0.00
44) Dimethylphthalate-d6	13.710	166	1608143	29.49	ng/ul	0.00
47) Acenaphthylene-d8	13.987	160	2008307	30.85	ng/ul	0.00
52) 4-Nitrophenol-d4	14.493	143	224572	22.36	ng/ul	0.00
58) Fluorene-d10	15.293	176	1347901	28.32	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.410	200	195080	22.39	ng/ul	0.00
71) Anthracene-d10	17.140	188	1973948	29.82	ng/ul	0.00
79) Pyrene-d10	19.439	212	2133177	30.15	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.304	264	2380702	30.79	ng/ul	0.00
Target Compounds						Qvalue
6) Phenol	6.858	94	27538	1.08	ng/ul	99
45) Dimethylphthalate	13.751	163	406963	7.24	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100520\
Data File : BN012075.D
Acq On : 06 Oct 2020 03:13
Operator : CG/JU
Sample : L4184-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AM5

Quant Time: Oct 06 04:07:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 06 00:53:35 2020
Response via : Initial Calibration

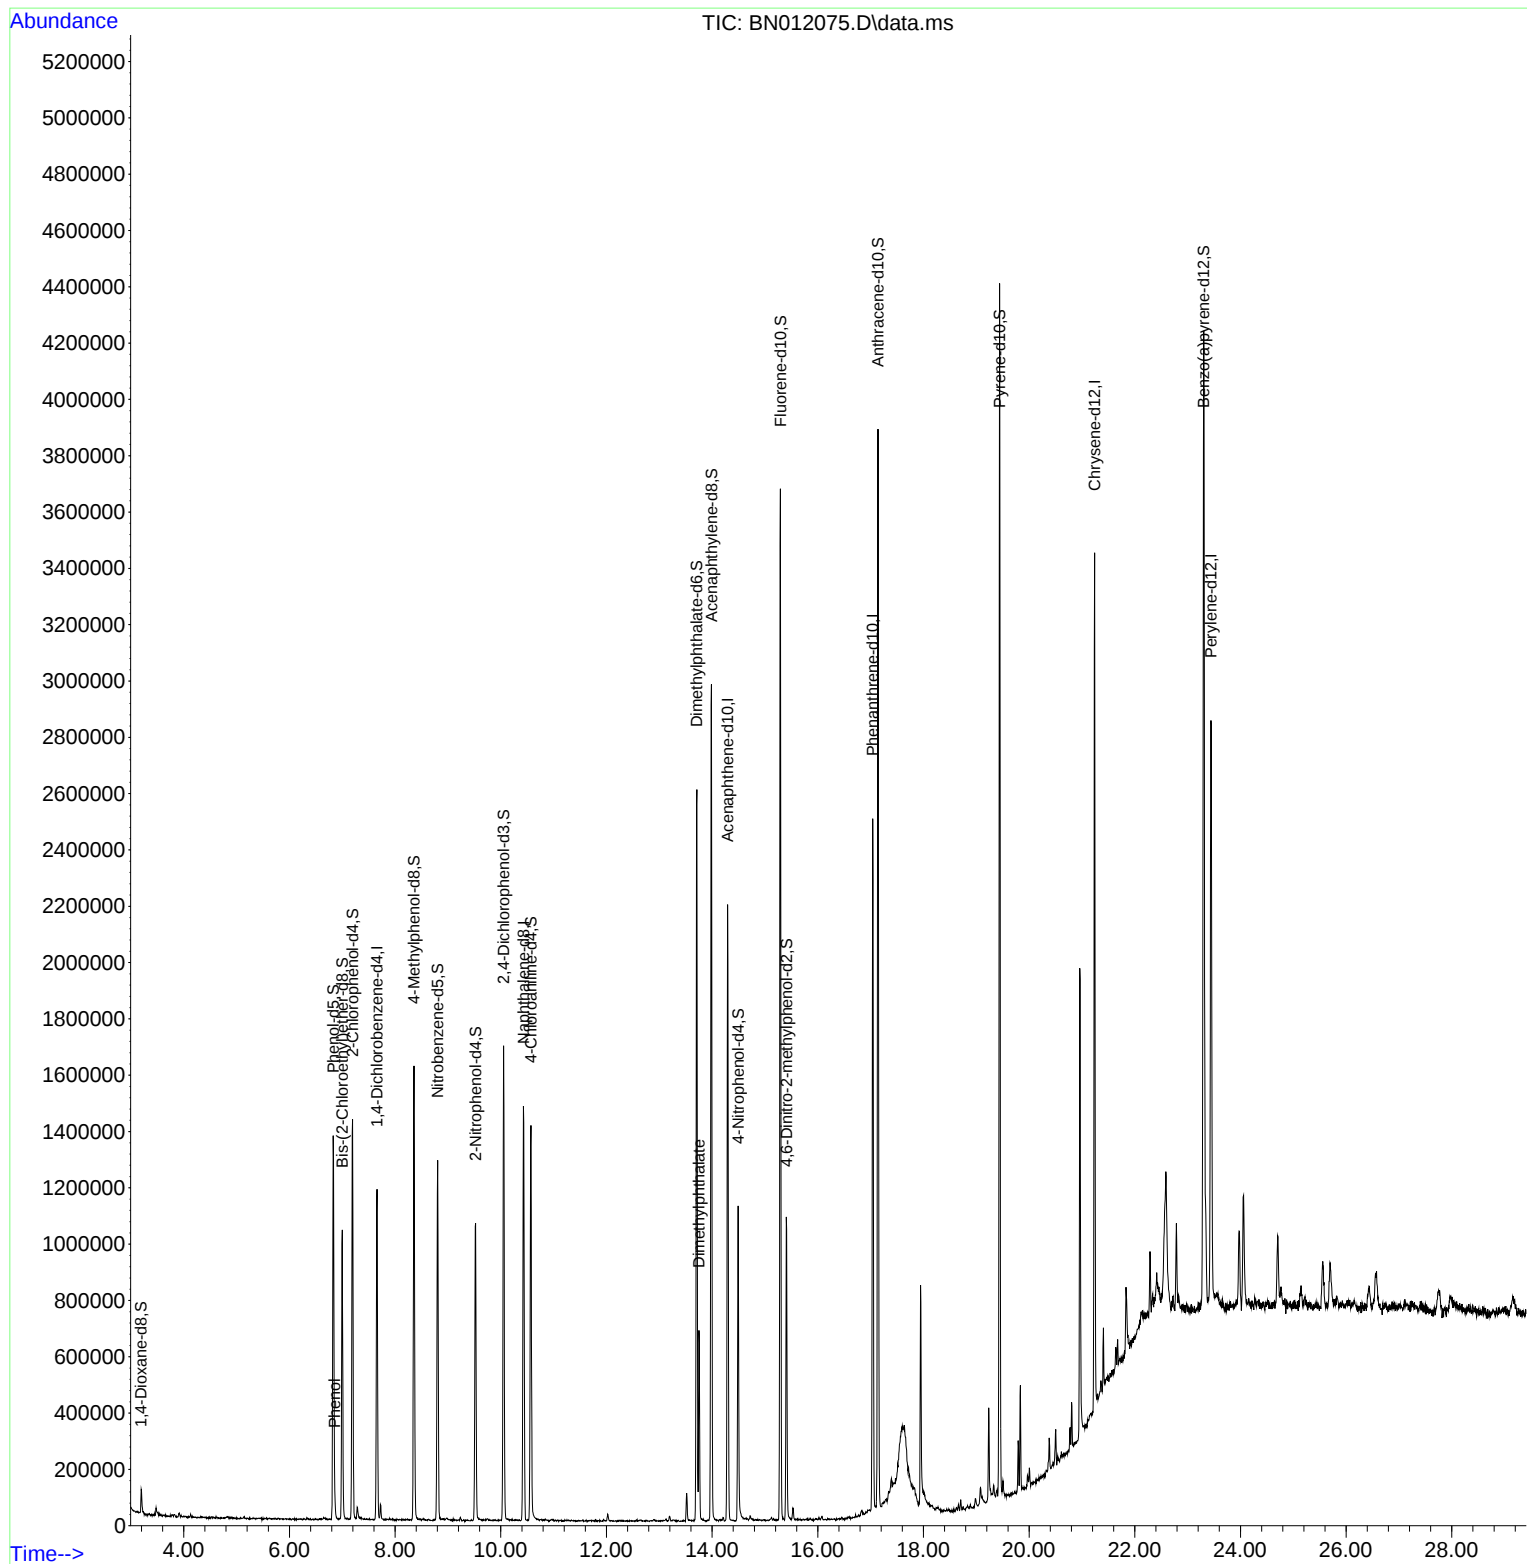




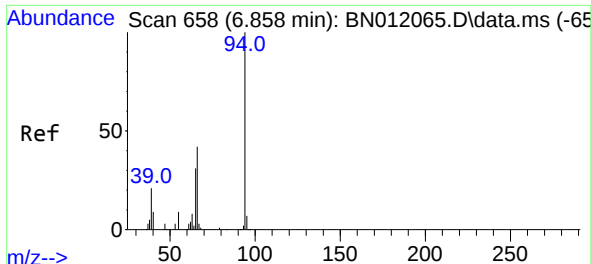


#6
Phenol
Concen: 1.08 ng/ul
RT: 6.858 min Scan# 658
Delta R.T. 0.000 min
Lab File: BN012075.D
Acq: 06 Oct 2020 03:13

Instrument :
BNA_N
ClientSampleId :
C0AM5

Tgt Ion: 94 Resp: 27538

Ion	Ratio	Lower	Upper
94	100		
65	33.0	26.8	40.2
66	47.9	37.9	56.9

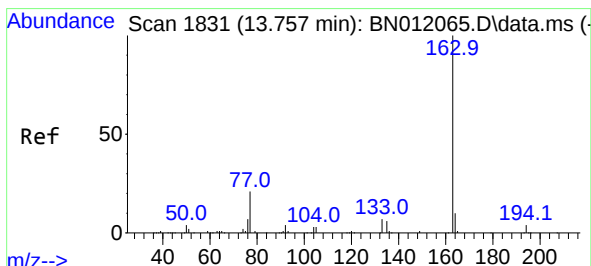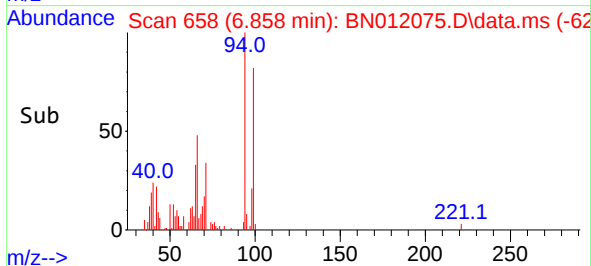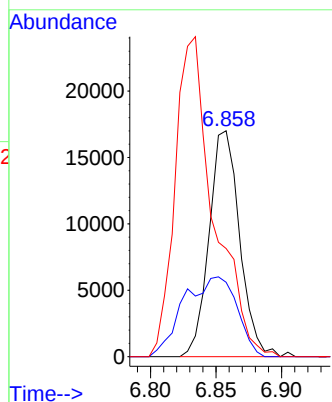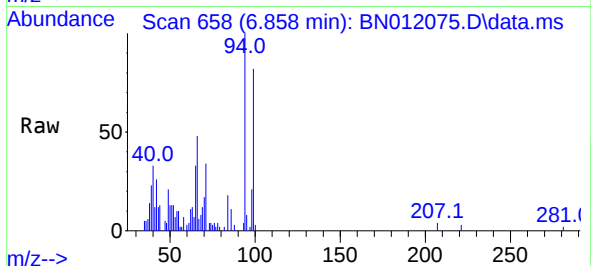

#45
Dimethylphthalate
Concen: 7.24 ng/ul
RT: 13.751 min Scan# 1830
Delta R.T. -0.006 min
Lab File: BN012075.D
Acq: 06 Oct 2020 03:13

Tgt Ion: 163 Resp: 406963

Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.4	5.0
164	10.4	7.8	11.8

