

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100520\
 Data File : BN012076.D
 Acq On : 06 Oct 2020 03:50
 Operator : CG/JU
 Sample : L4184-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AN7

Quant Time: Oct 06 05:17:21 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 06 00:53:35 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.658	152	284400	20.00	ng/ul	0.00
18) Naphthalene-d8	10.428	136	1156019	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.293	164	702320	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.039	188	1443412	20.00	ng/ul	0.00
78) Chrysene-d12	21.239	240	1401463	20.00	ng/ul	0.00
86) Perylene-d12	23.445	264	1504441	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	47321	7.24	ng/uL	0.00
5) Phenol-d5	6.828	99	769323	32.41	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	6.999	67	496885	34.07	ng/ul	0.00
9) 2-Chlorophenol-d4	7.193	132	668216	34.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.358	113	627220	33.57	ng/ul	0.00
19) Nitrobenzene-d5	8.805	128	317190	34.56	ng/ul	0.00
22) 2-Nitrophenol-d4	9.516	143	358246	36.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.052	165	620972	32.62	ng/ul	0.00
29) 4-Chloroaniline-d4	10.569	131	835968	37.25	ng/ul	0.00
44) Dimethylphthalate-d6	13.710	166	1911742	34.70	ng/ul	0.00
47) Acenaphthylene-d8	13.987	160	2357133	35.85	ng/ul	0.00
52) 4-Nitrophenol-d4	14.493	143	265464	26.17	ng/ul	0.00
58) Fluorene-d10	15.292	176	1608574	33.46	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.410	200	243040	26.38	ng/ul	0.00
71) Anthracene-d10	17.139	188	2424122	34.63	ng/ul	0.00
79) Pyrene-d10	19.439	212	2639055	35.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.304	264	2834424	33.57	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.751	163	319441	5.63	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100520\
Data File : BN012076.D
Acq On : 06 Oct 2020 03:50
Operator : CG/JU
Sample : L4184-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN7


Quant Time: Oct 06 05:17:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 06 00:53:35 2020
Response via : Initial Calibration

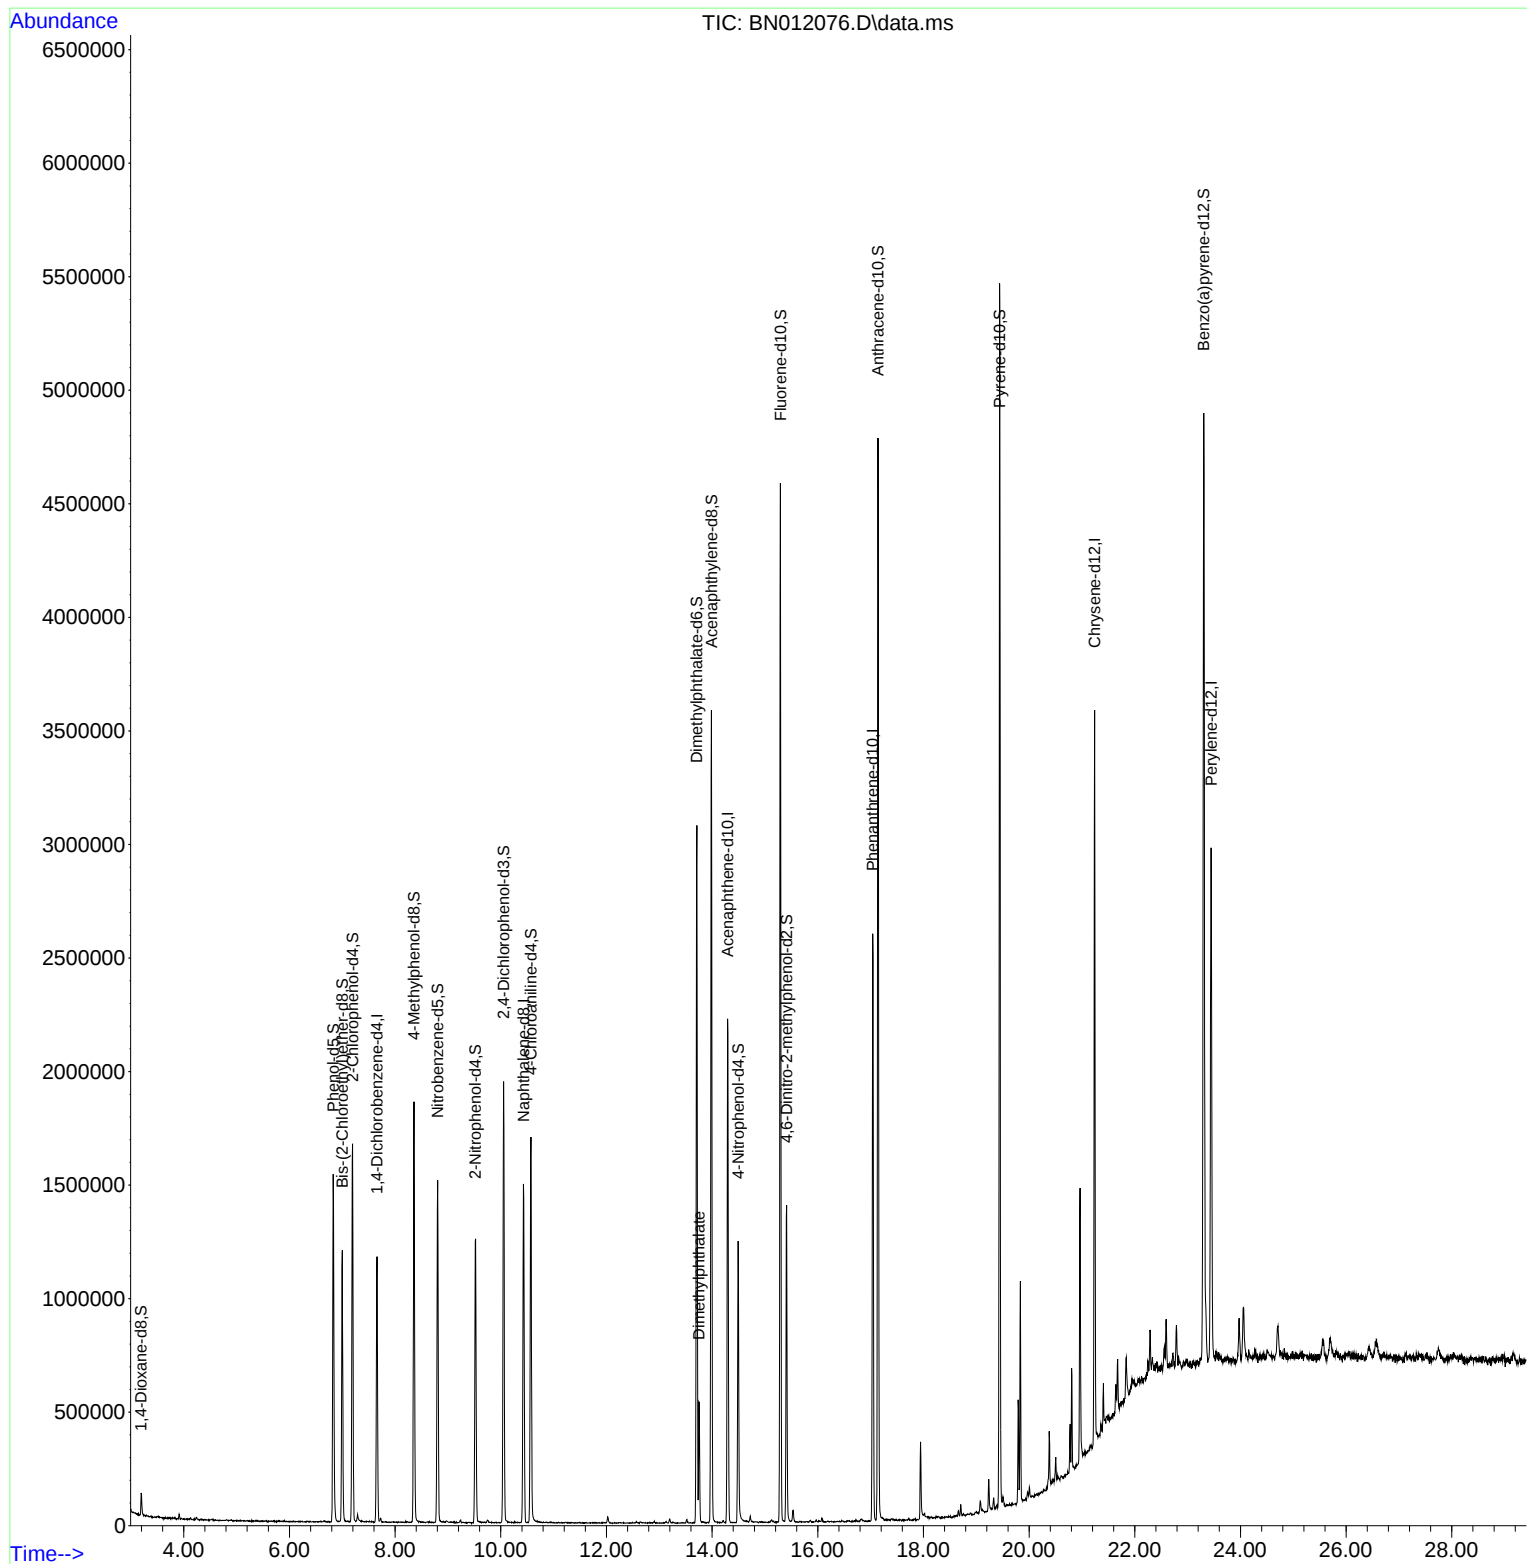

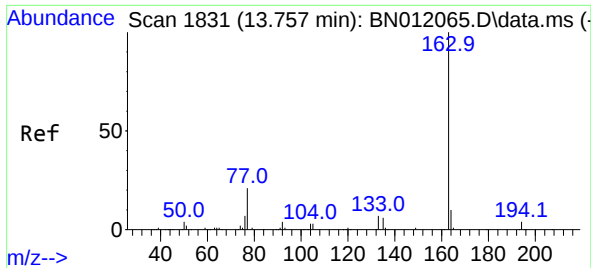

#45
Dimethylphthalate
Concen: 5.63 ng/ul
RT: 13.751 min Scan# 1830
Delta R.T. -0.006 min
Lab File: BN012076.D
Acq: 06 Oct 2020 03:50

Instrument :
BNA_N
ClientSampleId :
C0AN7

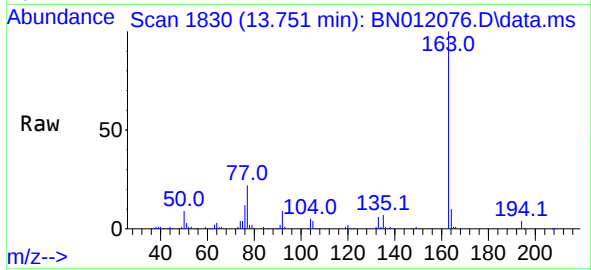

Tgt Ion:163 Resp: 319441
Ion Ratio Lower Upper
163 100
194 3.6 3.4 5.0
164 9.6 7.8 11.8

