

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100520\
 Data File : BN012078.D
 Acq On : 06 Oct 2020 05:02
 Operator : CG/JU
 Sample : L4184-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AK0

Quant Time: Oct 06 06:25:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 06 00:53:35 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.658	152	293456	20.00	ng/ul	0.00
18) Naphthalene-d8	10.428	136	1183972	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.293	164	741293	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.040	188	1525222	20.00	ng/ul	0.00
78) Chrysene-d12	21.239	240	1503244	20.00	ng/ul	0.00
86) Perylene-d12	23.445	264	1702810	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	63008	9.34	ng/uL	0.00
5) Phenol-d5	6.828	99	1129648	46.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	6.999	67	692819	46.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.193	132	927661	46.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.358	113	918051	47.62	ng/ul	0.00
19) Nitrobenzene-d5	8.805	128	445799	47.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.516	143	497988	48.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.052	165	885634	45.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.569	131	1178935	51.29	ng/ul	0.00
44) Dimethylphthalate-d6	13.710	166	2710808	46.62	ng/ul	0.00
47) Acenaphthylene-d8	13.987	160	3352885	48.31	ng/ul	0.00
52) 4-Nitrophenol-d4	14.493	143	455219	42.51	ng/ul	0.00
58) Fluorene-d10	15.293	176	2285542	45.04	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.410	200	408206	41.93	ng/ul	0.00
71) Anthracene-d10	17.140	188	3444551	46.57	ng/ul	0.00
79) Pyrene-d10	19.439	212	3632304	45.94	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.310	264	4207821	44.03	ng/ul	0.00
Target Compounds						Qvalue
6) Phenol	6.852	94	43455	1.71	ng/ul	97
45) Dimethylphthalate	13.757	163	1332695	22.24	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100520\
Data File : BN012078.D
Acq On : 06 Oct 2020 05:02
Operator : CG/JU
Sample : L4184-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK0

Quant Time: Oct 06 06:25:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 06 00:53:35 2020
Response via : Initial Calibration




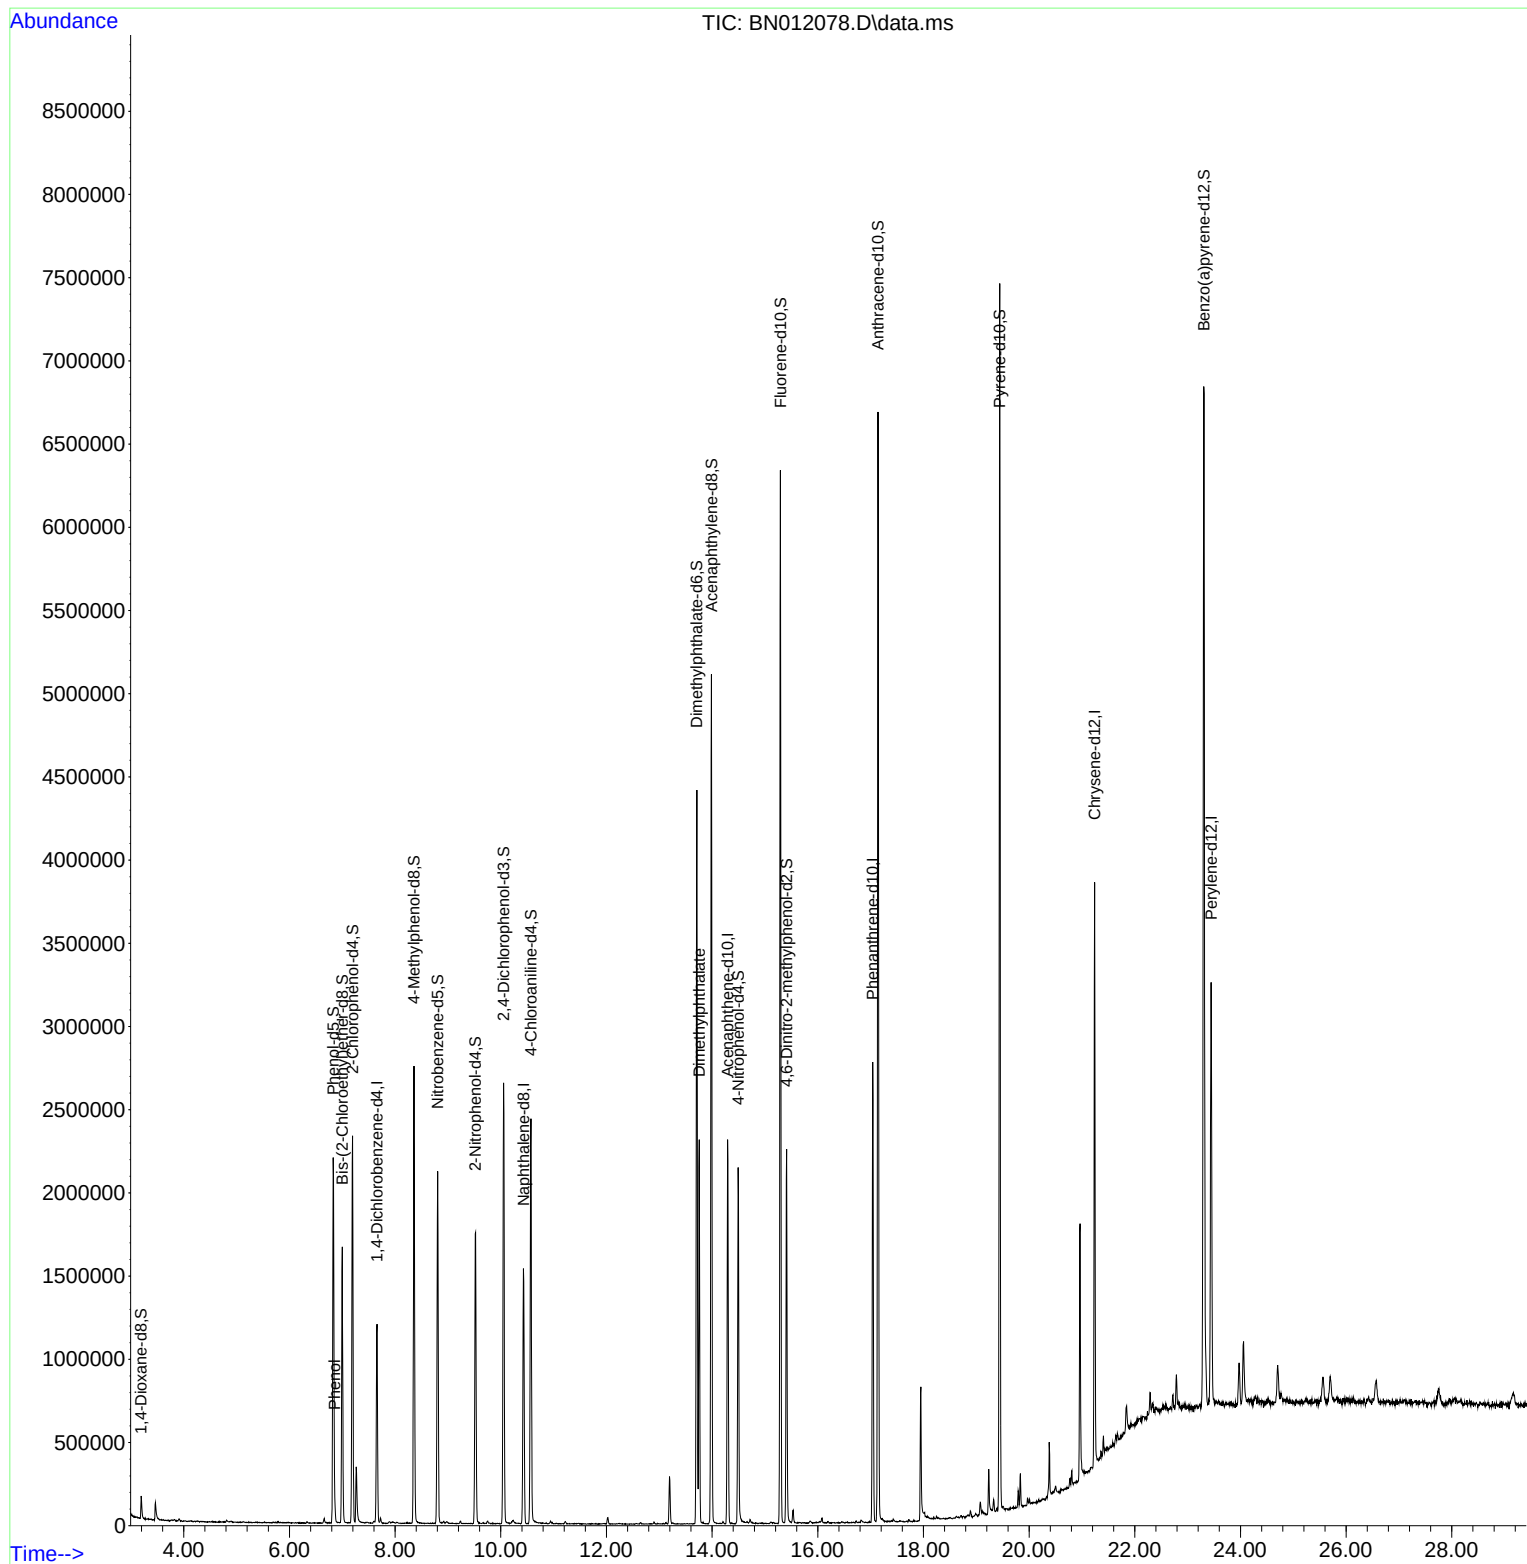


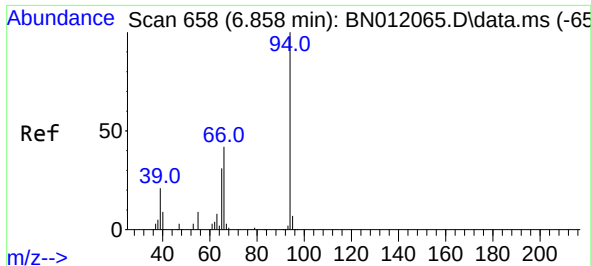

#6
Phenol
Concen: 1.71 ng/ul
RT: 6.852 min Scan# 657
Delta R.T. -0.006 min
Lab File: BN012078.D
Acq: 06 Oct 2020 05:02

Instrument :
BNA_N
ClientSampleId :
C0AK0

Tgt Ion: 94 Resp: 43455
Ion Ratio Lower Upper
94 100
65 32.5 26.8 40.2
66 50.0 37.9 56.9

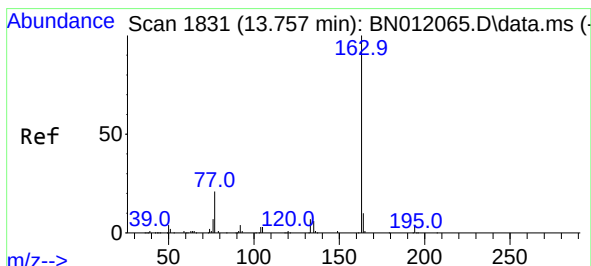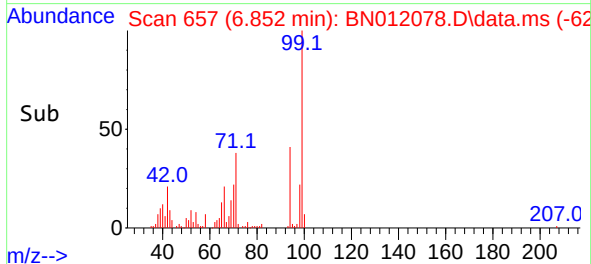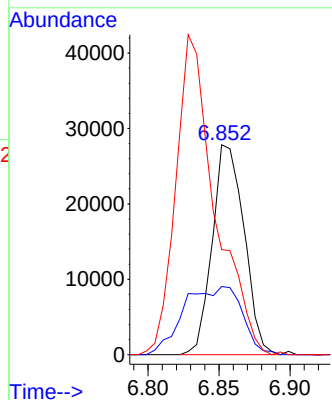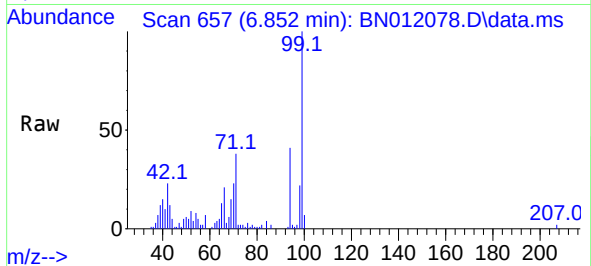

#45
Dimethylphthalate
Concen: 22.24 ng/ul
RT: 13.757 min Scan# 1831
Delta R.T. 0.000 min
Lab File: BN012078.D
Acq: 06 Oct 2020 05:02

Tgt Ion:163 Resp: 1332695
Ion Ratio Lower Upper
163 100
194 4.1 3.4 5.0
164 9.5 7.8 11.8

