

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100520\
 Data File : BN012082.D
 Acq On : 06 Oct 2020 09:12
 Operator : CG/JU
 Sample : L4151-14
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB7L5

Quant Time: Oct 06 11:05:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 16:22:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	356779	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.42	136	1406846	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.29	164	802717	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	1627747	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	1625616	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	1737757	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	32837	4.01	ng/uL	0.00
5) Phenol-d5	6.82	99	501760	16.85	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	6.99	67	347328	18.99	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.18	132	415990	17.28	ng/ul	-0.01
13) 4-Methylphenol-d8	8.35	113	418383	17.85	ng/ul	-0.02
19) Nitrobenzene-d5	8.79	128	206431	18.48	ng/ul	-0.02
22) 2-Nitrophenol-d4	9.51	143	225273	18.65	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.05	165	390700	16.86	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.56	131	379762	13.90	ng/ul	-0.01
44) Dimethylphthalate-d6	13.70	166	1275779	20.26	ng/ul	-0.01
47) Acenaphthylene-d8	13.98	160	1376880	18.32	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.49	143	160531	13.84	ng/ul	-0.01
58) Fluorene-d10	15.29	176	1018214	18.53	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.40	200	149611	14.40	ng/ul	-0.01
71) Anthracene-d10	17.14	188	1404572	17.79	ng/ul	0.00
79) Pyrene-d10	19.44	212	1491706	17.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	1600489	16.41	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.75	163	159068	2.452	ng/ul 97




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100520\
Data File : BN012082.D
Acq On : 06 Oct 2020 09:12
Operator : CG/JU
Sample : L4151-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB7L5

Quant Time: Oct 06 11:05:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 16:22:43 2020
Response via : Initial Calibration

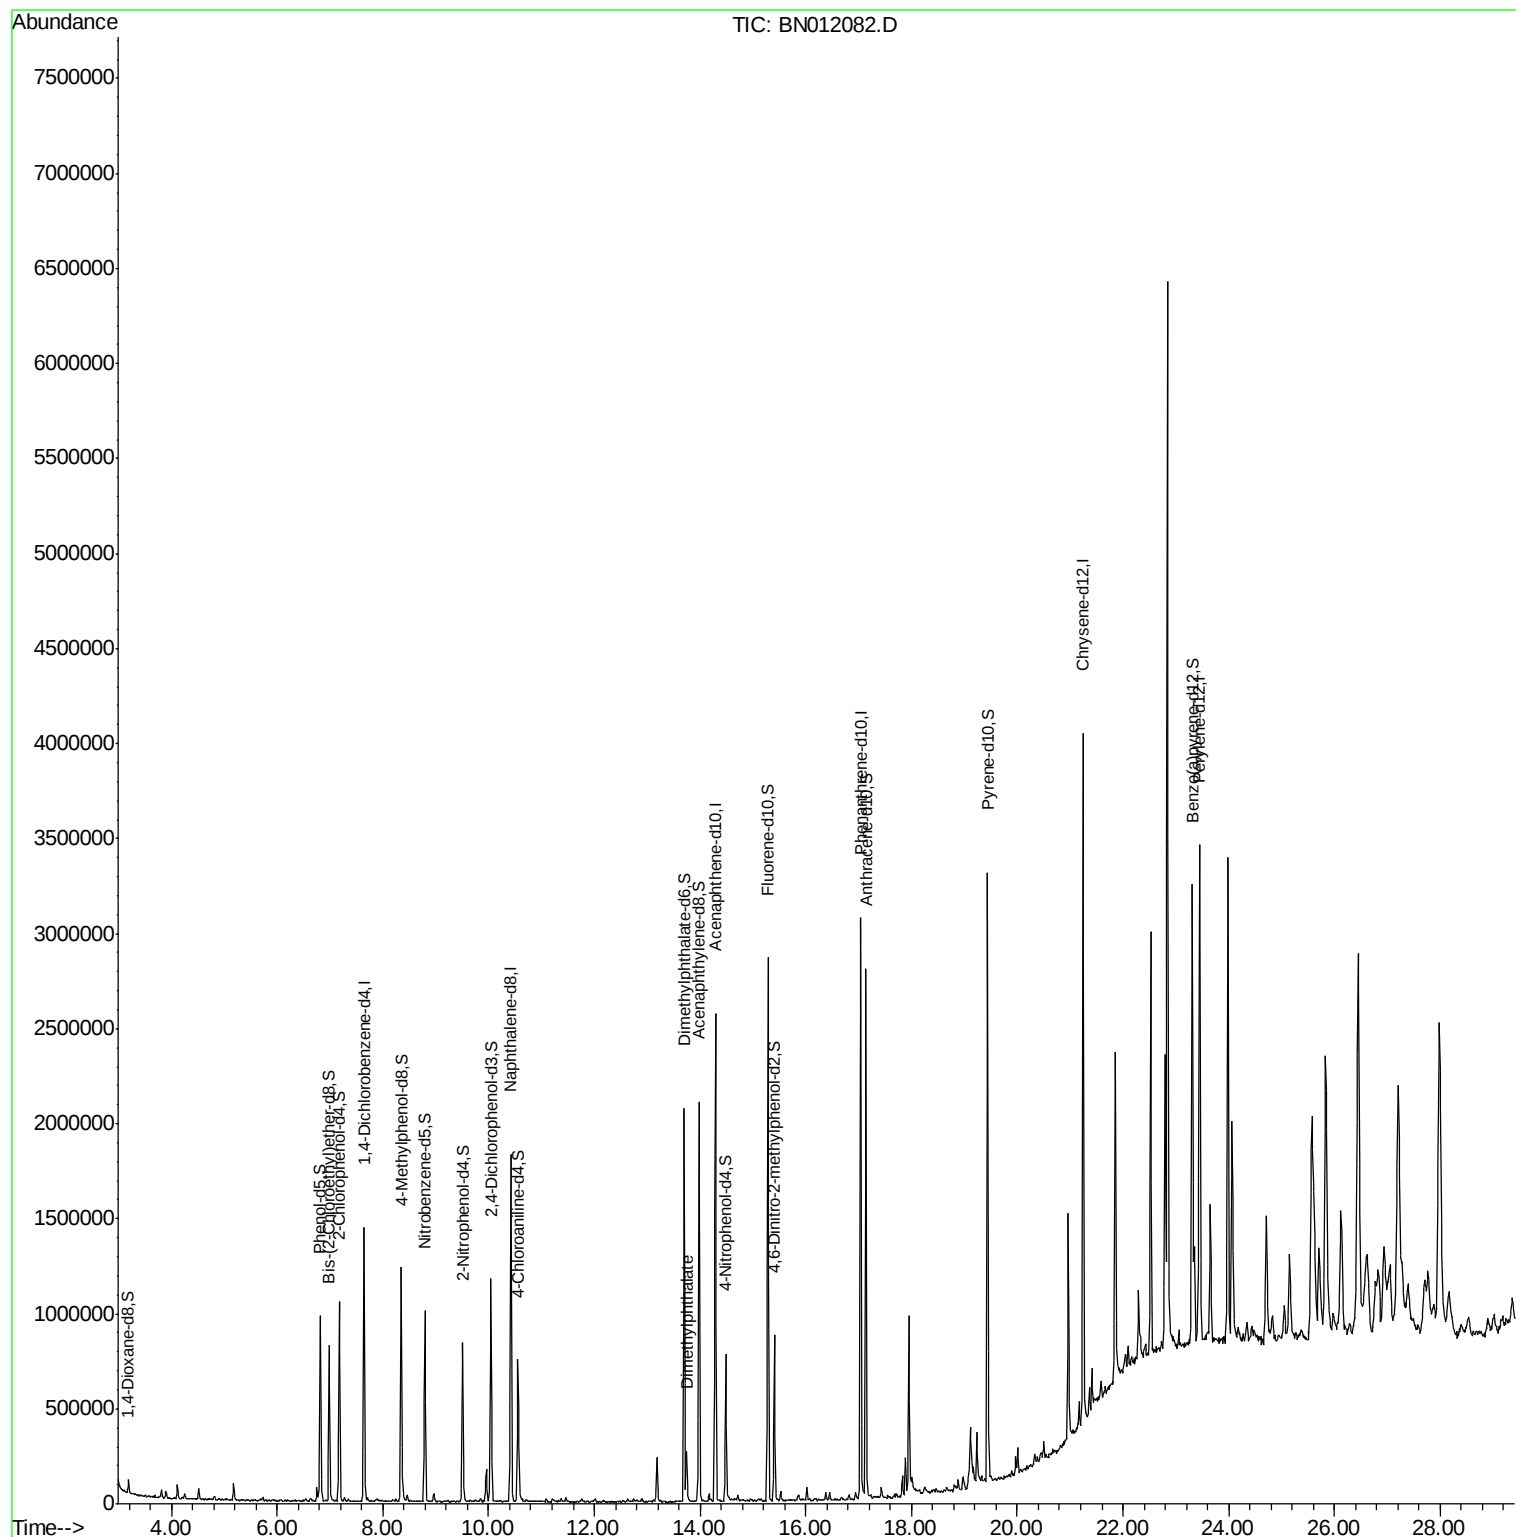

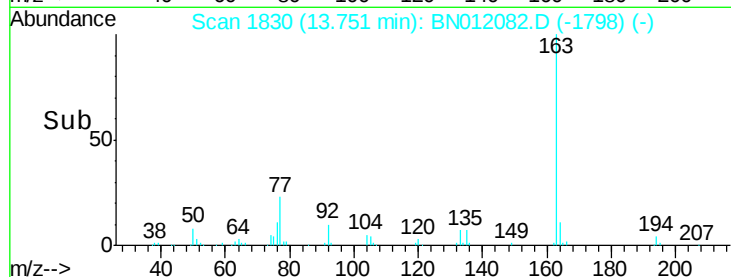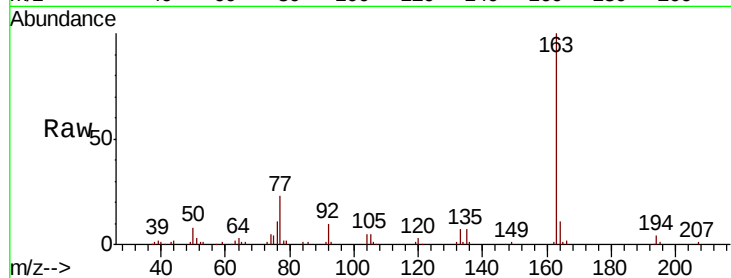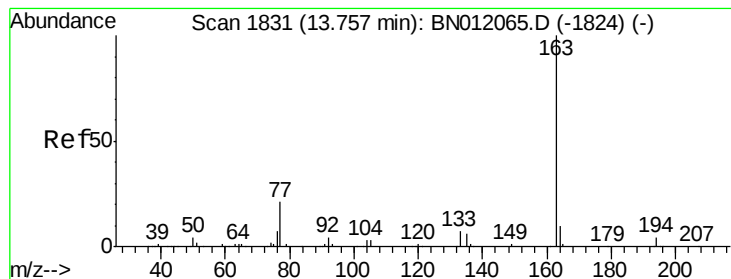

#45

Dimethylphthalate

Concen: 2.452 ng/ul

RT: 13.75 min Scan# 1830

Delta R.T. -0.01 min

Lab File: BN012082.D

Acq: 06 Oct 2020 09:12

Instrument :

BNA_N

ClientSampleId :

CB7L5

Tot Ion:163 Resp: 159068

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 11.1 7.8 11.8

