
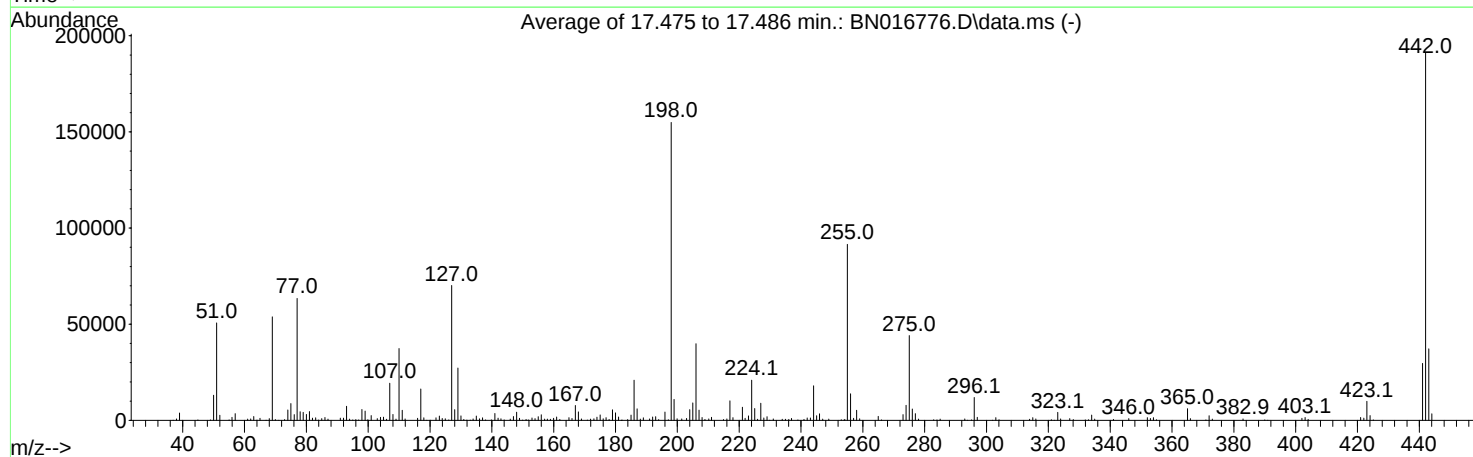


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100621\
 Data File : BN016776.D
 Acq On : 06 Oct 2021 13:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 06 14:22:07 2021

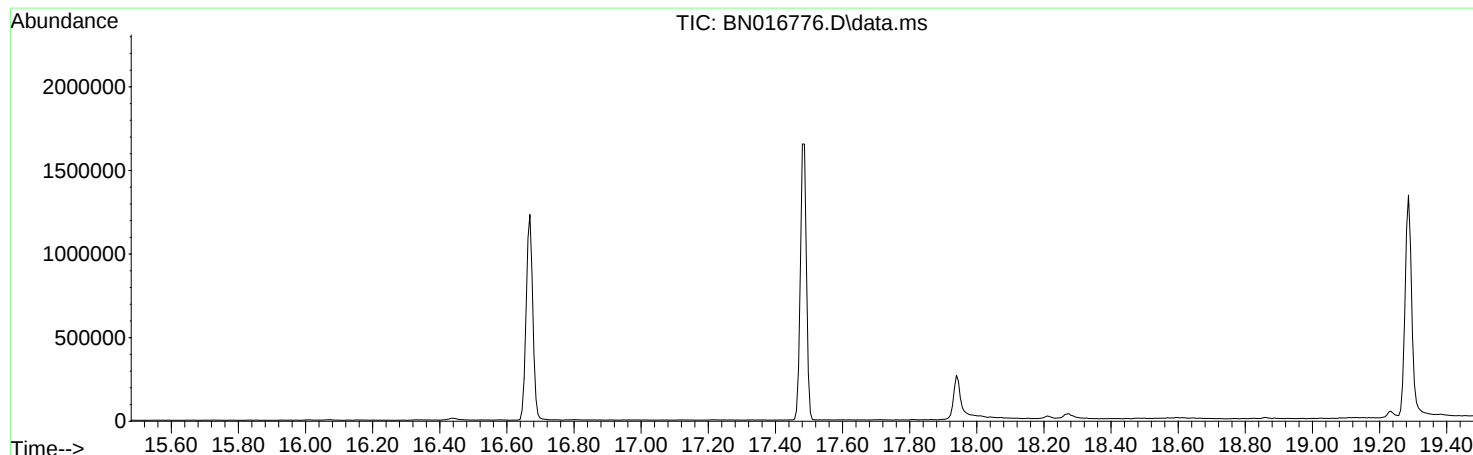

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	50653	PASS
68	69	0.00	2	1.8	943	PASS
69	198	0.00	100	34.8	53872	PASS
70	69	0.00	2	0.8	409	PASS
127	198	10	80	45.3	70144	PASS
197	198	0.00	2	0.2	359	PASS
198	198	100	100	100.0	154981	PASS
199	198	5	9	7.1	10951	PASS
275	198	10	60	28.4	44085	PASS
365	198	1	100	3.9	6057	PASS
441	198	0.01	100	19.1	29667	PASS
442	442	50	100	100.0	191299	PASS
443	442	15	24	19.5	37229	PASS

Instrument :
BNA_N
ClientSampleId :
DFTPP

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/6/2021	BNA_N	<u>BN016776.D</u>
Compound Name	Response	Retention Time
DDT	549422	20.53
DDD	6344	20.09
DDE	0	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6344	555766	1.14

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100621\
 Data File : BN016776.D
 Acq On : 06 Oct 2021 13:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 06 14:05:07 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 30 18:14:09 2021
 Response via : Initial Calibration

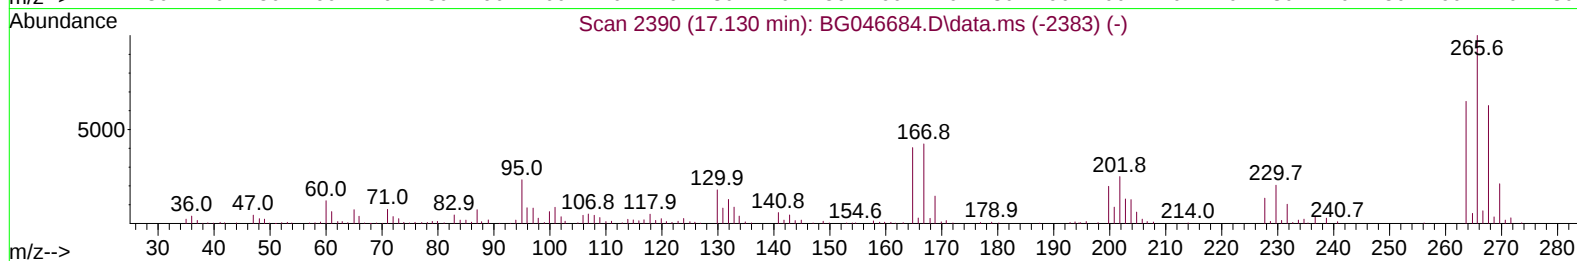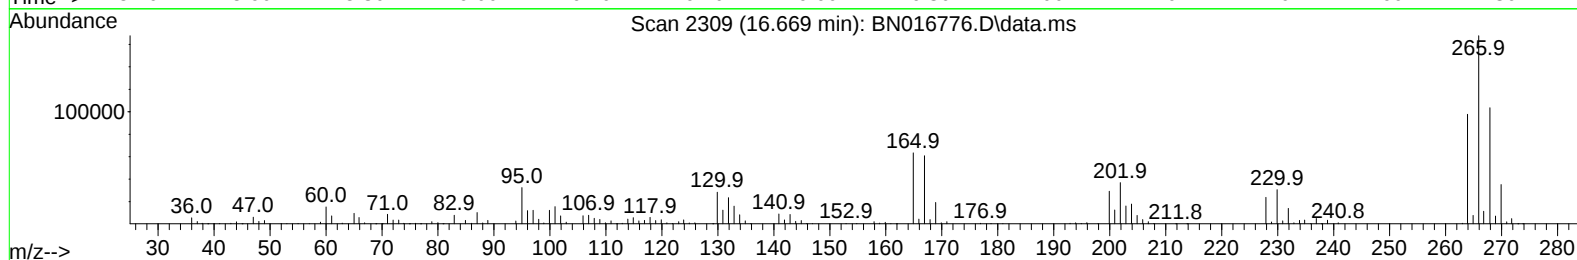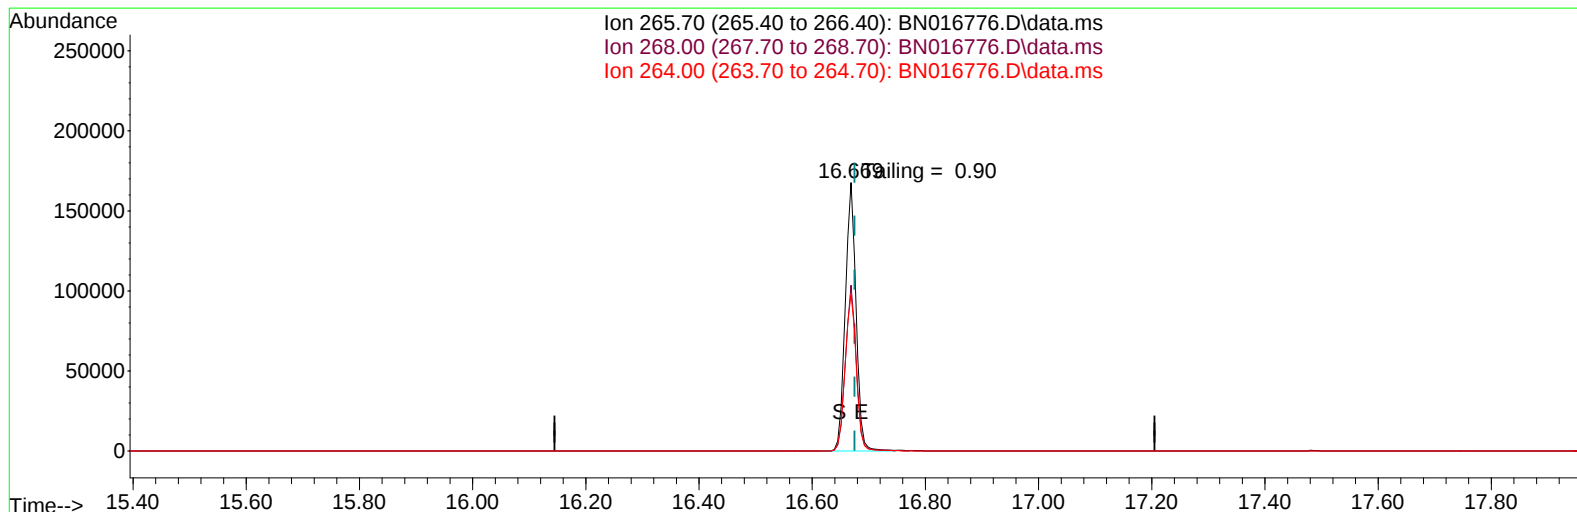

TIC: BN016776.D\data.ms

(70) Pentachlorophenol (C)

16.669min (-0.006) 33350.36 ng




response 221943

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.75
264.00	61.60	58.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100621\
Data File : BN016776.D
Acq On : 06 Oct 2021 13:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 06 14:05:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

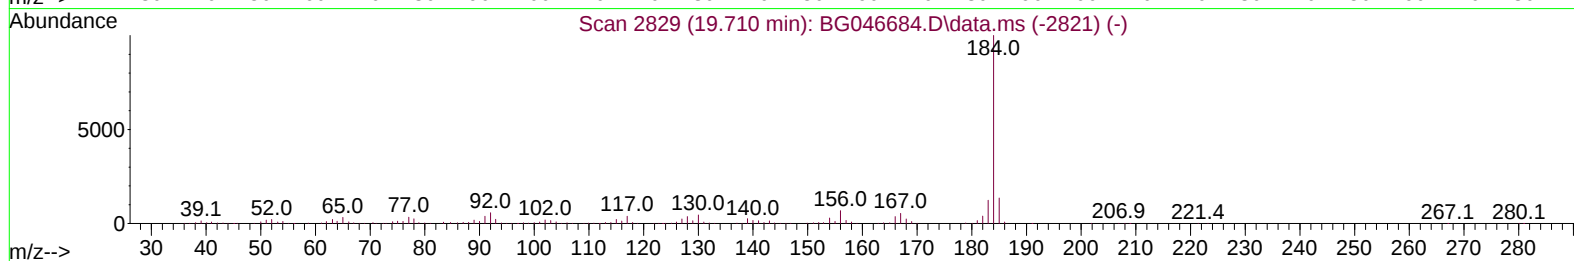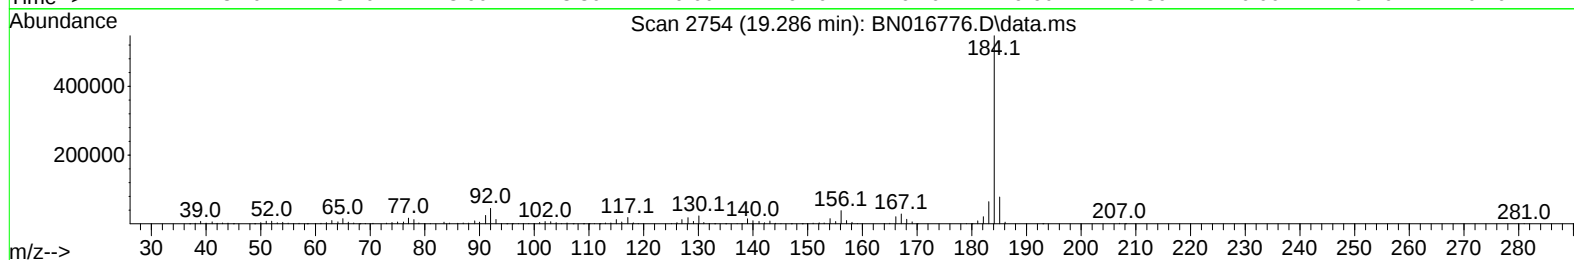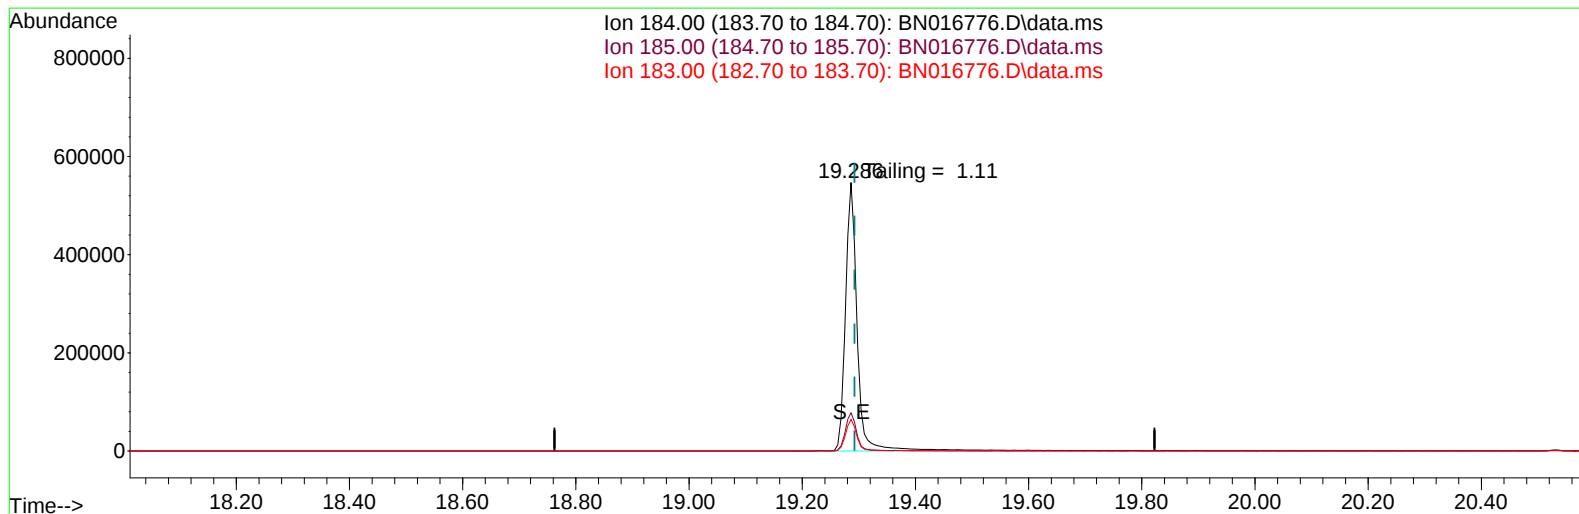

TIC: BN016776.D\data.ms

(77) Benzidine

19.286min (-0.006) 0.00 ng

response 777690

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.26
183.00	13.20	11.83
0.00	0.00	0.00