
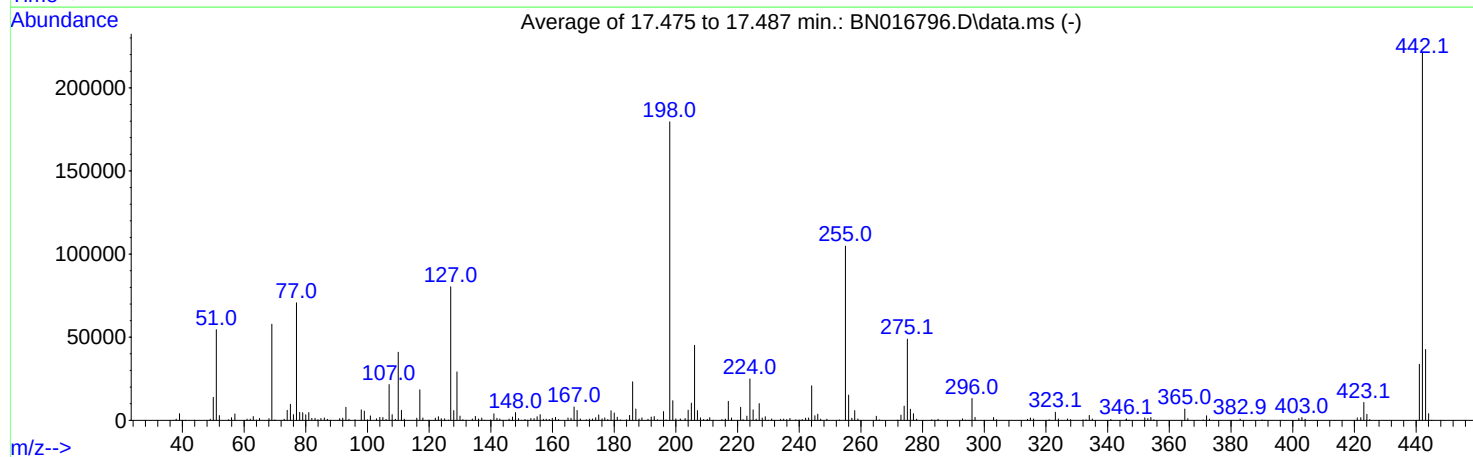


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100621\
 Data File : BN016796.D
 Acq On : 07 Oct 2021 01:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 06 14:22:07 2021

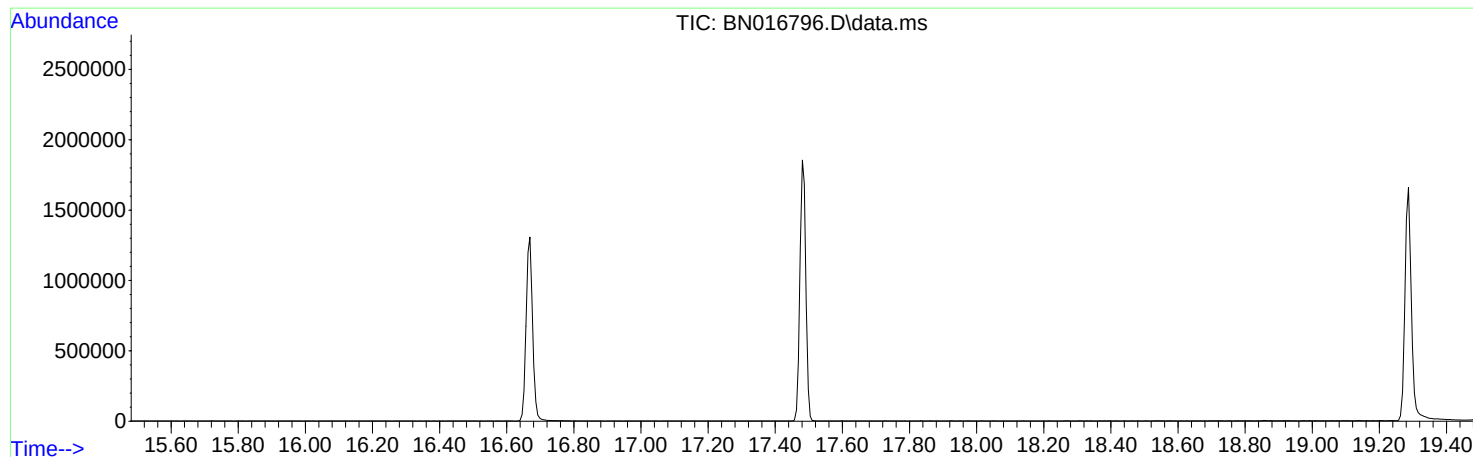




AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	54605	PASS
68	69	0.00	2	1.8	1027	PASS
69	198	0.00	100	32.2	57832	PASS
70	69	0.00	2	0.5	262	PASS
127	198	10	80	44.7	80336	PASS
197	198	0.00	2	0.2	294	PASS
198	198	100	100	100.0	179584	PASS
199	198	5	9	6.6	11864	PASS
275	198	10	60	27.2	48869	PASS
365	198	1	100	3.8	6798	PASS
441	198	0.01	100	18.8	33776	PASS
442	442	50	100	100.0	221245	PASS
443	442	15	24	19.3	42600	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100621\
 Data File : BN016796.D
 Acq On : 07 Oct 2021 01:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 07 04:05:46 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 30 18:14:09 2021
 Response via : Initial Calibration

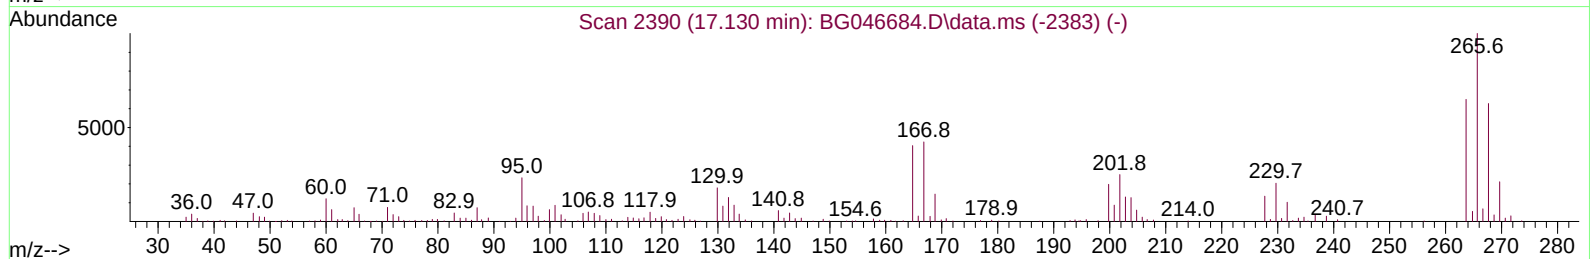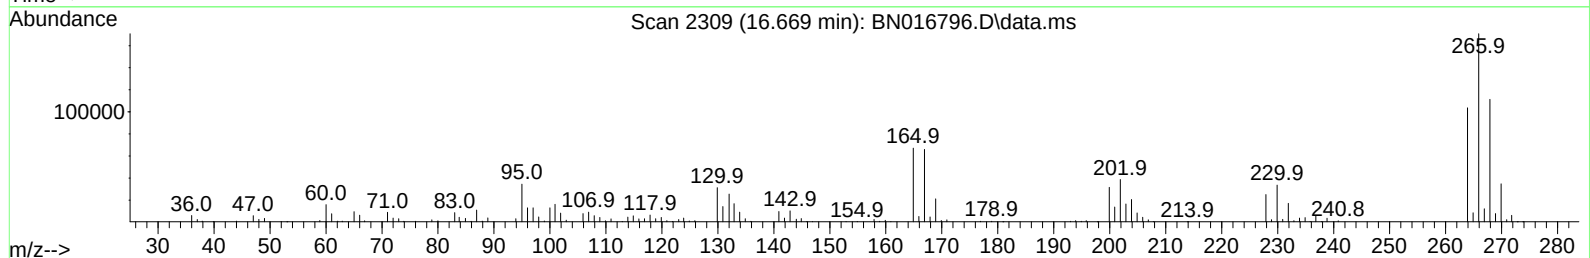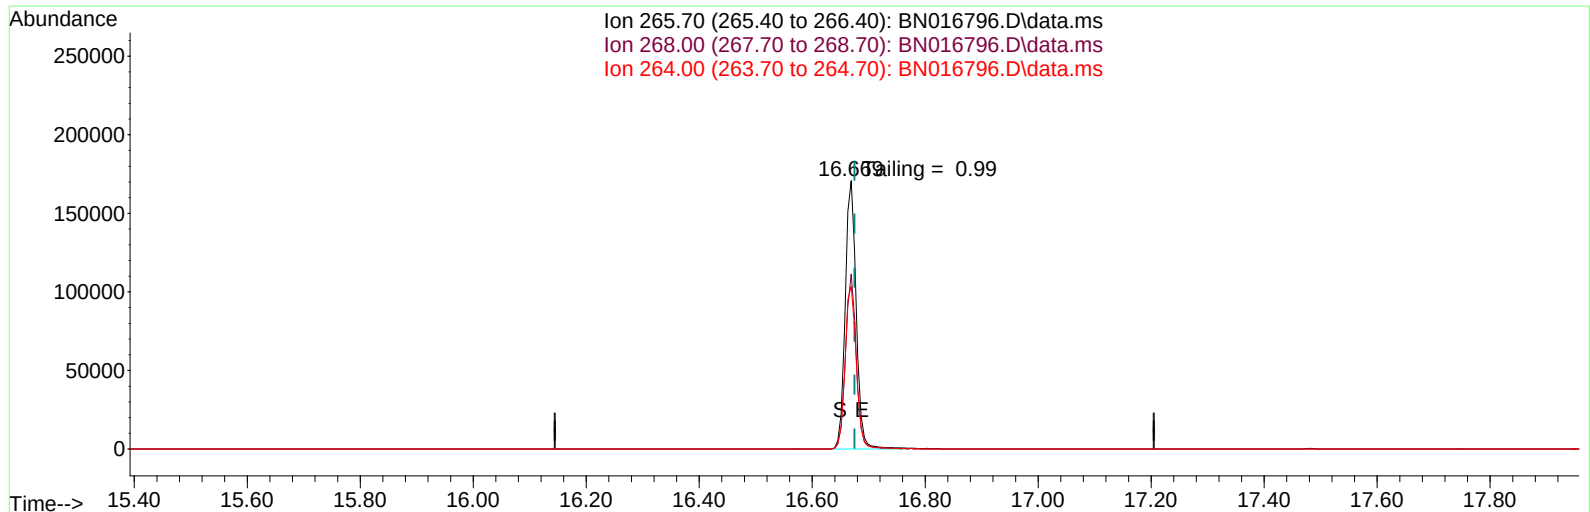

TIC: BN016796.D\data.ms

(70) Pentachlorophenol (C)

16.669min (-0.006) 29612.18 ng




response 231227

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.20
264.00	61.60	60.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100621\
 Data File : BN016796.D
 Acq On : 07 Oct 2021 01:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 07 04:05:46 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 30 18:14:09 2021
 Response via : Initial Calibration

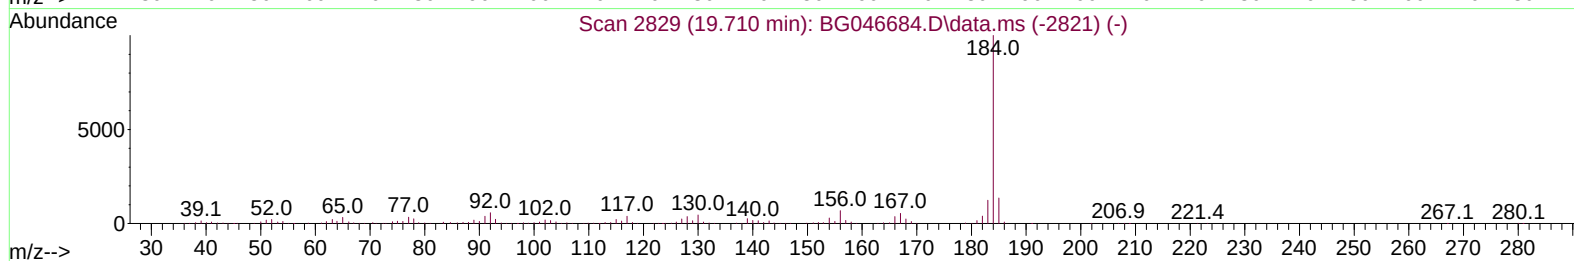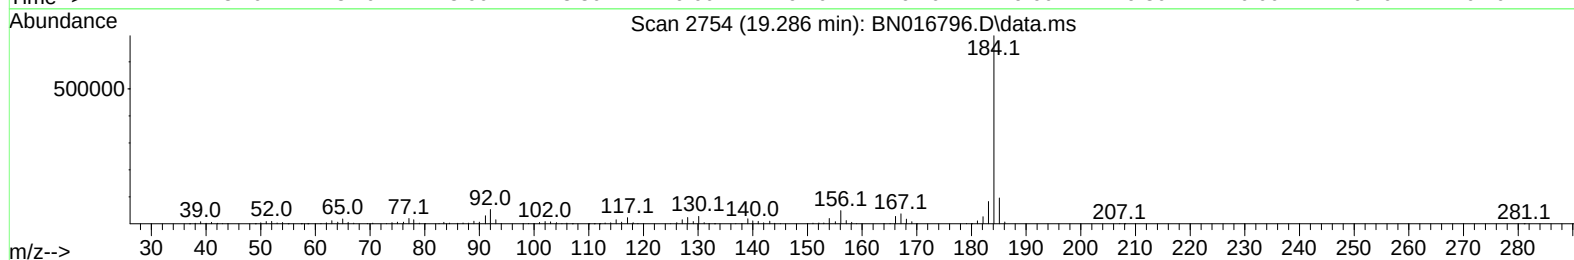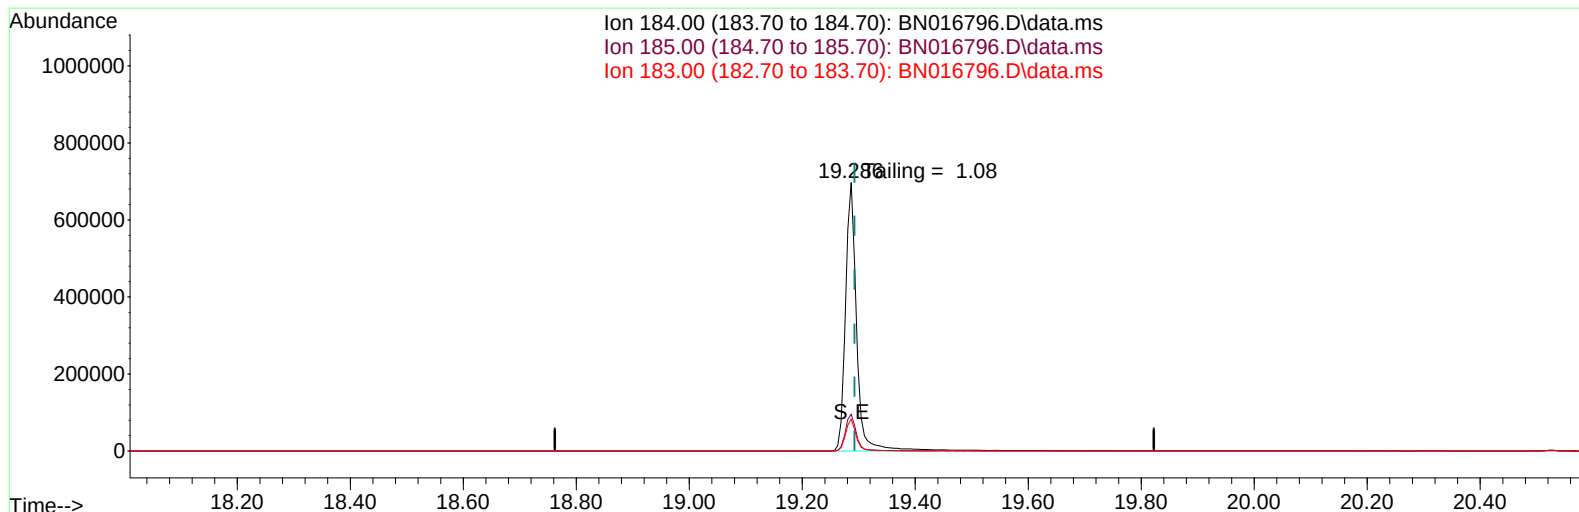

TIC: BN016796.D\data.ms

(77) Benzidine

19.286min (-0.006) 0.00 ng

response 951058

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.71
183.00	13.20	11.91
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
10/6/2021	BNA_N	<u>BN016796.D</u>
Compound Name	Response	Retention Time
DDT	619021	20.528
DDD	15317	20.086
DDE	0	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15317	634338	2.41

Instrument :
BNA_N
ClientSampleId :
DFTPP