
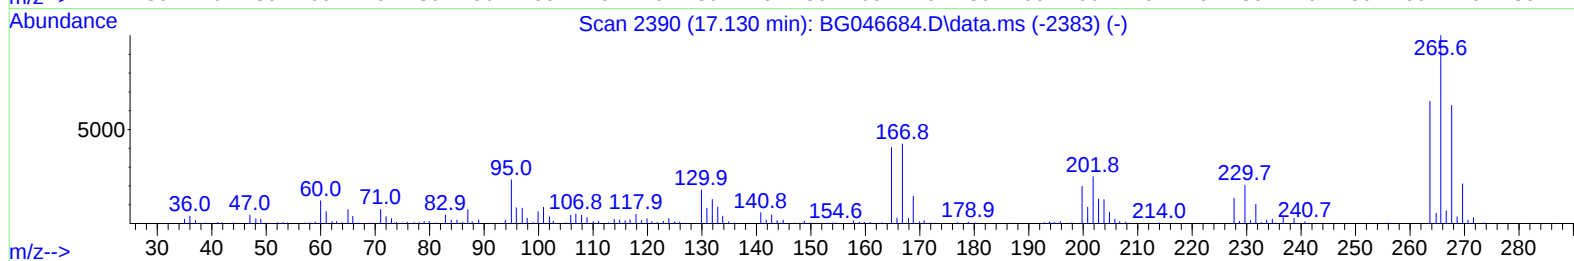
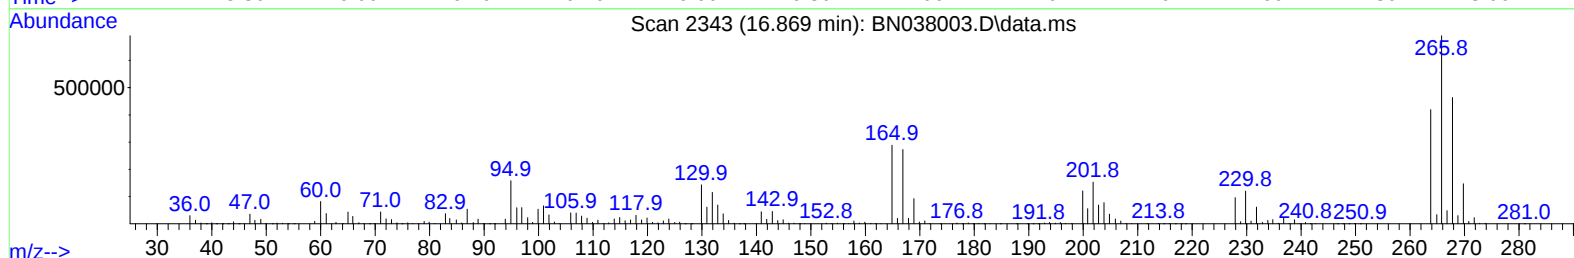


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100625\
Data File : BN038003.D
Acq On : 06 Oct 2025 10:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 11:09:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

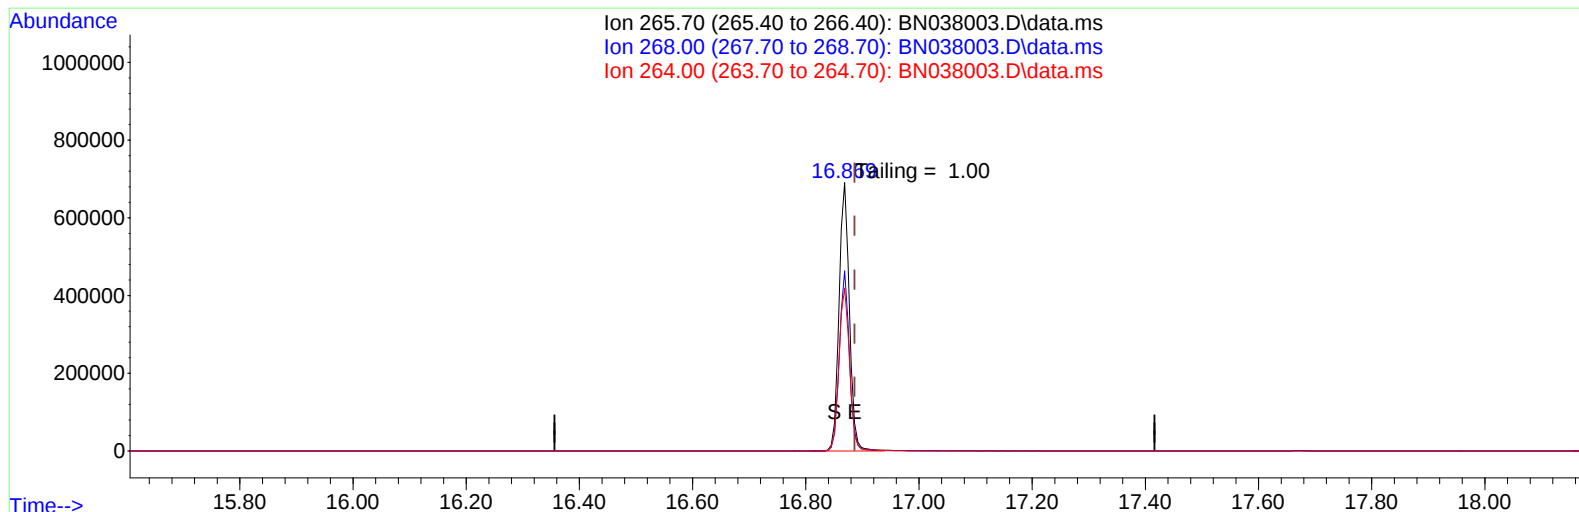

TIC: BN038003.D\data.ms

(70) Pentachlorophenol (C)




16.869min (-0.017) 28237.23 ng

response 876201

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.14
264.00	61.60	60.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100625\
Data File : BN038003.D
Acq On : 06 Oct 2025 10:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 11:09:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

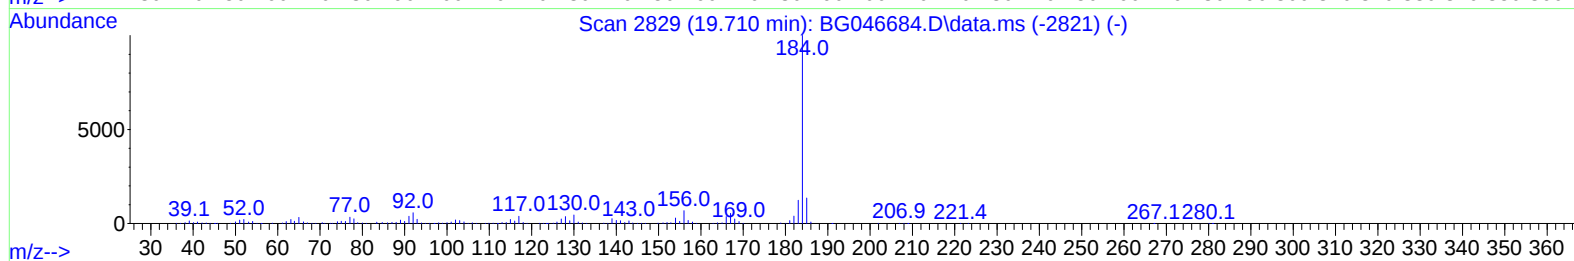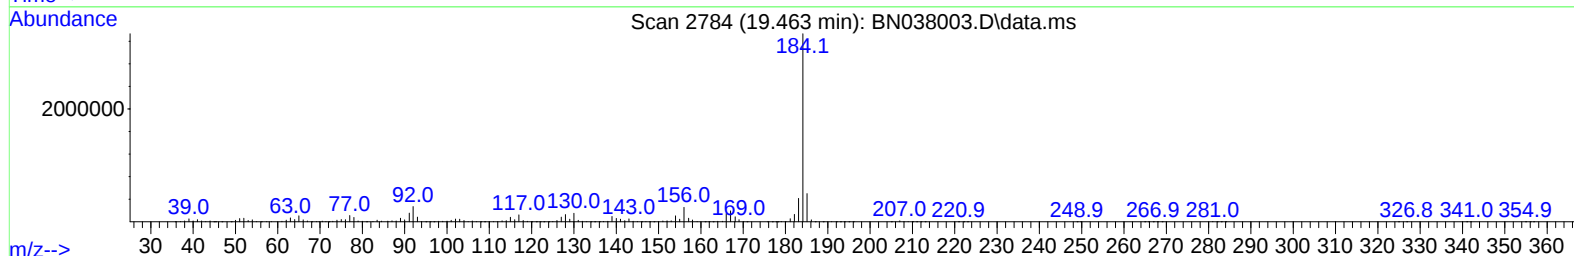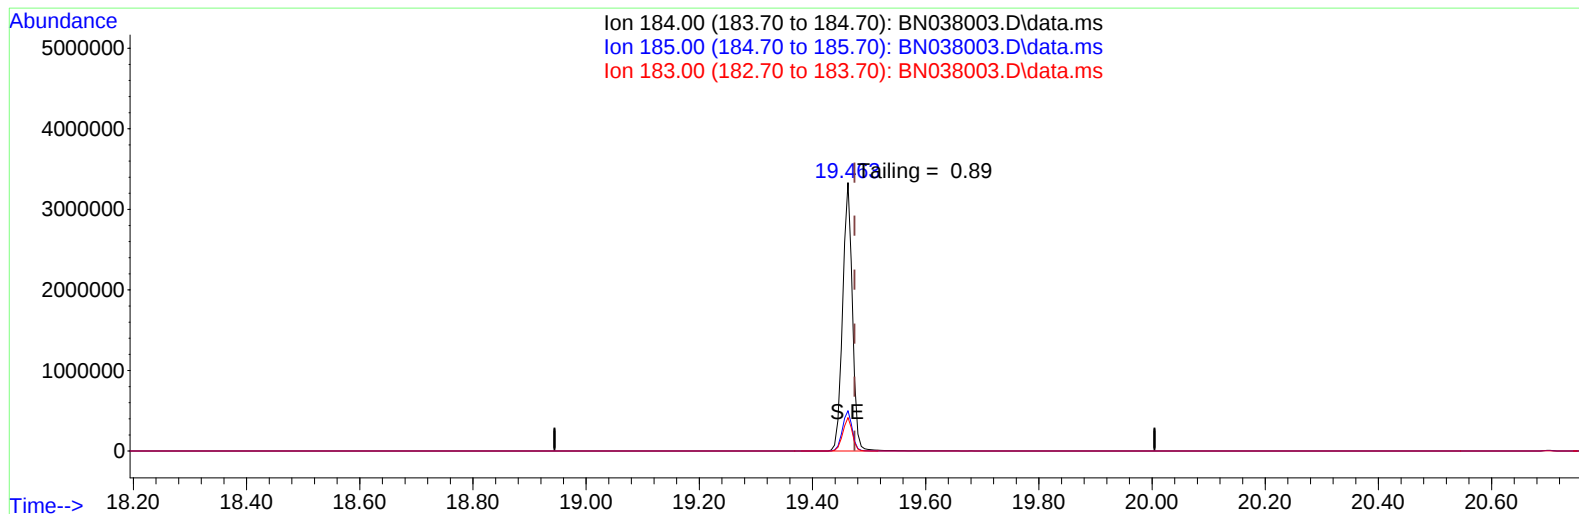

TIC: BN038003.D\data.ms

(77) Benzidine

19.463min (-0.012) 0.00 ng

response 4005964

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.03
183.00	13.20	12.47
0.00	0.00	0.00