
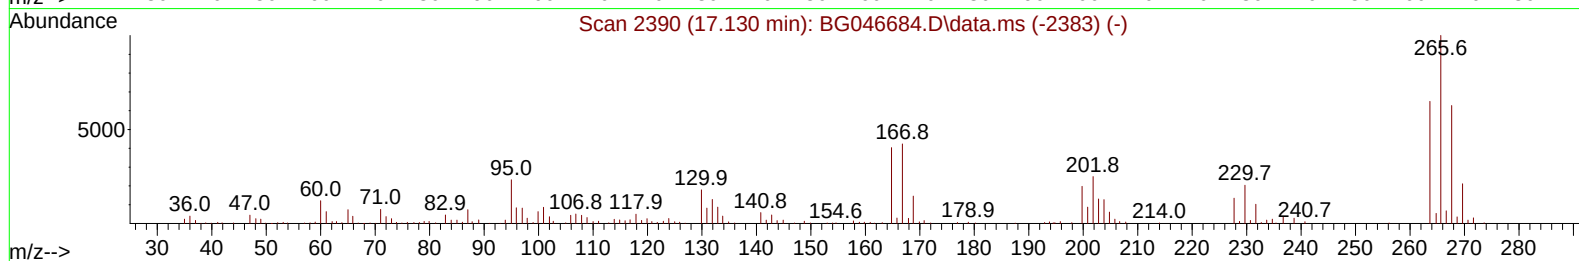
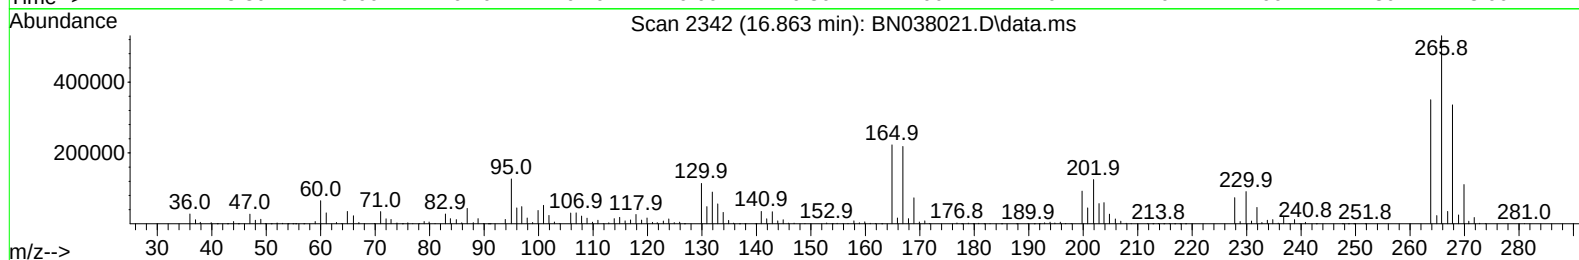


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100625\
Data File : BN038021.D
Acq On : 06 Oct 2025 22:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 01:36:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

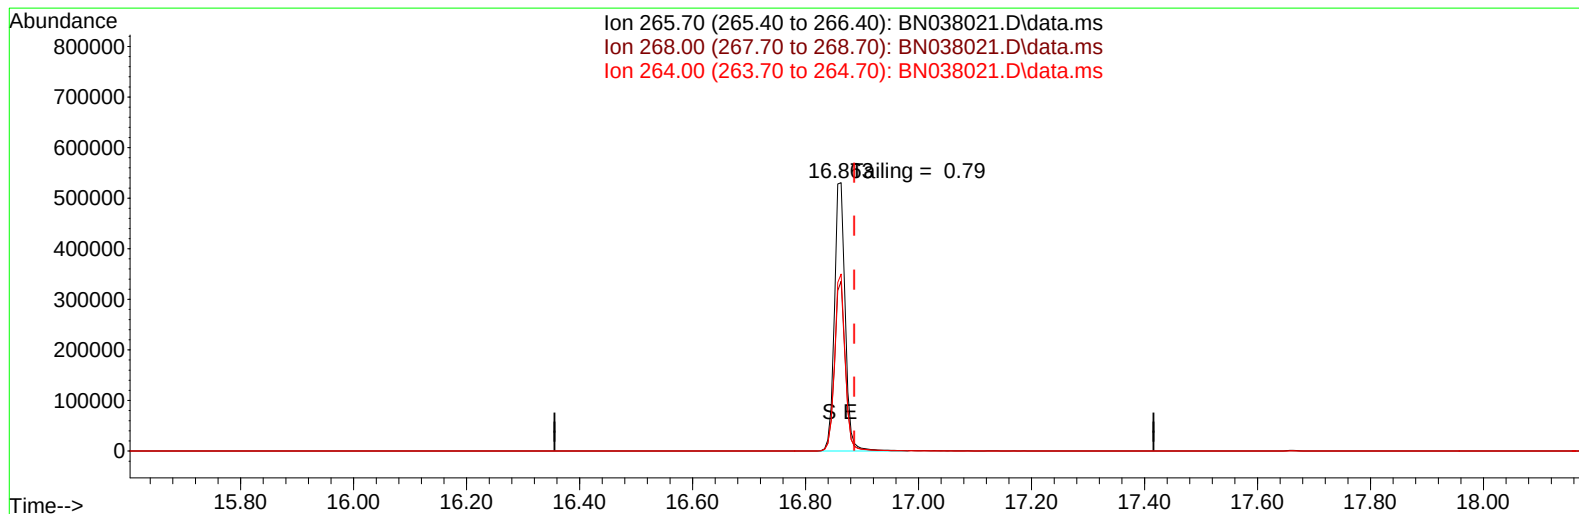

TIC: BN038021.D\data.ms

(70) Pentachlorophenol (C)




16.863min (-0.023) 25768.22 ng

response 704341

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.25
264.00	61.60	65.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100625\
Data File : BN038021.D
Acq On : 06 Oct 2025 22:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 01:36:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

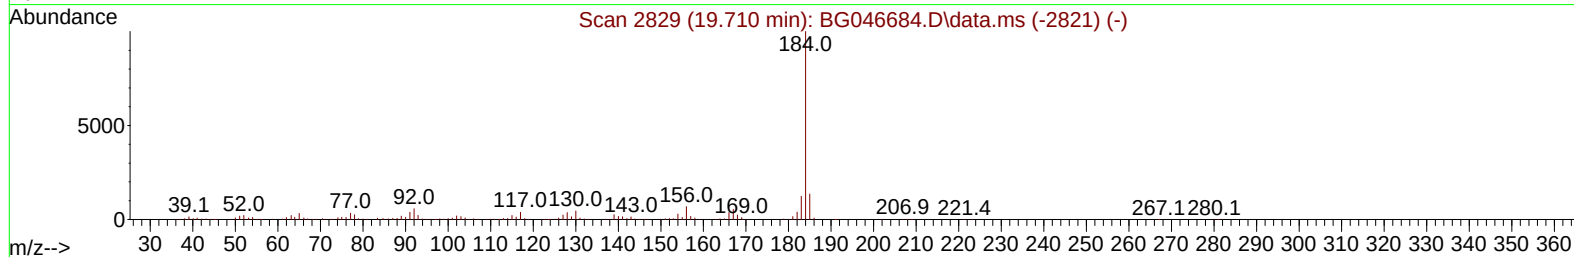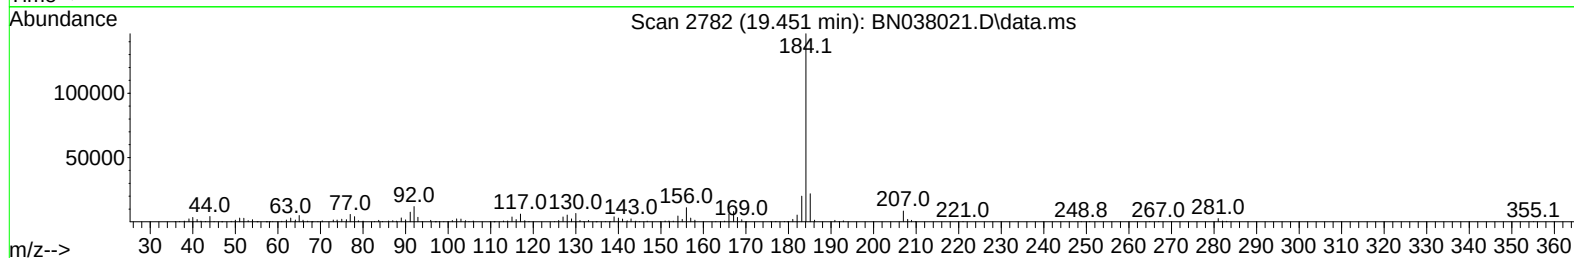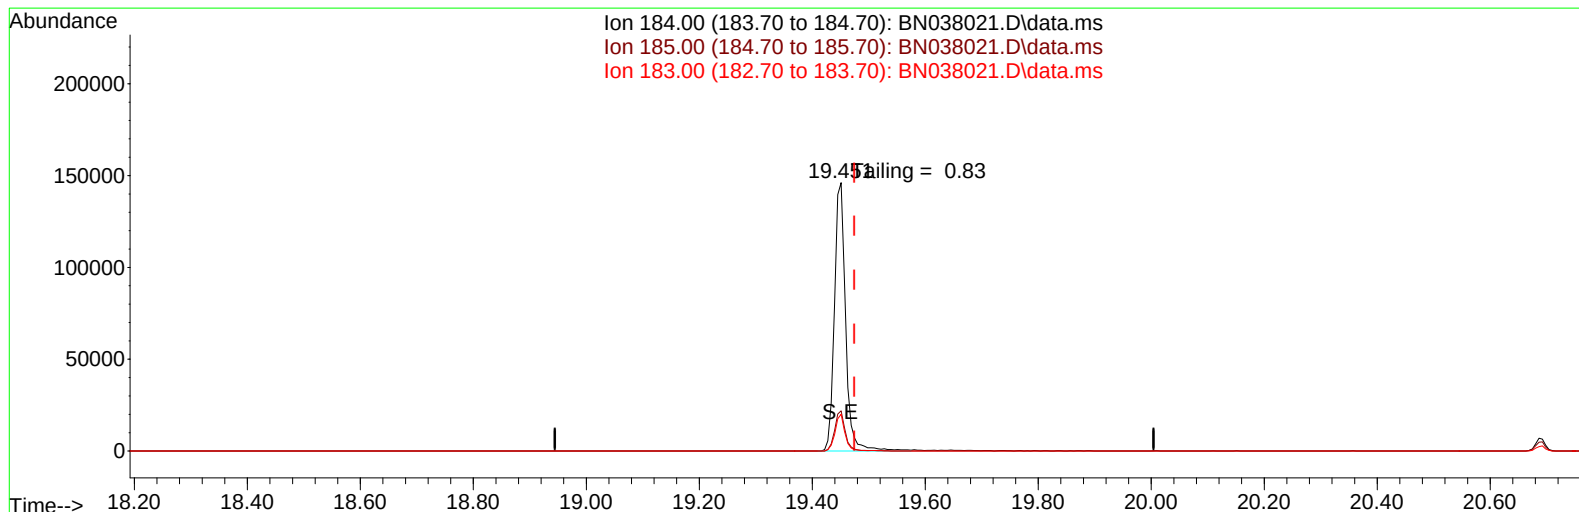

TIC: BN038021.D\data.ms

(77) Benzdine

19.451min (-0.023) 0.00 ng

response 201168

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.96
183.00	13.20	13.71
0.00	0.00	0.00