
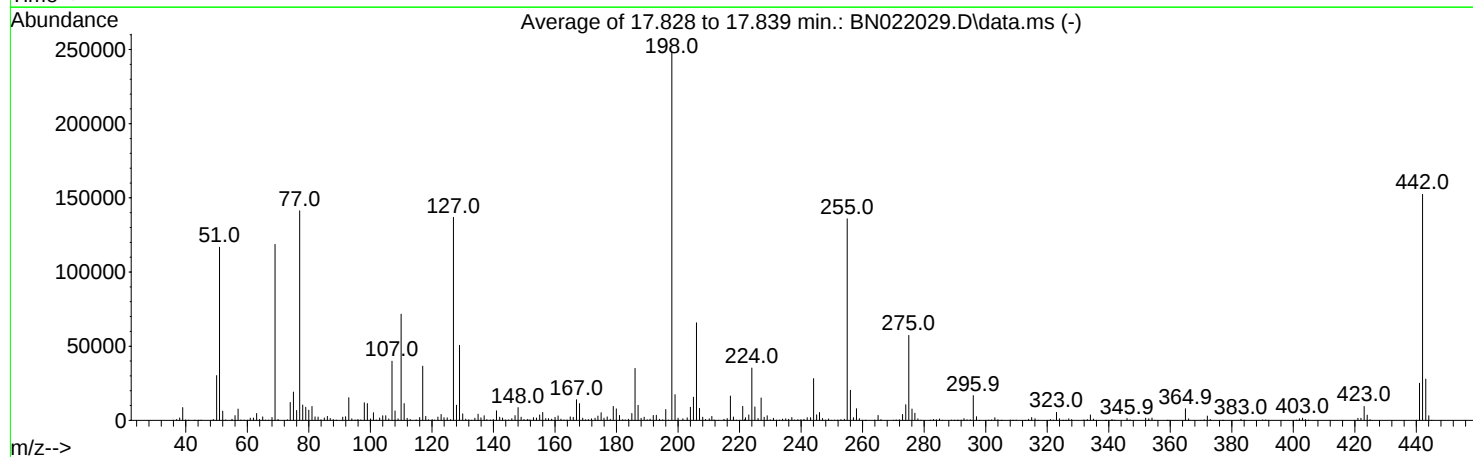


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100722\
 Data File : BN022029.D
 Acq On : 07 Oct 2022 08:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 04 01:32:21 2022

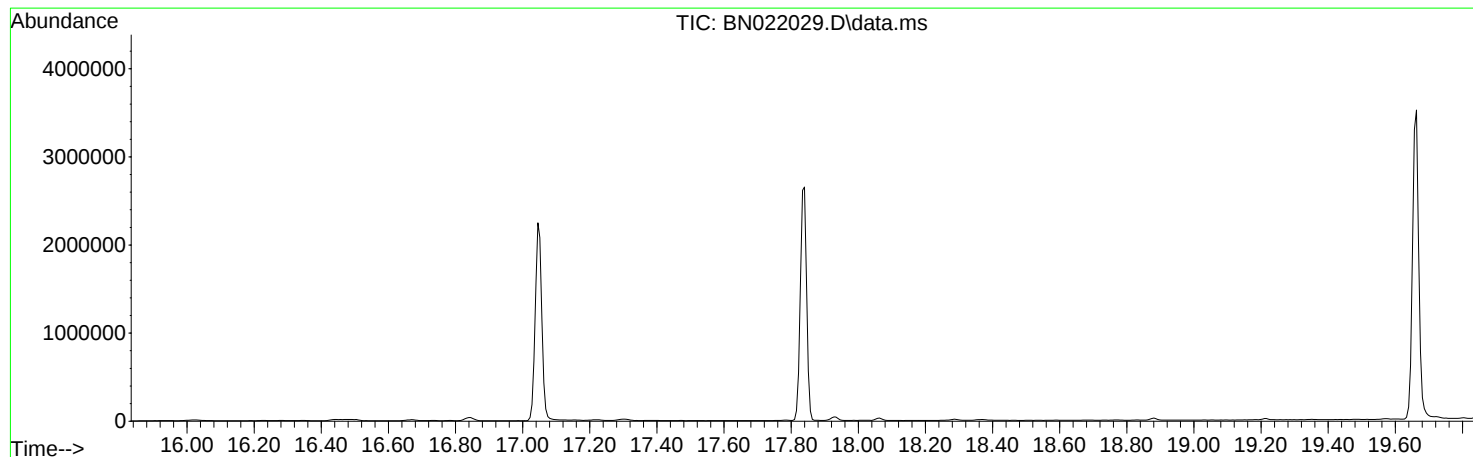

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.1	116713	PASS
68	69	0.00	2	1.6	1923	PASS
69	198	0.00	100	47.9	118680	PASS
70	69	0.00	2	0.5	615	PASS
127	198	10	80	55.2	136845	PASS
197	198	0.00	2	0.1	231	PASS
198	198	100	100	100.0	248000	PASS
199	198	5	9	7.0	17357	PASS
275	198	10	60	23.1	57280	PASS
365	198	1	100	3.2	7896	PASS
441	198	0.01	100	10.1	24988	PASS
442	442	50	100	100.0	152445	PASS
443	442	15	24	18.3	27843	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/7/2022	BNA_N	<u>BN022029.D</u>
Compound Name	Response	Retention Time
DDT	892301	20.892
DDD	10171	20.451
DDE	733	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10904	903205	1.21

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100722\
Data File : BN022029.D
Acq On : 07 Oct 2022 08:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 10 04:25:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 10 04:25:17 2022
Response via : Initial Calibration

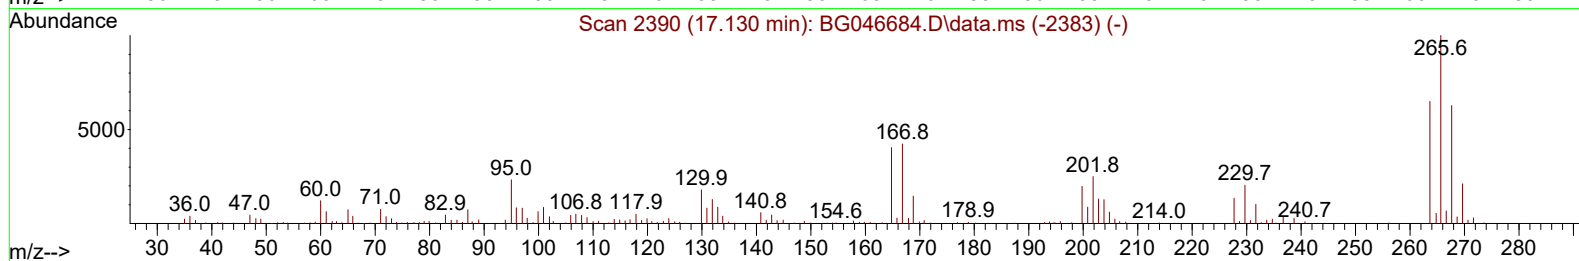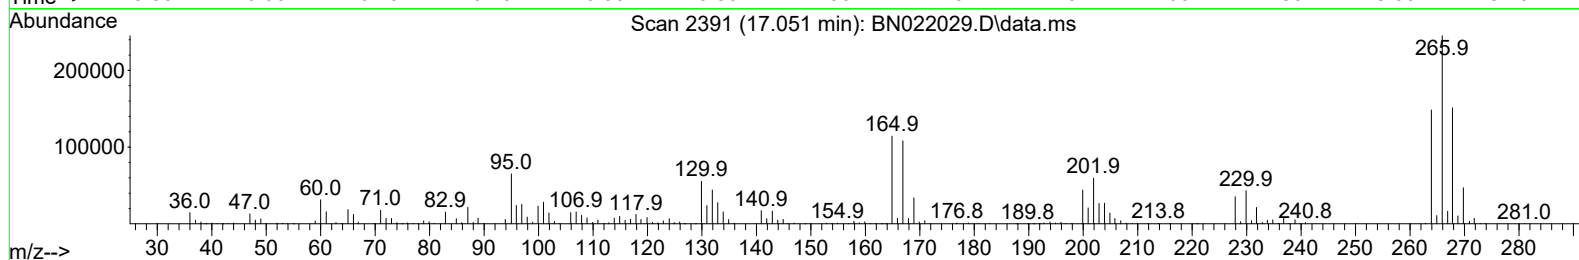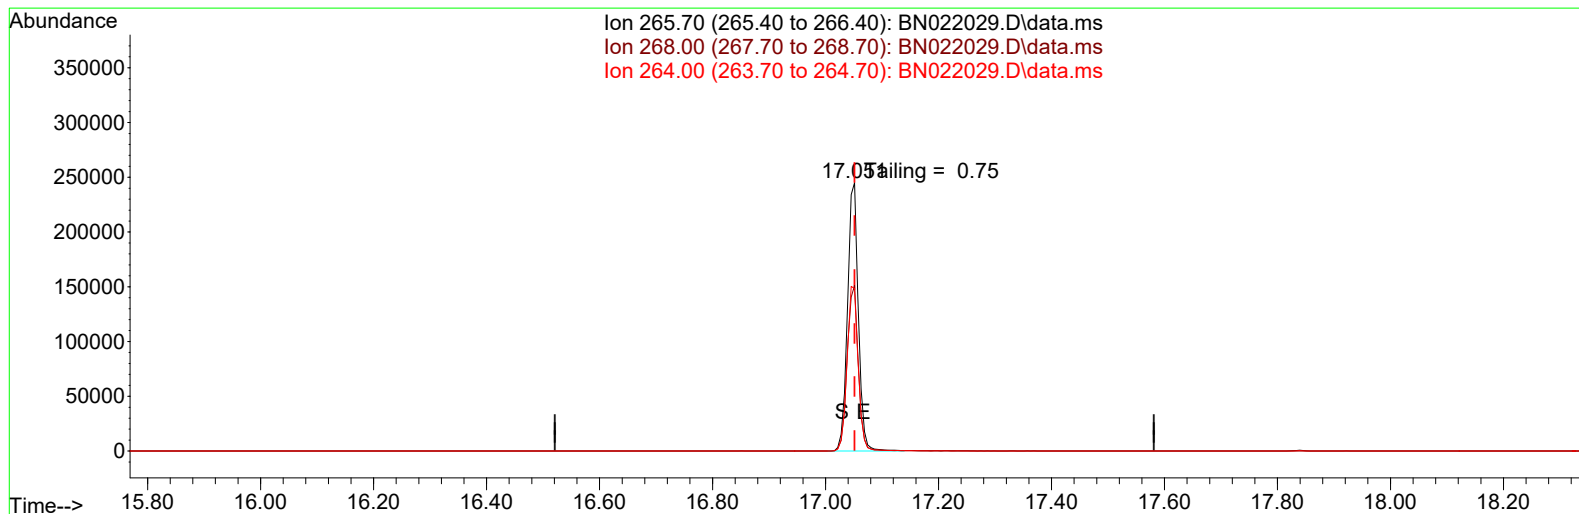

TIC: BN022029.D\data.ms

(70) Pentachlorophenol (C)

17.051min (0.000) 20631.17 ng




response 326407

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.64
264.00	61.60	60.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100722\
Data File : BN022029.D
Acq On : 07 Oct 2022 08:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 10 04:25:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 10 04:25:17 2022
Response via : Initial Calibration

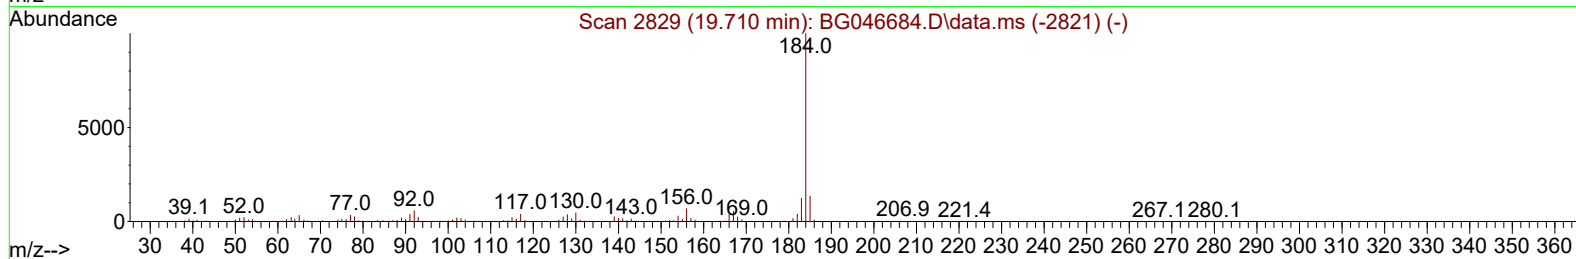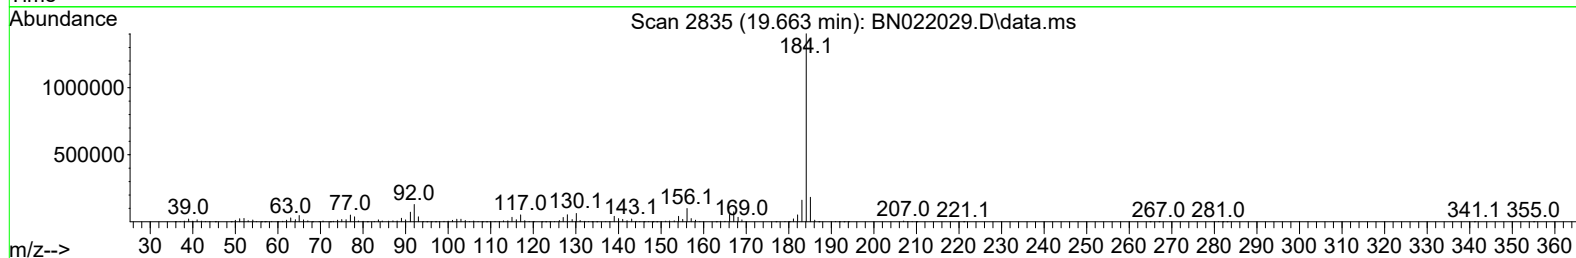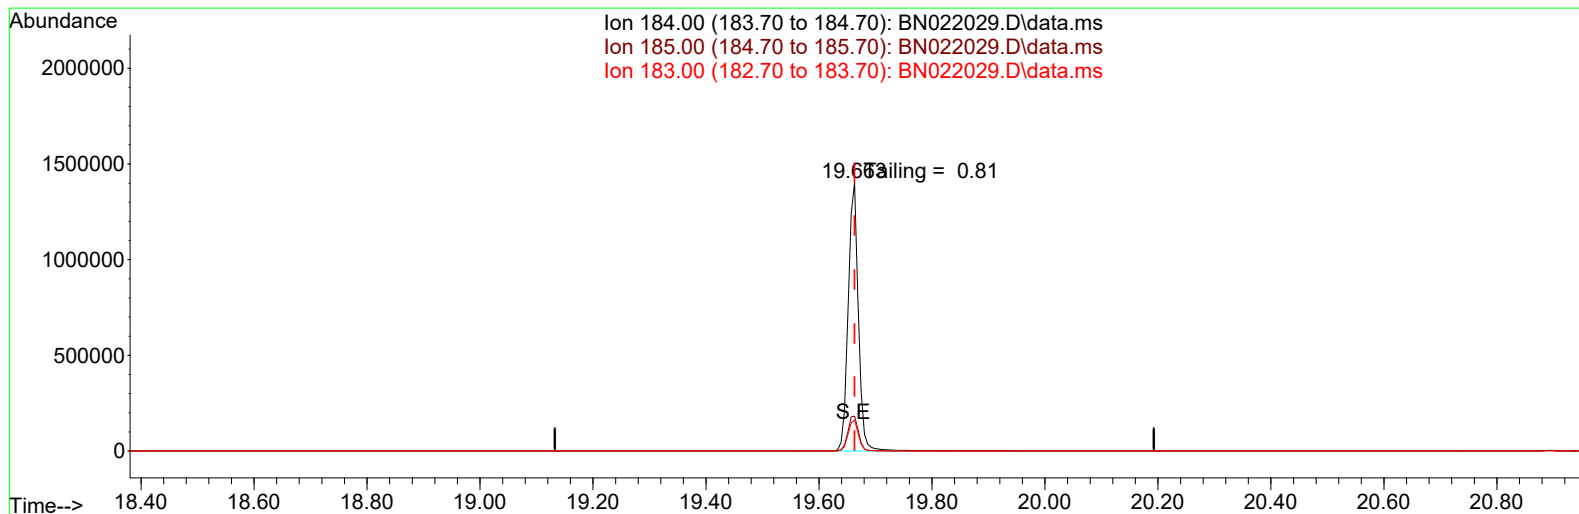

TIC: BN022029.D\data.ms

(77) Benzidine

19.663min (0.000) 0.00 ng

response 1758012

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.02
183.00	13.20	11.51
0.00	0.00	0.00