




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034435.D
Acq On : 07 Oct 2024 11:56
Operator : RC/JU
Sample : PB163648BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK648

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/09/2024

Quant Time: Oct 07 12:26:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

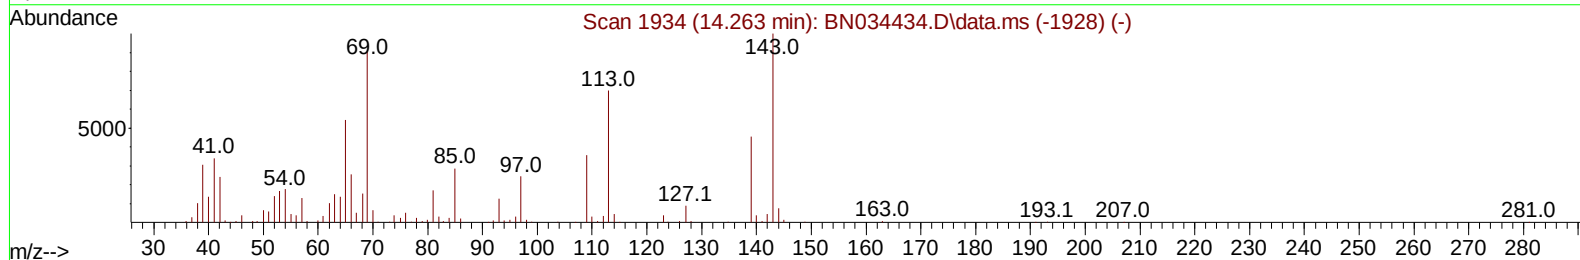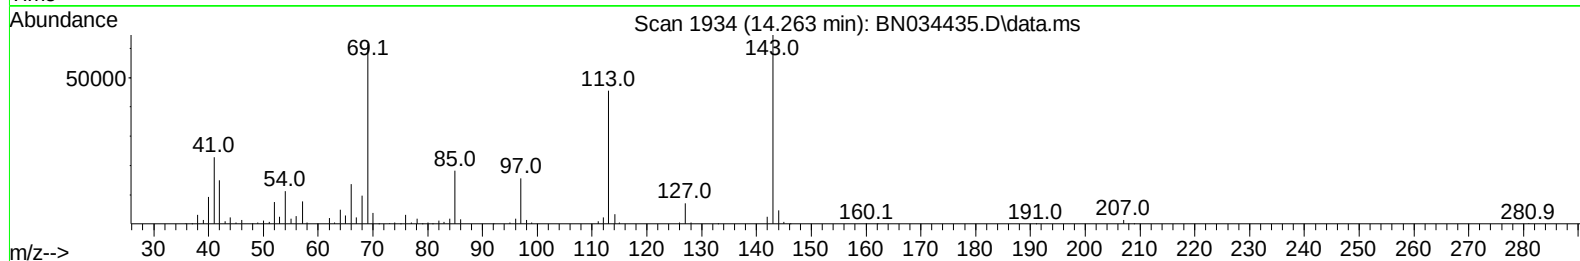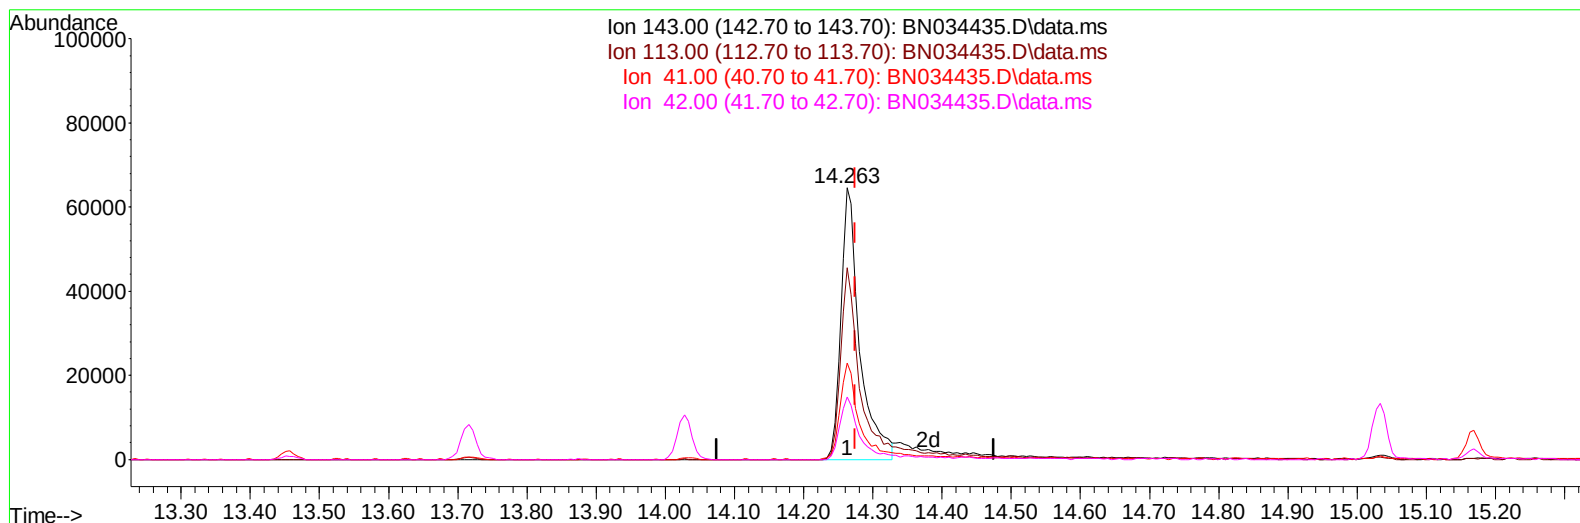

TIC: BN034435.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.263min (-0.012) 13.71 ng/u1

response 120924

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	76.90	70.61
41.00	41.70	35.50
42.00	28.50	23.09




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034435.D
Acq On : 07 Oct 2024 11:56
Operator : RC/JU
Sample : PB163648BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK648

Manual IntegrationsAPPROVED

Quant Time: Oct 07 12:26:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/09/2024

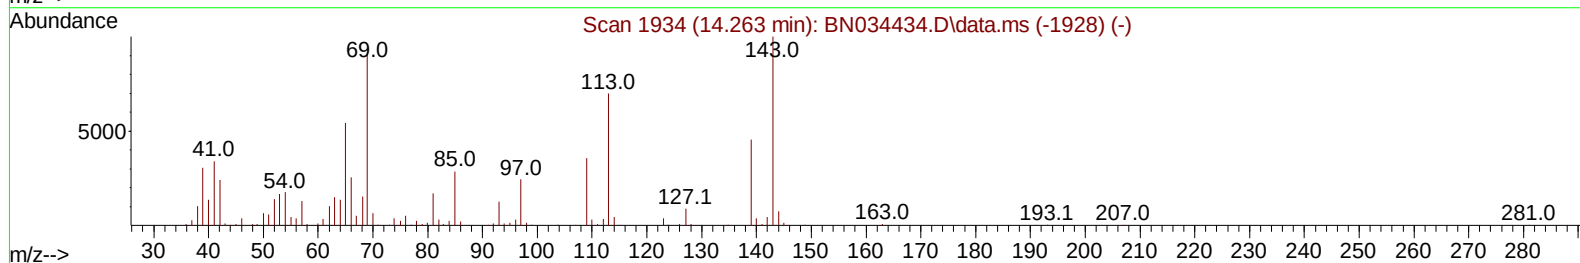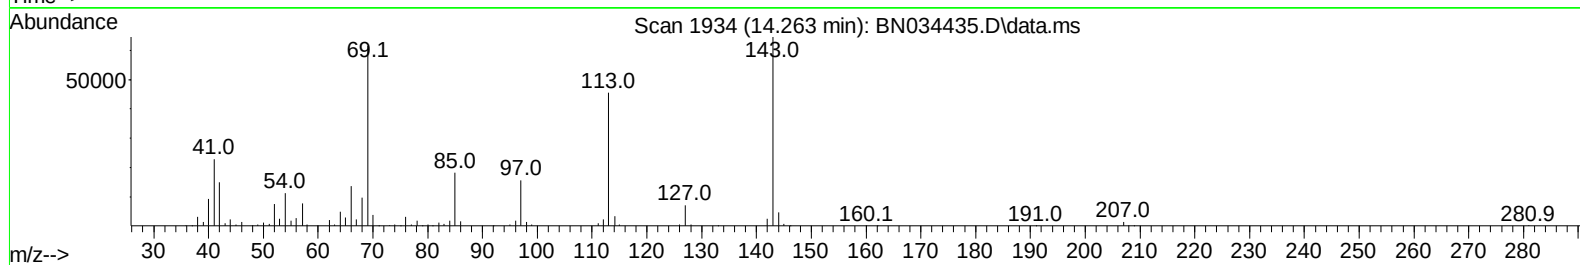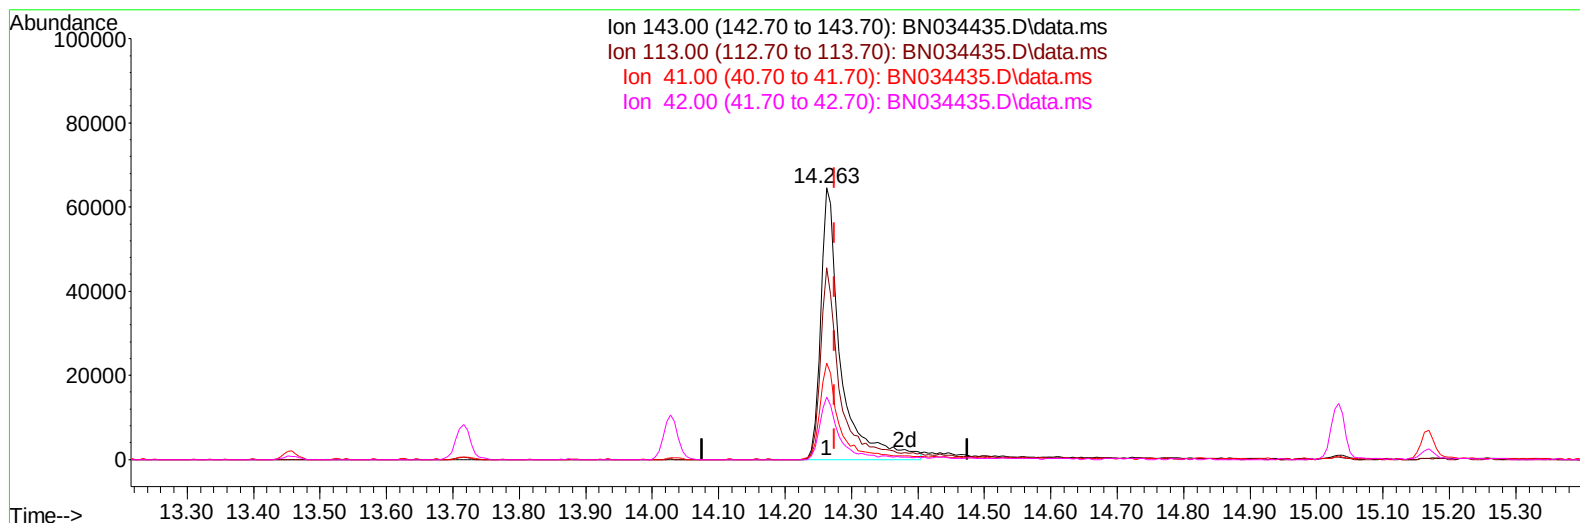

TIC: BN034435.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.263min (-0.012) 15.08 ng/ul m

response 133002

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	76.90	70.61
41.00	41.70	35.50
42.00	28.50	23.09

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
 Data File : BN034435.D
 Acq On : 07 Oct 2024 11:56
 Operator : RC/JU
 Sample : PB163648BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK648

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/08/2024
 Supervised By :mohammad ahmed 10/09/2024

Quant Time: Oct 07 12:26:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 30 14:14:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.375	152	235819	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.134	136	929877	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.028	164	575204	20.000	ng/ul	-0.01
64) Phenanthrene-d10	16.786	188	1183013	20.000	ng/ul	-0.01
79) Chrysene-d12	21.021	240	1039694	20.000	ng/ul	-0.01
88) Perylene-d12	23.727	264	1093892	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.999	96	29524	5.109	ng/uL	0.00
4) Pyridine-d5	3.381	84	359792	20.946	ng/ul	0.00
7) Phenol-d5	6.575	99	434623	20.767	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.734	67	275975	21.253	ng/ul	0.00
11) 2-Chlorophenol-d4	6.916	132	394485	23.946	ng/ul	-0.01
15) 4-Methylphenol-d8	8.093	113	353853	20.548	ng/ul	-0.01
21) Nitrobenzene-d5	8.522	128	181482	24.486	ng/ul	0.00
24) 2-Nitrophenol-d4	9.234	143	194349	25.500	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.763	165	336123	23.418	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.281	131	498910	22.959	ng/ul	-0.01
46) Dimethylphthalate-d6	13.457	166	1063758	24.746	ng/ul	-0.01
49) Acenaphthylene-d8	13.716	160	1177239	24.344	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.263	143	133002m	15.076	ng/ul	-0.01
60) Fluorene-d10	15.034	176	890529	24.444	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.169	200	119591	16.955	ng/ul	0.00
73) Anthracene-d10	16.886	188	1373667	24.698	ng/ul	-0.01
81) Pyrene-d10	19.198	212	1554005	26.826	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.545	264	1413399	25.154	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034435.D
Acq On : 07 Oct 2024 11:56
Operator : RC/JU
Sample : PB163648BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK648

Manual IntegrationsAPPROVED

Quant Time: Oct 07 12:26:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/09/2024

