




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
 Data File : BN034437.D
 Acq On : 07 Oct 2024 14:19
 Operator : RC/JU
 Sample : P4109-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4EH6

Manual IntegrationsAPPROVED

Quant Time: Oct 07 14:59:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 30 14:14:38 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
 Supervised By :mohammad ahmed 10/09/2024

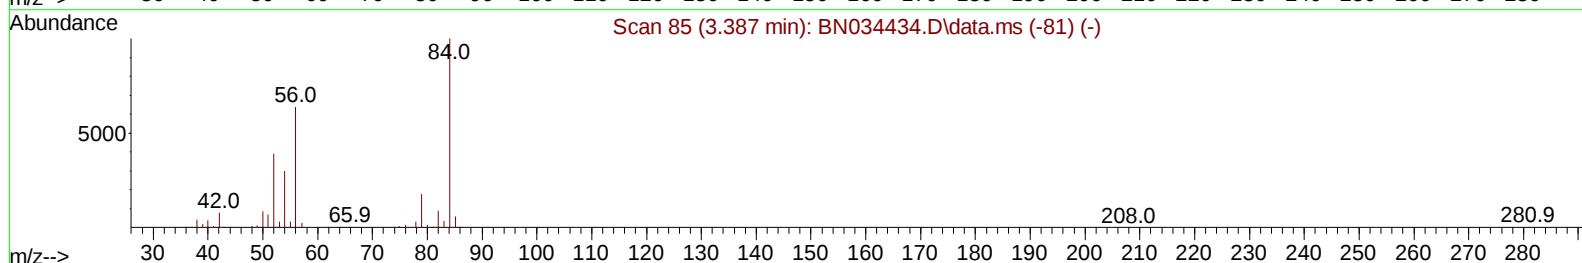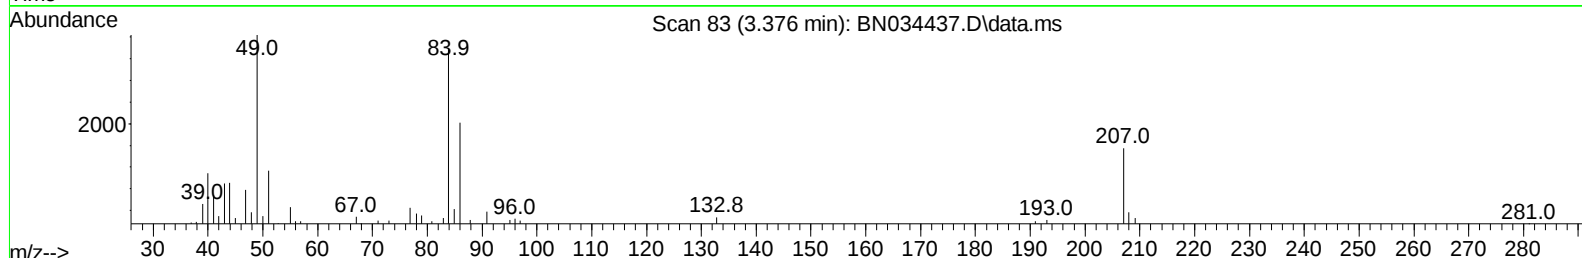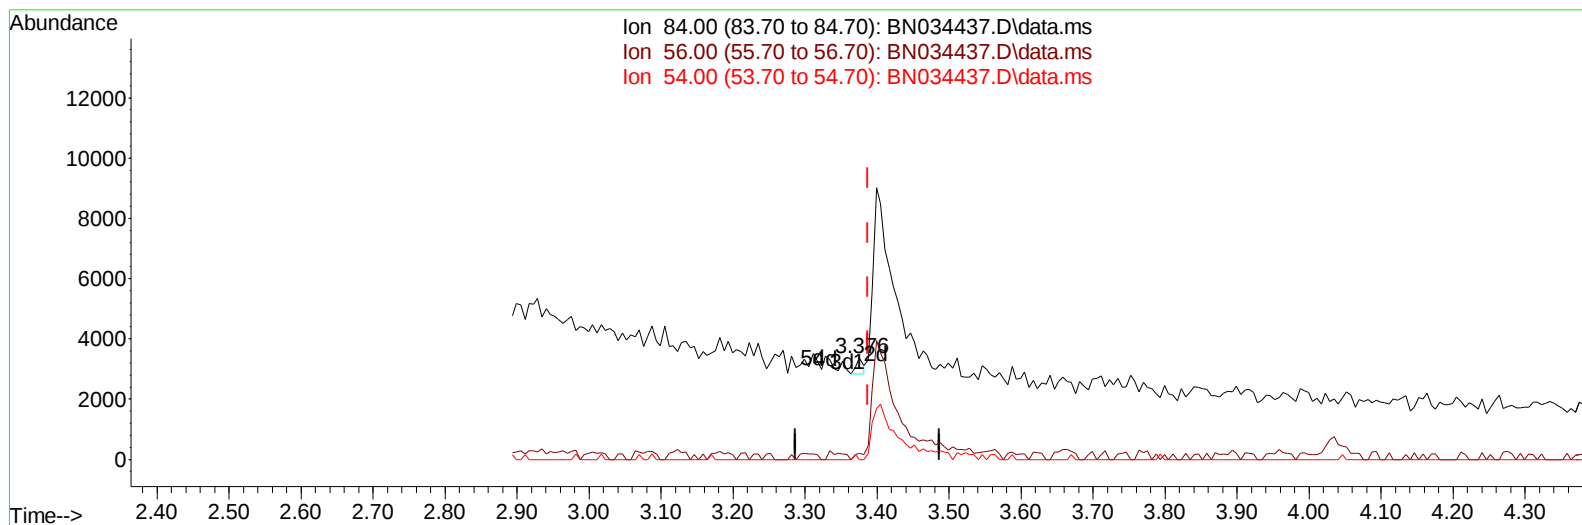

TIC: BN034437.D\data.ms

(4) Pyridine-d5 (S)

3.376min (-0.012) 0.03 ng/u1

response 375

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	67.90	5.77#
54.00	32.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034437.D
Acq On : 07 Oct 2024 14:19
Operator : RC/JU
Sample : P4109-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4EH6

Manual IntegrationsAPPROVED

Quant Time: Oct 07 14:59:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/09/2024

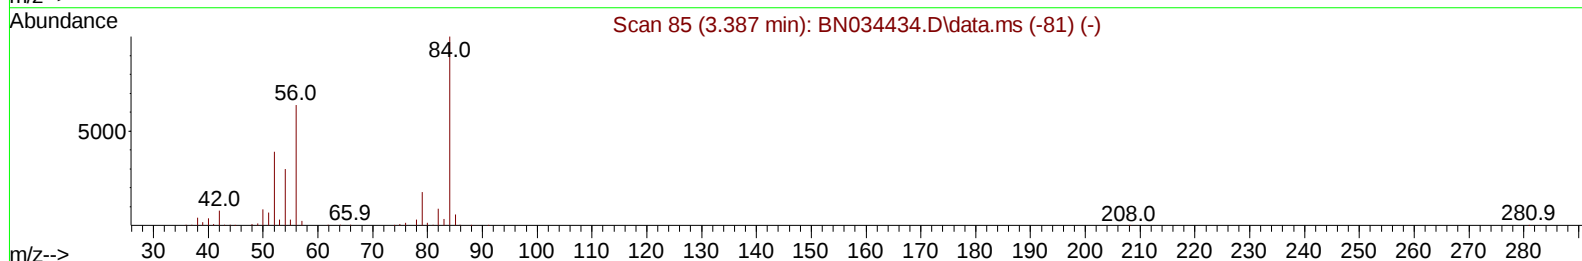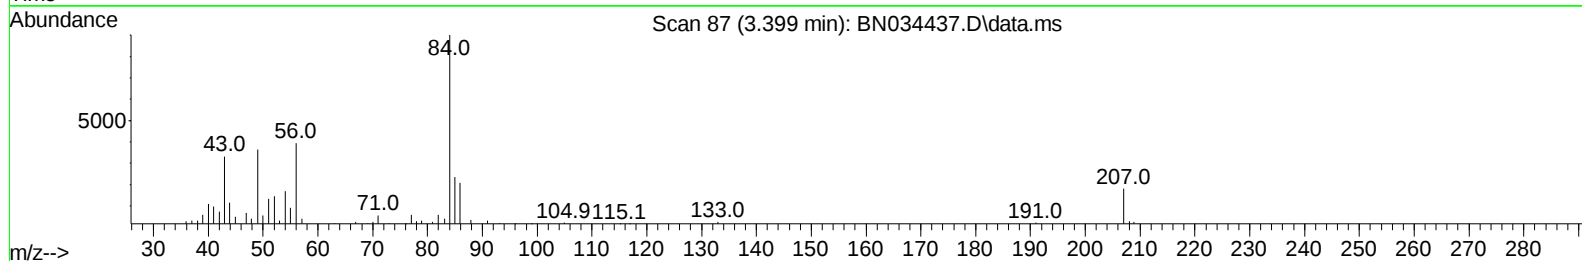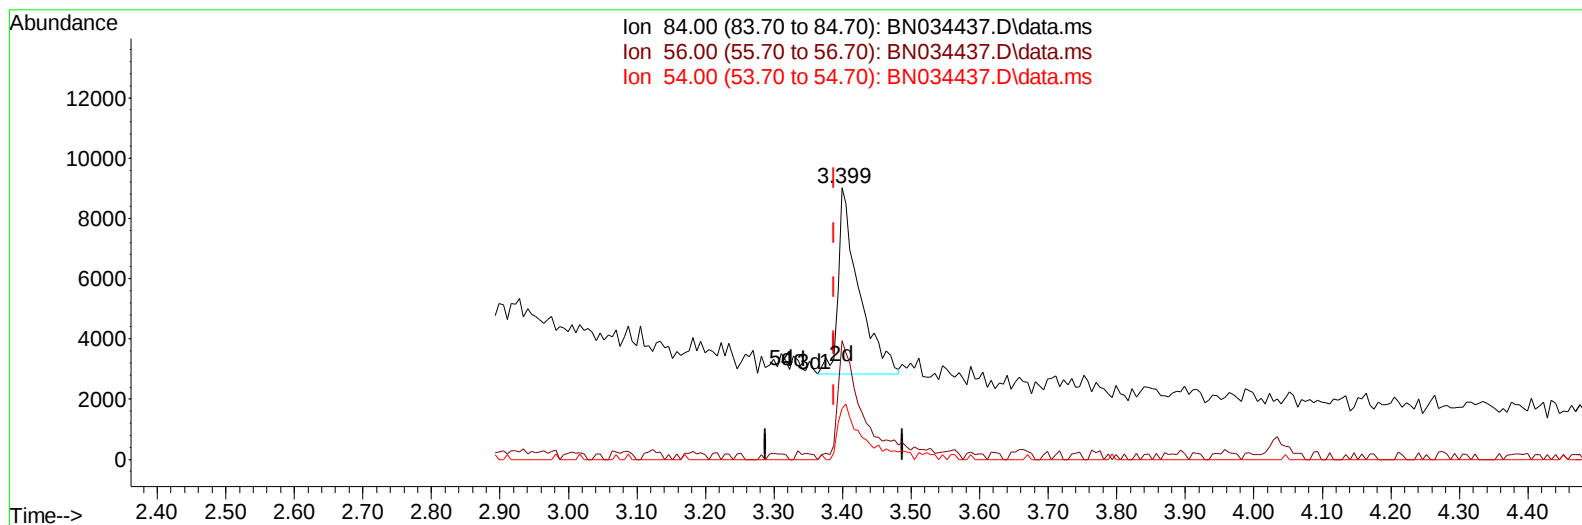

TIC: BN034437.D\data.ms

(4) Pyridine-d5 (S)

3.399min (+ 0.012) 1.02 ng/u1 m

response 12983

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	67.90	43.87#
54.00	32.80	18.69#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034437.D
Acq On : 07 Oct 2024 14:19
Operator : RC/JU
Sample : P4109-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4EH6

Manual IntegrationsAPPROVED

Quant Time: Oct 07 14:59:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/09/2024

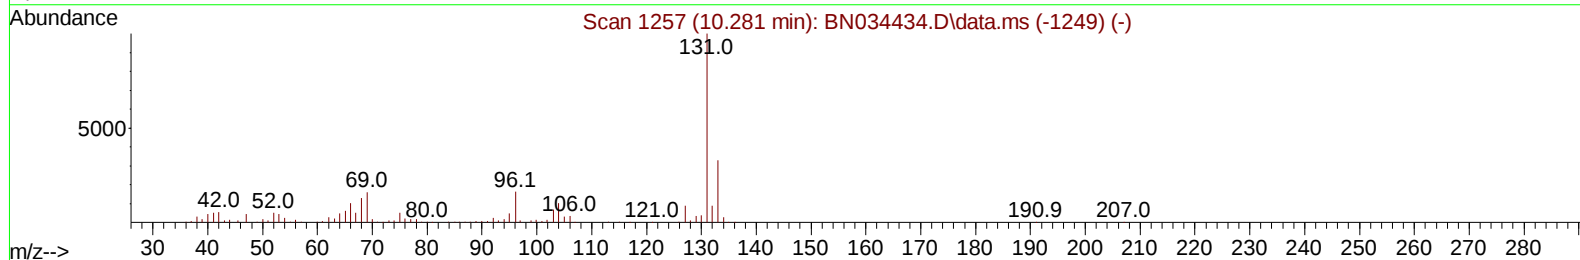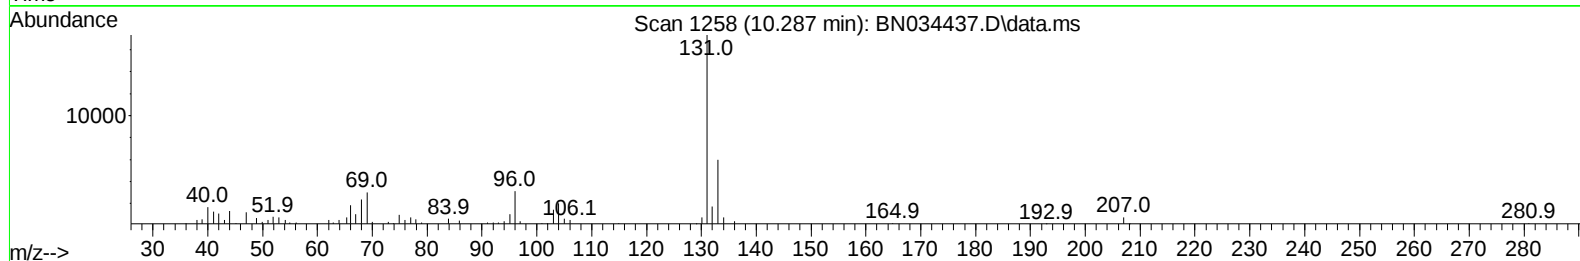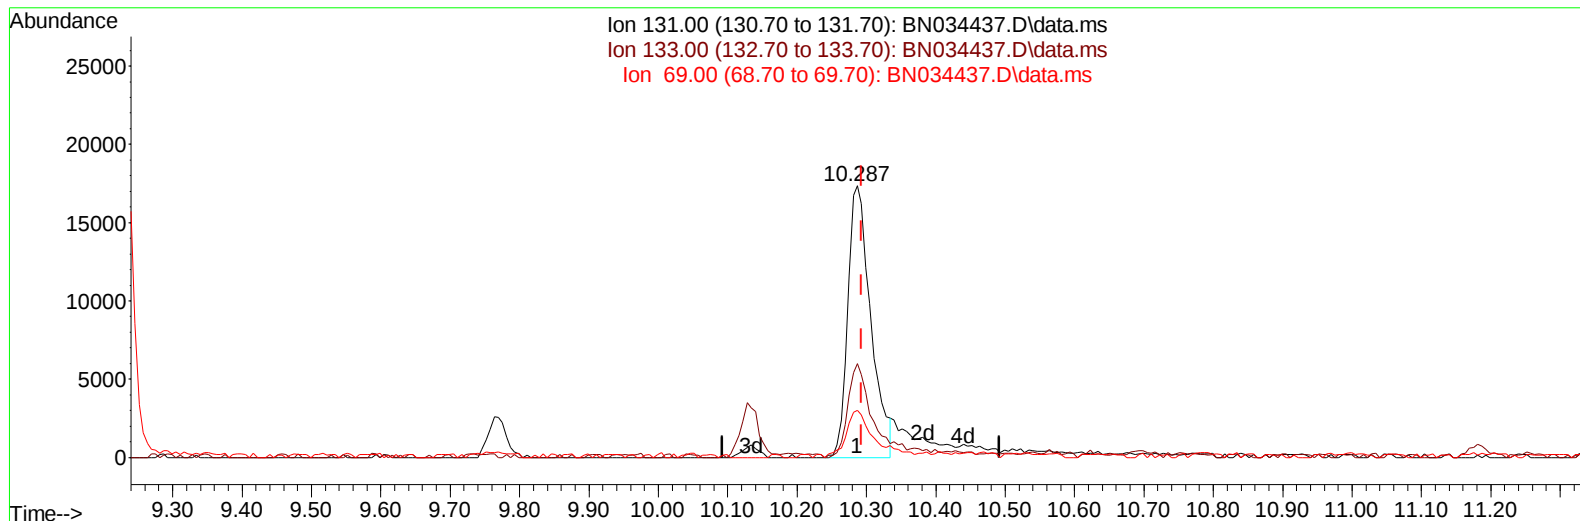

TIC: BN034437.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.287min (-0.006) 2.45 ng/u1

response 39990

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.00	34.51
69.00	17.80	17.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
 Data File : BN034437.D
 Acq On : 07 Oct 2024 14:19
 Operator : RC/JU
 Sample : P4109-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4EH6

Manual IntegrationsAPPROVED

Quant Time: Oct 07 14:59:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 30 14:14:38 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
 Supervised By :mohammad ahmed 10/09/2024

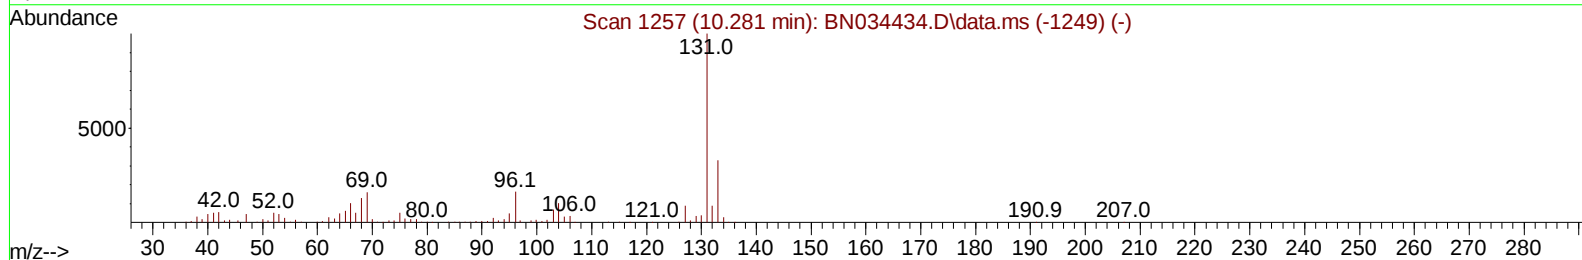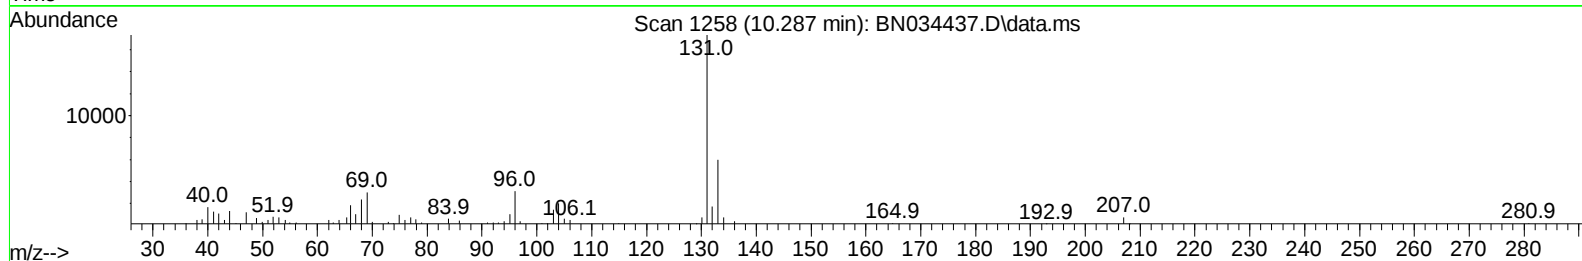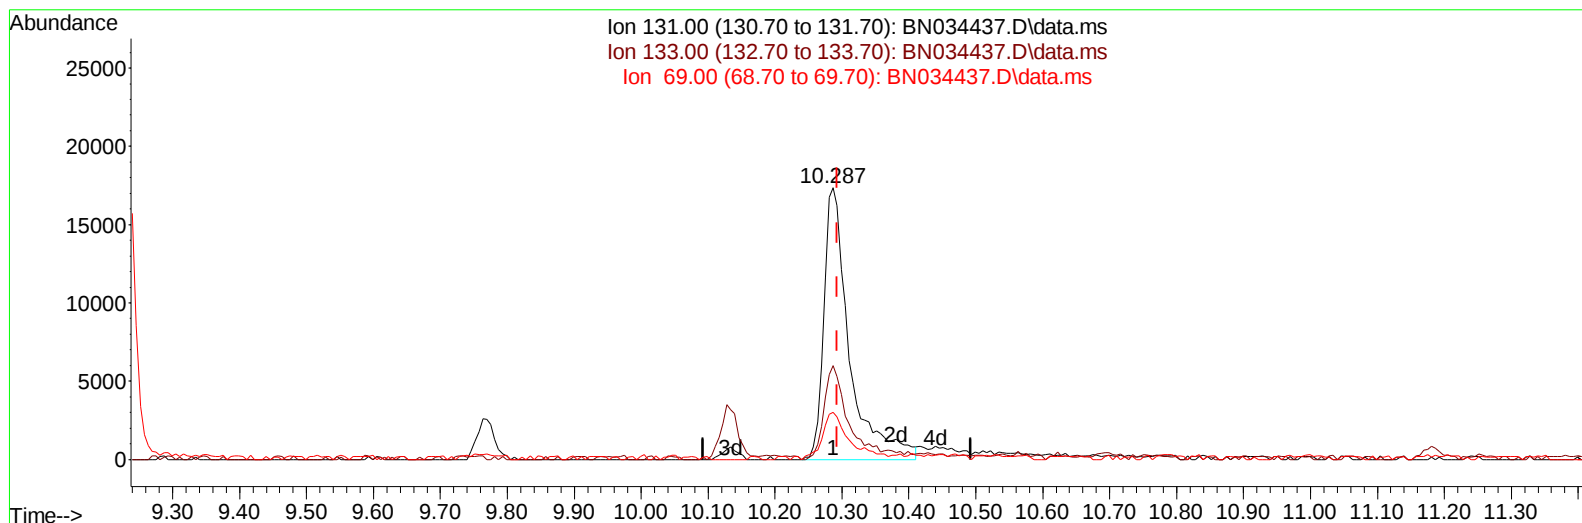

TIC: BN034437.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.287min (-0.006) 2.82 ng/ul m

response 46031

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.00	34.51
69.00	17.80	17.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
 Data File : BN034437.D
 Acq On : 07 Oct 2024 14:19
 Operator : RC/JU
 Sample : P4109-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4EH6

Manual IntegrationsAPPROVED

Quant Time: Oct 07 15:04:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 30 14:14:38 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
 Supervised By :mohammad ahmed 10/09/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.375	152		174561	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.128	136		697409	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.028	164		438132	20.000	ng/ul	-0.01
64) Phenanthrene-d10	16.787	188		925758	20.000	ng/ul	-0.01
79) Chrysene-d12	21.028	240		885503	20.000	ng/ul	0.00
88) Perylene-d12	23.733	264		932378	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	2.993	96		9084	2.124	ng/uL	0.00
4) Pyridine-d5	3.399	84		12983m	1.021	ng/ul	0.01
7) Phenol-d5	6.575	99		158850	10.253	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.734	67		109830	11.426	ng/ul	0.00
11) 2-Chlorophenol-d4	6.917	132		152218	12.482	ng/ul	-0.01
15) 4-Methylphenol-d8	8.093	113		100622	7.893	ng/ul	-0.01
21) Nitrobenzene-d5	8.516	128		70848	12.745	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.234	143		76197	13.330	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.769	165		136063	12.639	ng/ul	0.00
31) 4-Chloroaniline-d4	10.287	131		46031m	2.824	ng/ul	0.00
46) Dimethylphthalate-d6	13.457	166		442013	13.499	ng/ul	-0.01
49) Acenaphthylene-d8	13.716	160		509626	13.835	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.269	143		36204	5.388	ng/ul	0.00
60) Fluorene-d10	15.034	176		397382	14.320	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.169	200		45619	8.265	ng/ul	0.00
73) Anthracene-d10	16.887	188		617088	14.178	ng/ul	-0.01
81) Pyrene-d10	19.198	212		646273	13.099	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.551	264		411088	8.583	ng/ul	0.00
Target Compounds							
						Qvalue	
16) Acetophenone	8.193	105		56931	2.819	ng/ul	97
50) Acenaphthylene	13.746	152		47473	1.178	ng/ul	97
61) Fluorene	15.093	166		33993	1.056	ng/ul	93
72) Phenanthrene	16.828	178		783399	15.347	ng/ul	99
74) Anthracene	16.922	178		149339	2.865	ng/ul	99
77) Carbazole	17.198	167		77662	1.619	ng/ul	99
80) Fluoranthene	18.863	202		1840587	31.911	ng/ul	98
82) Pyrene	19.228	202		1263639	20.379	ng/ul	95
85) Benzo(a)anthracene	21.010	228		806670	12.777	ng/ul	95
86) Bis(2-ethylhexyl)phtha...	20.975	149		173715	4.268	ng/ul#	94
87) Chrysene	21.069	228		952233	15.807	ng/ul	99
90) Benzo(b)fluoranthene	22.892	252		1226783	21.581	ng/ul	100
91) Benzo(k)fluoranthene	22.939	252		423257	7.548	ng/ul	97
93) Benzo(a)pyrene	23.610	252		362022	6.741	ng/ul#	94
94) Indeno(1,2,3-cd)pyrene	26.721	276		383029	5.757	ng/ul	99
95) Dibenzo(a,h)anthracene	26.763	278		137718	2.561	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

