




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034438.D
Acq On : 07 Oct 2024 14:59
Operator : RC/JU
Sample : P4109-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4EH7

Manual IntegrationsAPPROVED

Quant Time: Oct 07 15:39:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/09/2024

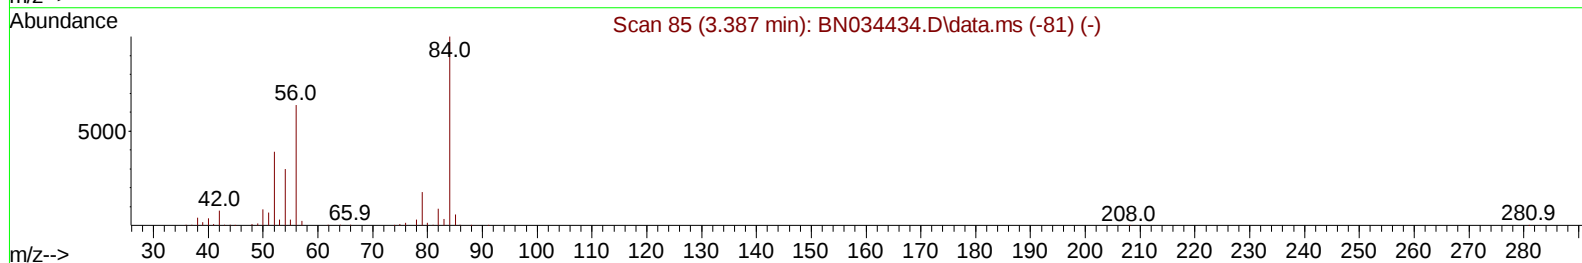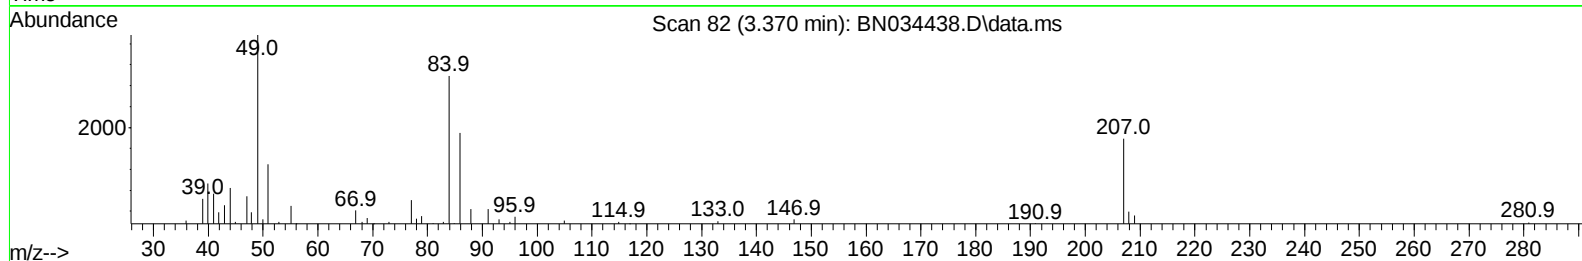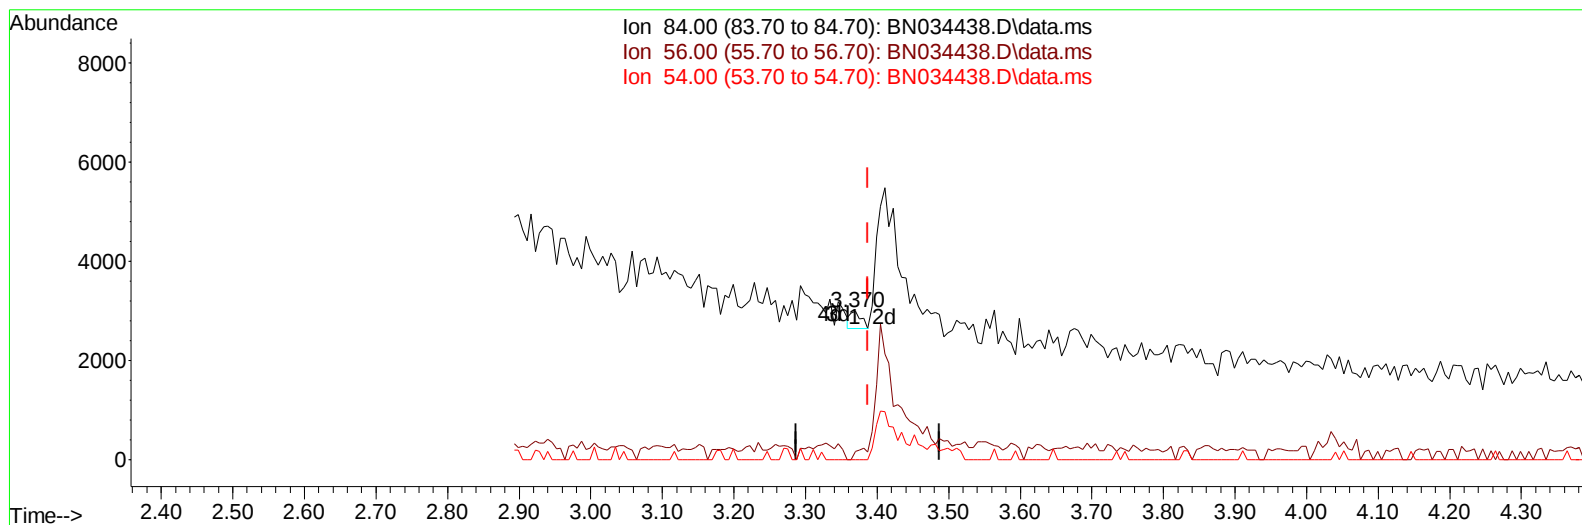

TIC: BN034438.D\data.ms

(4) Pyridine-d5 (S)

3.370min (-0.018) 0.03 ng/u1

response 369

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	67.90	5.39#
54.00	32.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034438.D
Acq On : 07 Oct 2024 14:59
Operator : RC/JU
Sample : P4109-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4EH7

Manual IntegrationsAPPROVED

Quant Time: Oct 07 15:39:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/09/2024

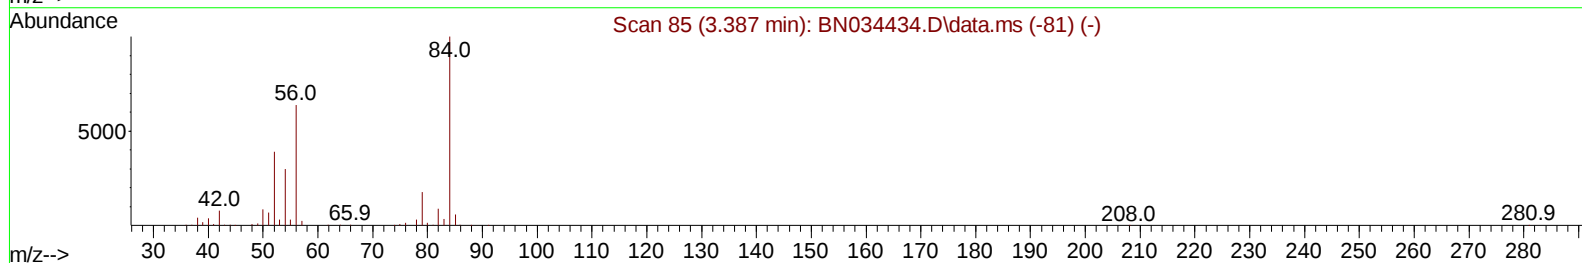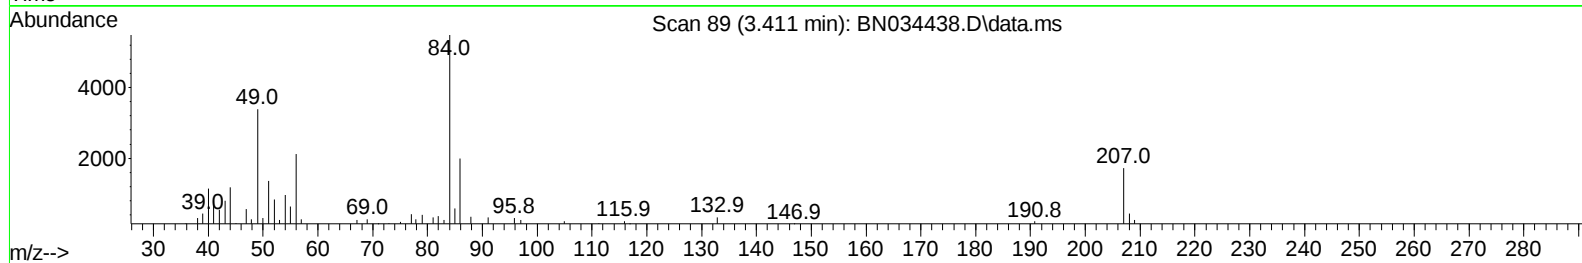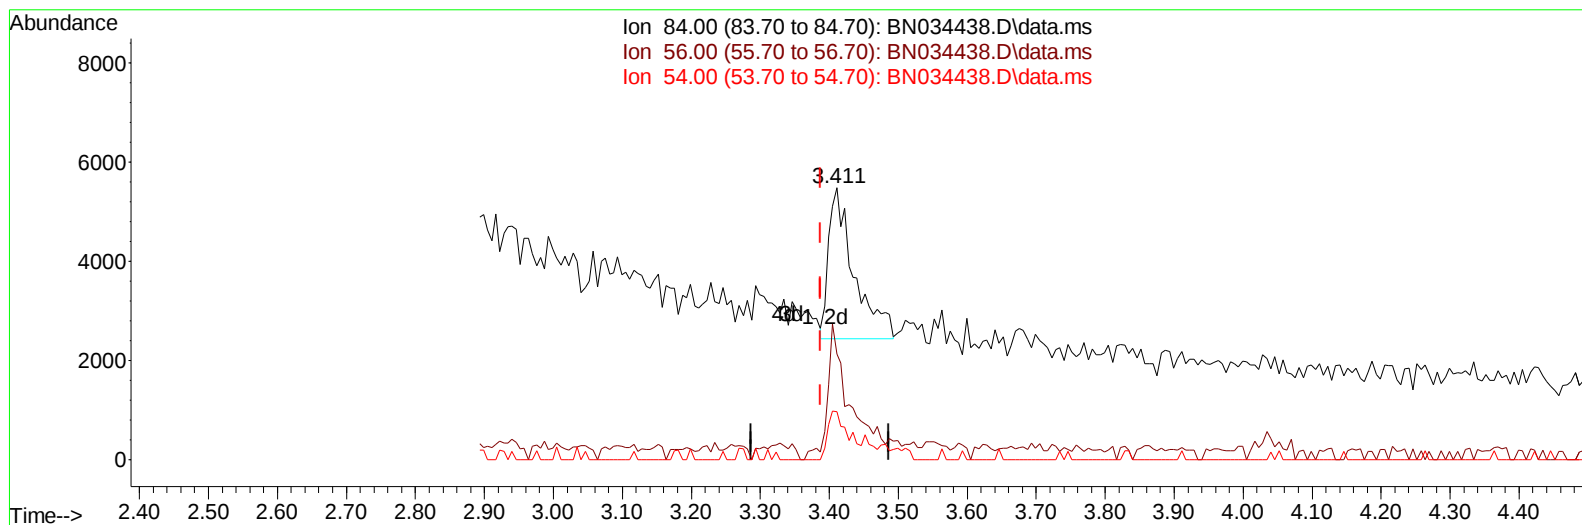

TIC: BN034438.D\data.ms

(4) Pyridine-d5 (S)

3.411min (+ 0.024) 0.74 ng/ul m

response 7812

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	67.90	38.81#
54.00	32.80	17.65#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
 Data File : BN034438.D
 Acq On : 07 Oct 2024 14:59
 Operator : RC/JU
 Sample : P4109-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4EH7

Manual IntegrationsAPPROVED

Quant Time: Oct 07 15:39:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 30 14:14:38 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
 Supervised By :mohammad ahmed 10/09/2024

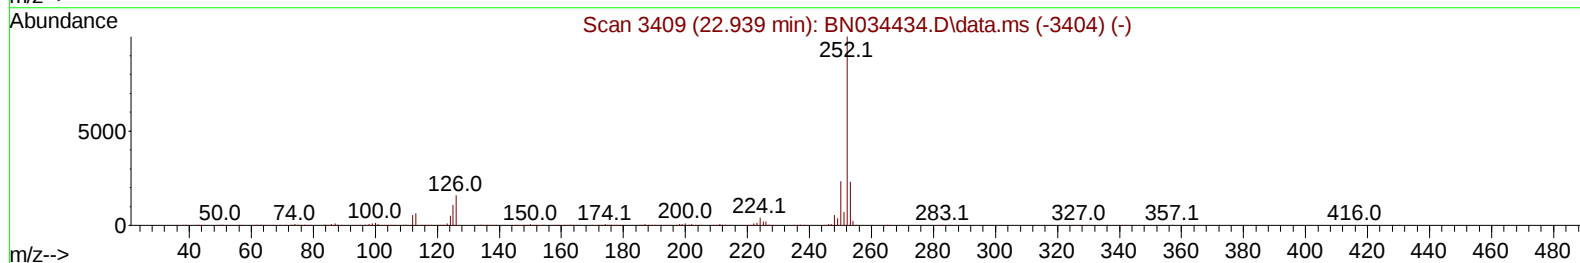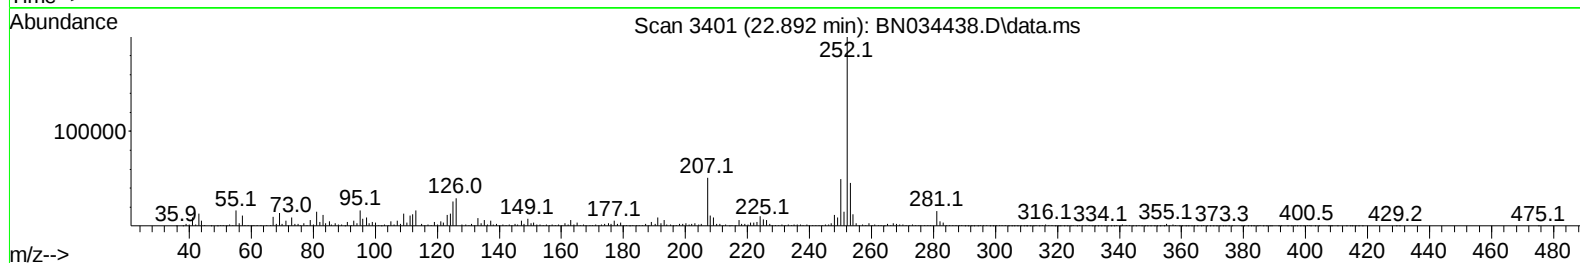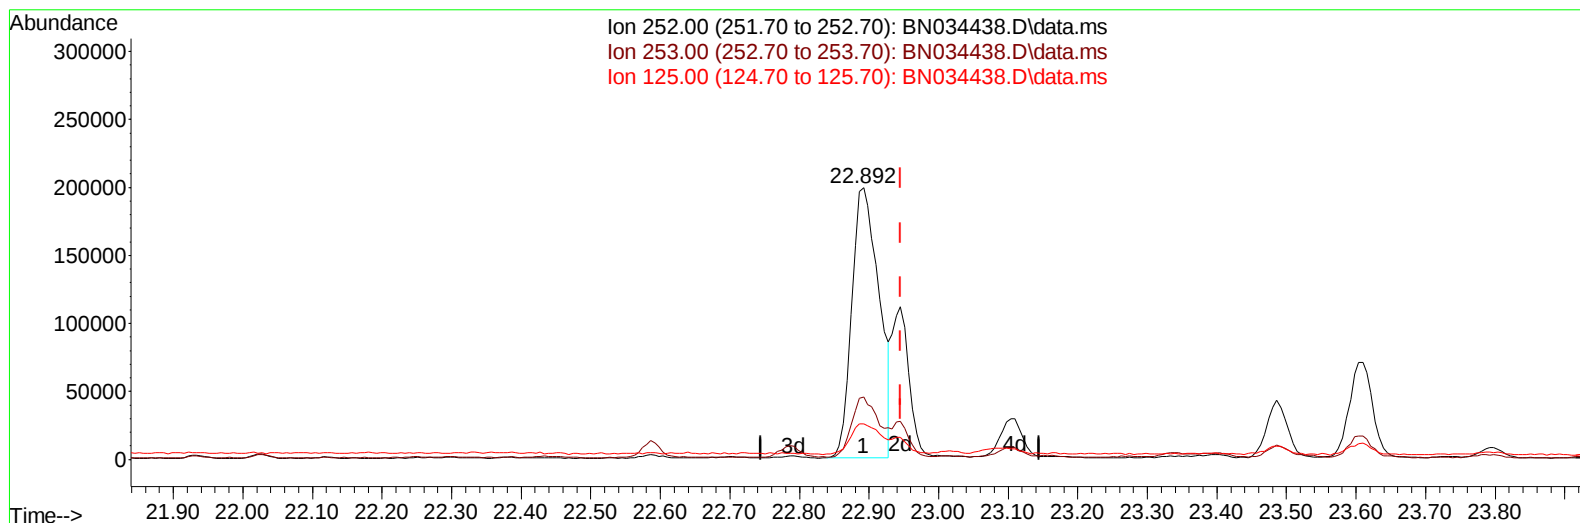

TIC: BN034438.D\data.ms

(91) Benzo(k)fluoranthene

22.892min (-0.053) 10.66 ng/u1

response 541818

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.70	22.90
125.00	11.00	13.13
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034438.D
Acq On : 07 Oct 2024 14:59
Operator : RC/JU
Sample : P4109-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4EH7

Manual IntegrationsAPPROVED

Quant Time: Oct 07 15:39:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/09/2024

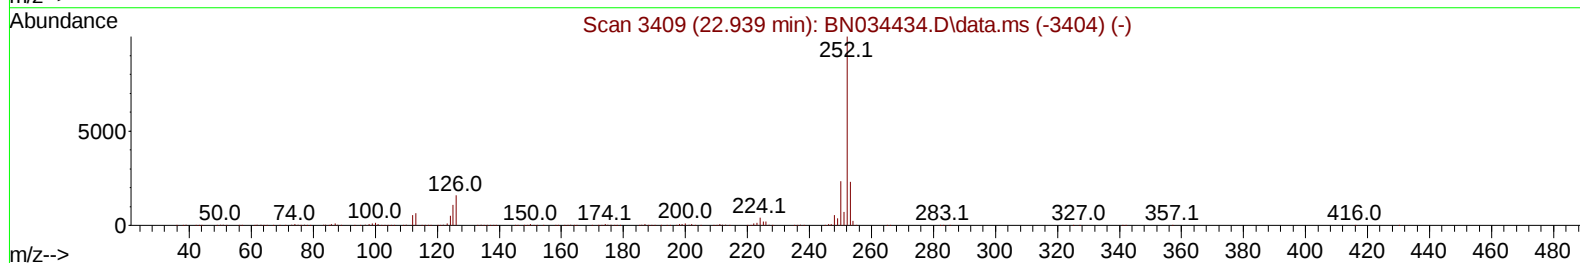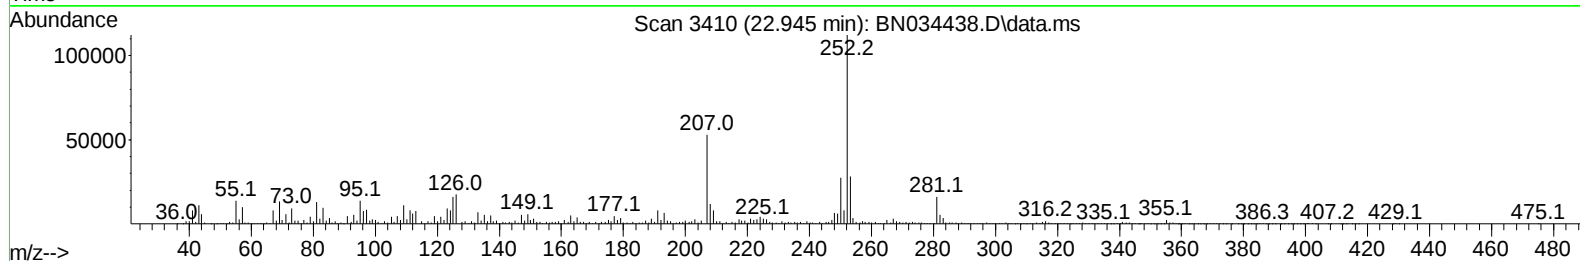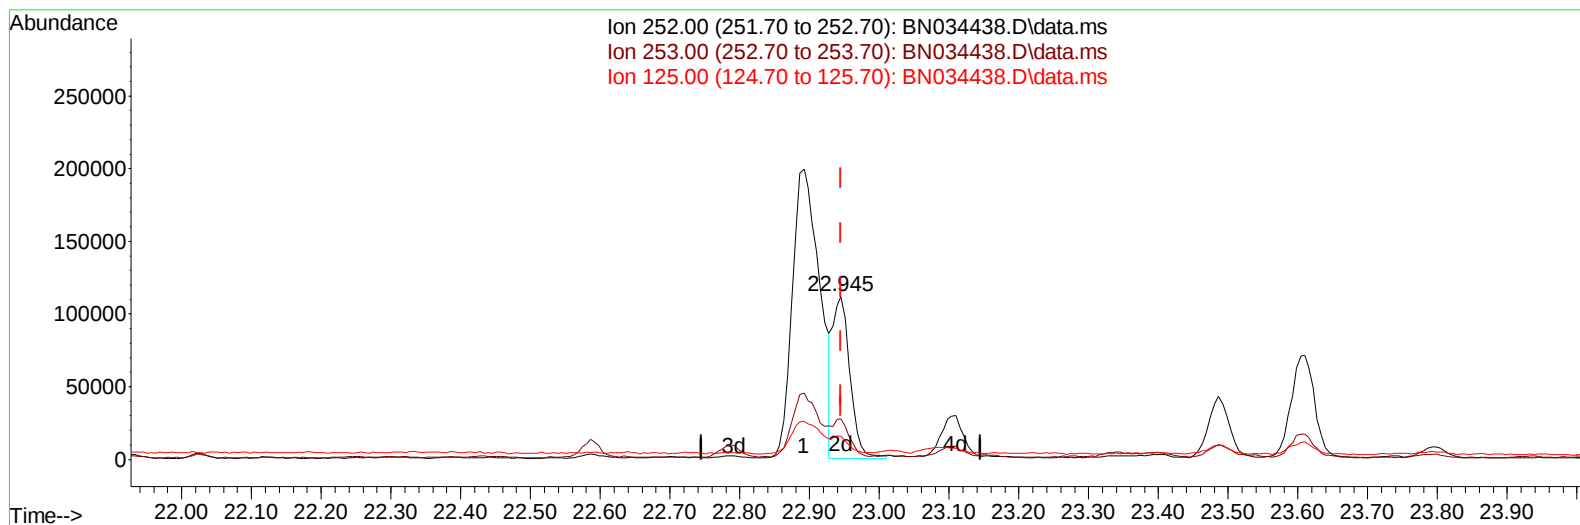

TIC: BN034438.D\data.ms

(91) Benzo(k)fluoranthene

22.945min (+ 0.000) 3.80 ng/u1 m

response 192880

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.70	25.13
125.00	11.00	14.33#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
 Data File : BN034438.D
 Acq On : 07 Oct 2024 14:59
 Operator : RC/JU
 Sample : P4109-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4EH7

Manual IntegrationsAPPROVED

Quant Time: Oct 07 15:41:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 30 14:14:38 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
 Supervised By :mohammad ahmed 10/09/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.375	152		145580	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.134	136		568231	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.028	164		363878	20.000	ng/ul	-0.01
64) Phenanthrene-d10	16.787	188		783400	20.000	ng/ul	-0.01
79) Chrysene-d12	21.027	240		798775	20.000	ng/ul	0.00
88) Perylene-d12	23.733	264		844881	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	2.993	96		7059	1.979	ng/uL	0.00
4) Pyridine-d5	3.411	84		7812m	0.737	ng/ul	0.02
7) Phenol-d5	6.581	99		128978	9.983	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.734	67		80179	10.002	ng/ul	0.00
11) 2-Chlorophenol-d4	6.916	132		117960	11.599	ng/ul	-0.01
15) 4-Methylphenol-d8	8.093	113		93979	8.840	ng/ul	-0.01
21) Nitrobenzene-d5	8.522	128		53026	11.708	ng/ul	0.00
24) 2-Nitrophenol-d4	9.234	143		57253	12.293	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.769	165		106222	12.110	ng/ul	0.00
31) 4-Chloroaniline-d4	10.287	131		77533	5.839	ng/ul	0.00
46) Dimethylphthalate-d6	13.457	166		341286	12.550	ng/ul	-0.01
49) Acenaphthylene-d8	13.716	160		380994	12.454	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.269	143		32589	5.839	ng/ul	0.00
60) Fluorene-d10	15.034	176		305337	13.249	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.169	200		32434	6.944	ng/ul	0.00
73) Anthracene-d10	16.887	188		486118	13.199	ng/ul	-0.01
81) Pyrene-d10	19.198	212		497005	11.167	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.545	264		346075	7.974	ng/ul	-0.01
Target Compounds							
						Qvalue	
16) Acetophenone	8.193	105		40380	2.398	ng/ul#	91
30) Naphthalene	10.181	128		38696	1.245	ng/ul	99
52) Acenaphthene	14.093	153		27567	1.153	ng/ul	97
61) Fluorene	15.087	166		32814	1.227	ng/ul	93
72) Phenanthrene	16.828	178		550512	12.744	ng/ul	99
74) Anthracene	16.922	178		103824	2.354	ng/ul	98
77) Carbazole	17.198	167		53955	1.329	ng/ul	99
80) Fluoranthene	18.863	202		898229	17.264	ng/ul	99
82) Pyrene	19.228	202		594516	10.629	ng/ul	96
83) Butylbenzylphthalate	20.169	149		51590	2.057	ng/ul	100
85) Benzo(a)anthracene	21.010	228		422080	7.411	ng/ul	95
86) Bis(2-ethylhexyl)phtha...	20.975	149		365251	9.948	ng/ul#	97
87) Chrysene	21.063	228		432792	7.964	ng/ul	94
90) Benzo(b)fluoranthene	22.892	252		541818	10.518	ng/ul	97
91) Benzo(k)fluoranthene	22.945	252		192880m	3.796	ng/ul	
93) Benzo(a)pyrene	23.610	252		162980	3.349	ng/ul#	89
94) Indeno(1,2,3-cd)pyrene	26.715	276		151599	2.514	ng/ul	97
95) Dibenzo(a,h)anthracene	26.762	278		57939	1.189	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

