

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
 Data File : BN034443.D
 Acq On : 07 Oct 2024 18:15
 Operator : RC/JU
 Sample : PB163651BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK651

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.999	15	19	29	rVB	59638	84222	2.51%	0.193%
2	3.381	81	84	102	rBV	634401	958039	28.57%	2.192%
3	3.687	131	136	140	rBV	14912	19838	0.59%	0.045%
4	4.128	208	211	216	rBV6	5890	12697	0.38%	0.029%
5	5.158	382	386	388	rBV5	4107	4507	0.13%	0.010%
6	5.987	523	527	528	rBV3	3867	4295	0.13%	0.010%
7	6.452	605	606	612	rVB5	1952	3461	0.10%	0.008%
8	6.581	620	628	643	rBV	740872	1206595	35.98%	2.761%
9	6.734	648	654	664	rVV	658073	978377	29.17%	2.239%
10	6.917	679	685	698	rBV	861499	1315269	39.22%	3.010%
11	7.022	701	703	706	rVV4	3518	3820	0.11%	0.009%
12	7.234	736	739	743	rBV5	2309	3581	0.11%	0.008%
13	7.375	757	763	773	rBV	842949	1295697	38.63%	2.965%
14	8.093	878	885	902	rBV	942416	1508878	44.99%	3.453%
15	8.328	919	925	926	rBV5	3310	5193	0.15%	0.012%
16	8.522	951	958	968	rBV	698606	1160602	34.60%	2.656%
17	8.963	1027	1033	1038	rVV2	12498	21196	0.63%	0.048%
18	9.234	1071	1079	1093	rBV	595933	984799	29.36%	2.253%
19	9.769	1163	1170	1184	rBV	898812	1541502	45.96%	3.527%
20	10.134	1224	1232	1240	rVB	1090928	1799056	53.64%	4.116%
21	10.281	1250	1257	1279	rBV	856729	1515544	45.19%	3.468%
22	11.446	1449	1455	1463	rBV3	9083	16629	0.50%	0.038%
23	11.740	1498	1505	1511	rBV2	12679	25734	0.77%	0.059%
24	13.457	1791	1797	1811	rBV	1492816	2069976	61.72%	4.736%
25	13.716	1834	1841	1851	rBV	1802246	2615053	77.97%	5.984%
26	14.028	1887	1894	1909	rBV	1556676	2280574	68.00%	5.218%
27	14.269	1928	1935	1953	rBV	369933	769265	22.94%	1.760%
28	15.034	2058	2065	2082	rBV	2224810	3134341	93.45%	7.172%
29	15.169	2082	2088	2103	rVV	551853	778760	23.22%	1.782%
30	15.275	2103	2106	2111	rVB2	11253	16414	0.49%	0.038%
31	15.604	2159	2162	2166	rBV6	2662	3649	0.11%	0.008%
32	15.828	2197	2200	2203	rBV5	2293	3687	0.11%	0.008%
33	16.316	2280	2283	2290	rBV7	3695	6612	0.20%	0.015%
34	16.575	2324	2327	2330	rVB4	3083	3888	0.12%	0.009%
35	16.787	2357	2363	2374	rBV	1728590	2514152	74.96%	5.753%
36	16.887	2374	2380	2396	rVV2	2277684	3179405	94.80%	7.275%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034443.D
Acq On : 07 Oct 2024 18:15
Operator : RC/JU
Sample : PB163651BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK651

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION

37	17.522	2486	2488	2492	rBV5	2713	3592	0.11%	0.008%
38	17.745	2517	2526	2529	rBV10	6019	14626	0.44%	0.033%
39	18.022	2571	2573	2576	rBV4	3173	3930	0.12%	0.009%
40	18.757	2694	2698	2705	rVB2	28174	40913	1.22%	0.094%
41	18.834	2707	2711	2715	rVV2	23252	32351	0.96%	0.074%
42	19.198	2767	2773	2786	rBV2	2409225	3353882	100.00%	7.674%
43	21.028	3079	3084	3094	rBV2	1723142	2379286	70.94%	5.444%
44	23.551	3505	3513	3525	rBV	1470961	3335452	99.45%	7.632%
45	23.733	3537	3544	3564	rVB	1162105	2694292	80.33%	6.165%

Sum of corrected areas: 43703631




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034443.D
Acq On : 07 Oct 2024 18:15
Operator : RC/JU
Sample : PB163651BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK651

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

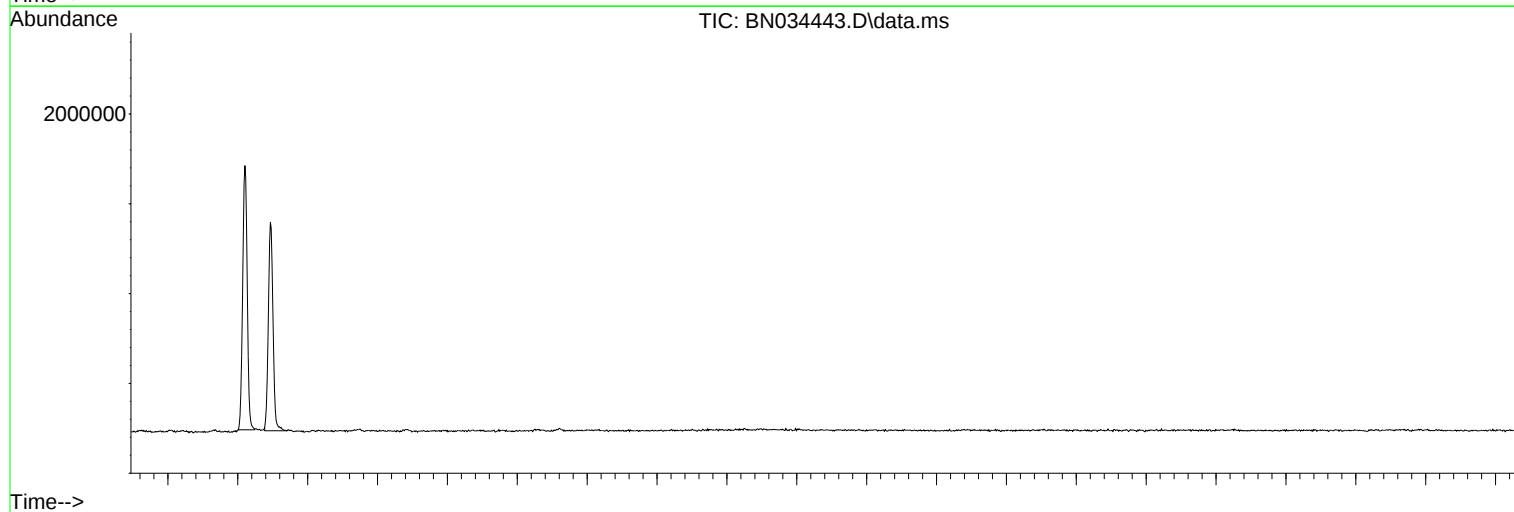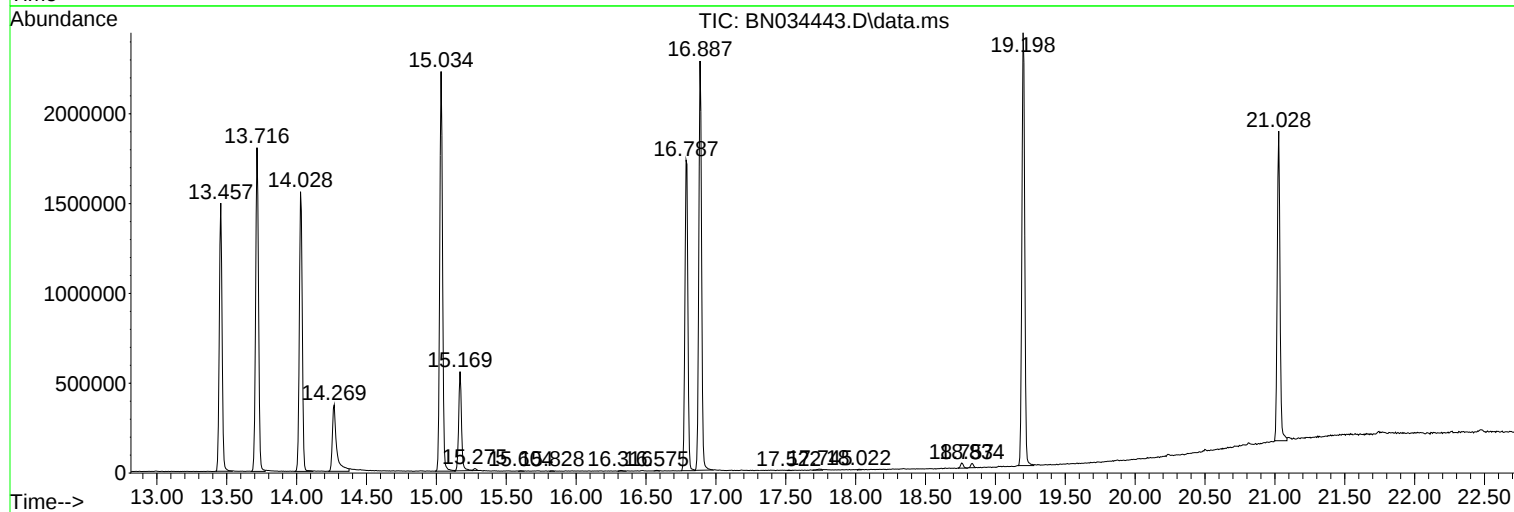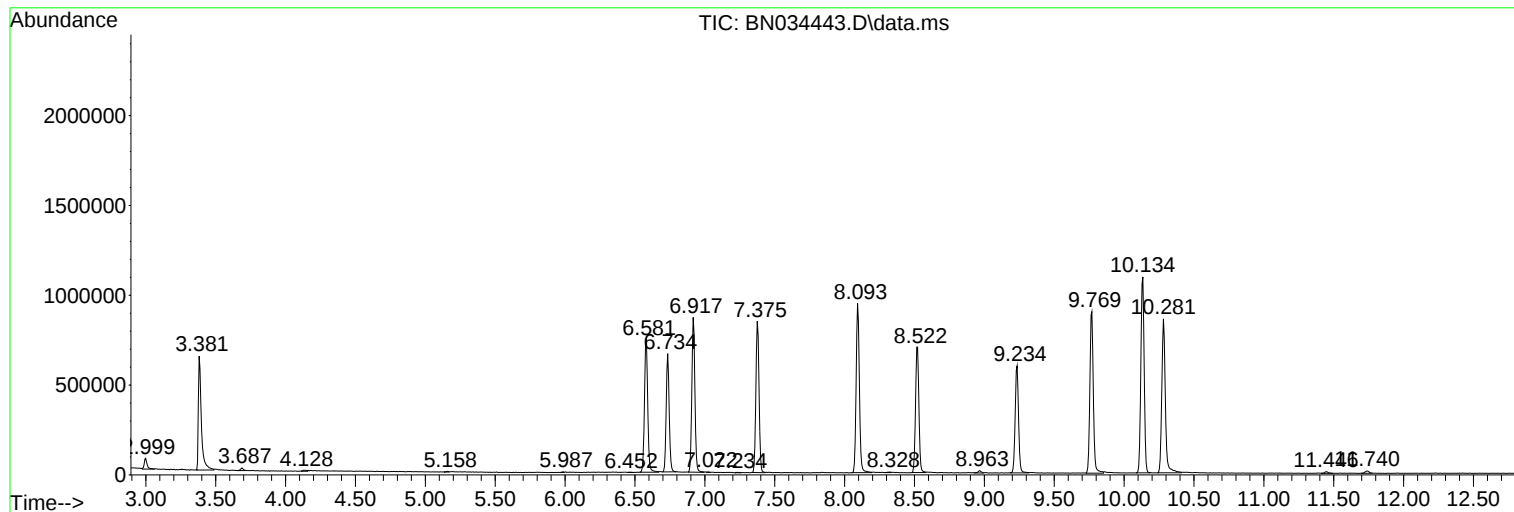

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034443.D
Acq On : 07 Oct 2024 18:15
Operator : RC/JU
Sample : PB163651BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK651

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034443.D
Acq On : 07 Oct 2024 18:15
Operator : RC/JU
Sample : PB163651BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK651

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
