

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
 Data File : BN034458.D
 Acq On : 08 Oct 2024 04:44
 Operator : RC/JU
 Sample : PB163680BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK680

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034458.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.993	15	18	27	rVB	64187	86500	2.26%	0.174%
2	3.381	80	84	100	rBV	761165	1100574	28.71%	2.210%
3	3.687	131	136	142	rBV	13714	21166	0.55%	0.043%
4	6.146	551	554	558	rBV4	2343	5010	0.13%	0.010%
5	6.581	619	628	638	rBV	914394	1429440	37.29%	2.871%
6	6.734	648	654	665	rVB	787744	1151248	30.03%	2.312%
7	6.916	678	685	697	rBV	1014920	1546564	40.35%	3.106%
8	7.375	756	763	772	rBV	950000	1433574	37.40%	2.879%
9	8.093	879	885	901	rBV	1131763	1815637	47.37%	3.646%
10	8.522	950	958	969	rBV	871248	1406037	36.68%	2.824%
11	8.963	1030	1033	1039	rVB8	2652	4857	0.13%	0.010%
12	9.234	1071	1079	1090	rBV	741277	1204802	31.43%	2.420%
13	9.310	1090	1092	1097	rVV5	4121	5645	0.15%	0.011%
14	9.769	1162	1170	1182	rBV	1121359	1868068	48.73%	3.752%
15	10.134	1224	1232	1245	rVB	1235348	2034714	53.08%	4.086%
16	10.281	1247	1257	1280	rBV	1047188	1862184	48.58%	3.740%
17	11.740	1498	1505	1511	rBV4	16506	33174	0.87%	0.067%
18	13.457	1790	1797	1805	rBV	1750581	2481124	64.73%	4.983%
19	13.716	1834	1841	1855	rBV	2130548	3130112	81.66%	6.286%
20	14.028	1888	1894	1902	rBV	1726467	2562159	66.84%	5.146%
21	14.269	1928	1935	1953	rBV	480528	934006	24.37%	1.876%
22	15.033	2059	2065	2079	rBV	2505539	3653978	95.33%	7.338%
23	15.169	2083	2088	2102	rVV	533877	755499	19.71%	1.517%
24	15.269	2102	2105	2110	rVB3	14780	24272	0.63%	0.049%
25	16.469	2306	2309	2312	rVB3	3649	4214	0.11%	0.008%
26	16.575	2323	2327	2333	rVB3	4068	4598	0.12%	0.009%
27	16.786	2357	2363	2374	rBV	1899911	2672482	69.72%	5.367%
28	16.886	2374	2380	2398	rVB2	2565323	3577796	93.34%	7.185%
29	17.075	2409	2412	2413	rBV3	4988	4729	0.12%	0.009%
30	17.739	2520	2525	2529	rBV8	3526	7804	0.20%	0.016%
31	18.033	2570	2575	2578	rBV7	5058	9124	0.24%	0.018%
32	18.763	2694	2699	2702	rBV3	29026	38475	1.00%	0.077%
33	18.833	2706	2711	2717	rBV	30418	43040	1.12%	0.086%
34	19.198	2767	2773	2785	rBV2	2697982	3650442	95.23%	7.331%
35	21.021	3078	3083	3094	rBV2	1785040	2460107	64.18%	4.941%
36	23.551	3505	3513	3526	rVB	1760246	3833156	100.00%	7.698%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034458.D
Acq On : 08 Oct 2024 04:44
Operator : RC/JU
Sample : PB163680BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK680

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION

37	23.733	3536	3544	3560	rVB	1232673	2936587	76.61%	5.898%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 49792898

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034458.D
Acq On : 08 Oct 2024 04:44
Operator : RC/JU
Sample : PB163680BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK680

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

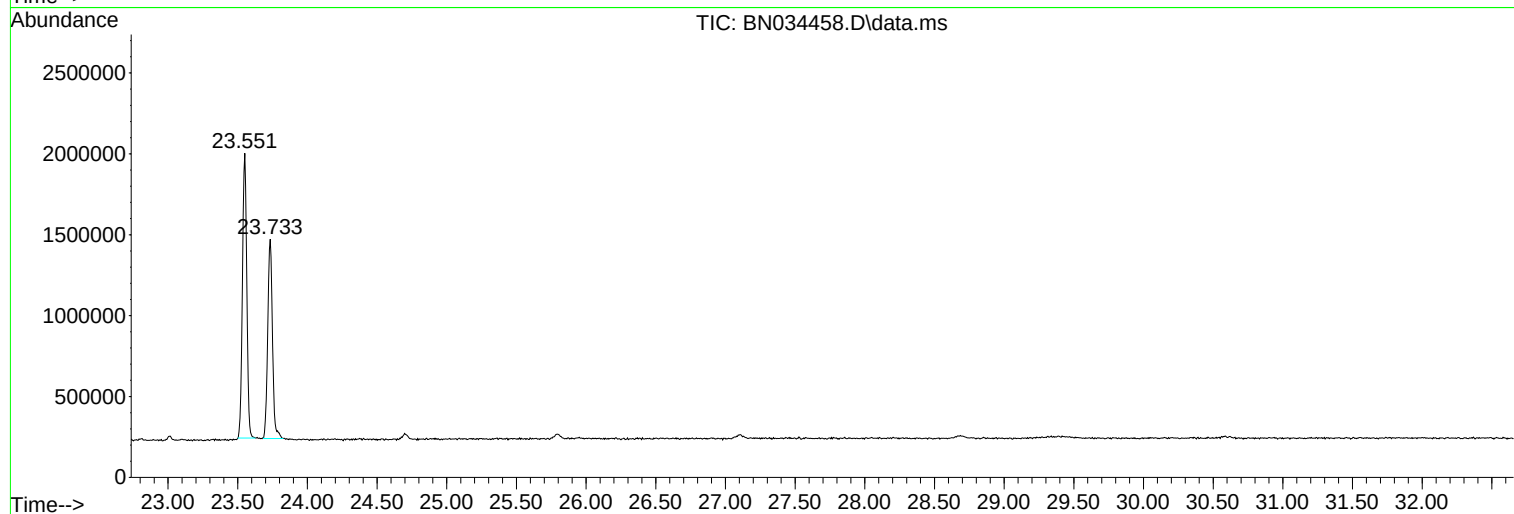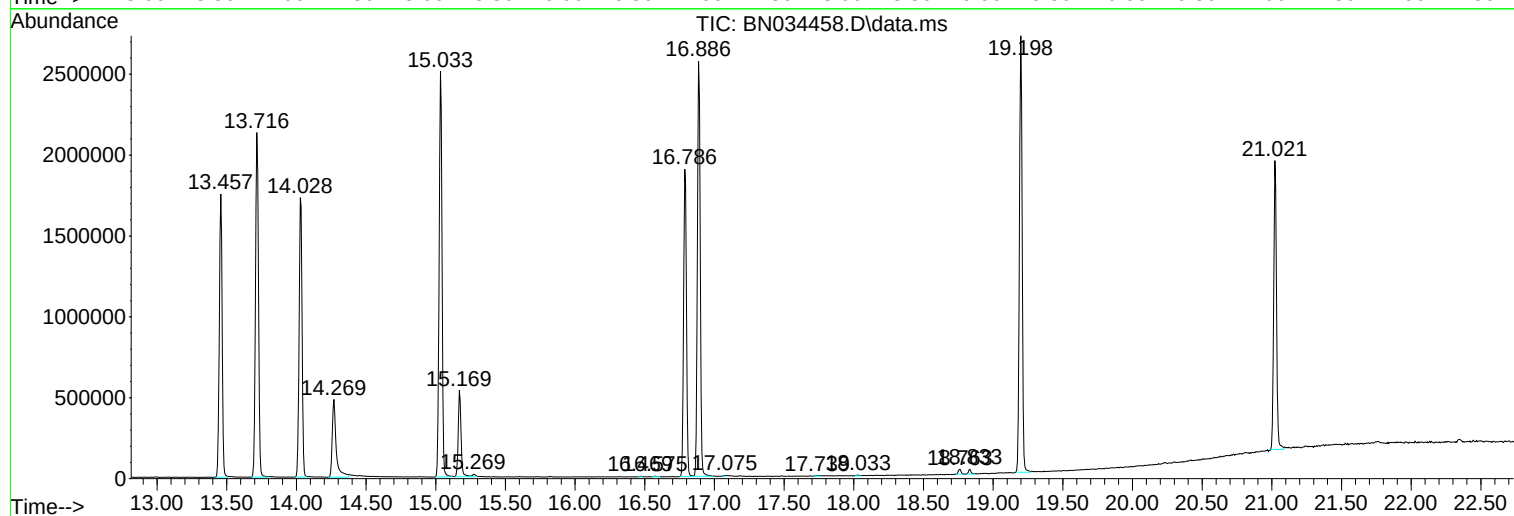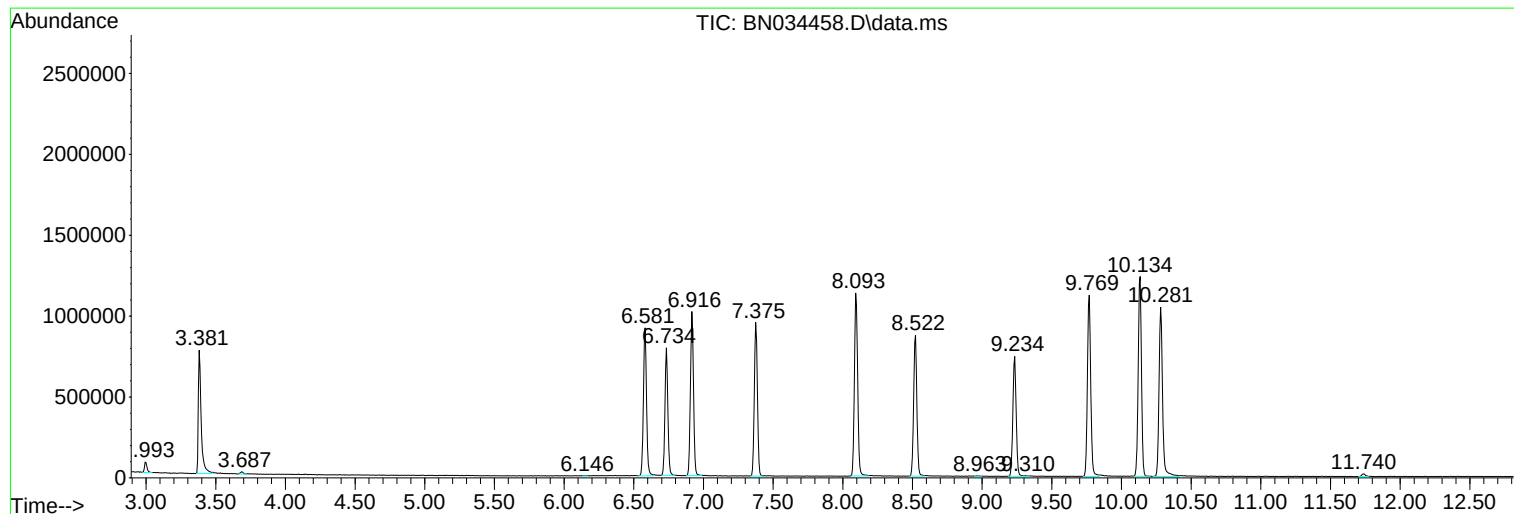

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034458.D
Acq On : 08 Oct 2024 04:44
Operator : RC/JU
Sample : PB163680BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK680

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034458.D
Acq On : 08 Oct 2024 04:44
Operator : RC/JU
Sample : PB163680BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK680

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc