

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
 Data File : BN034460.D
 Acq On : 08 Oct 2024 06:03
 Operator : RC/JU
 Sample : P4187-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EY045

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.999	15	19	22	rBV	48631	58190	1.28%	0.121%
2	3.028	22	24	29	rVB	19012	23530	0.52%	0.049%
3	3.387	81	85	101	rBV	274806	430821	9.49%	0.897%
4	3.687	133	136	141	rVB	17044	20920	0.46%	0.044%
5	4.040	194	196	200	rVB4	4975	6067	0.13%	0.013%
6	4.117	207	209	214	rVB3	6218	7867	0.17%	0.016%
7	4.187	216	221	232	rVB	127175	196862	4.34%	0.410%
8	4.446	261	265	270	rVB	12179	16716	0.37%	0.035%
9	4.564	281	285	292	rBV3	13658	25215	0.56%	0.053%
10	4.911	341	344	348	rVB5	3553	5262	0.12%	0.011%
11	5.675	468	474	480	rVB	27744	42408	0.93%	0.088%
12	5.975	521	525	529	rVB5	4594	5879	0.13%	0.012%
13	6.581	619	628	640	rBV	303271	495449	10.91%	1.032%
14	6.734	647	654	664	rBV	764041	1159905	25.54%	2.416%
15	6.916	678	685	697	rBV	934656	1442994	31.78%	3.006%
16	7.016	700	702	707	rVB5	7038	7977	0.18%	0.017%
17	7.375	756	763	772	rVV	863533	1318630	29.04%	2.747%
18	7.458	775	777	786	rVB7	5876	10852	0.24%	0.023%
19	7.634	801	807	809	rBV3	8792	12774	0.28%	0.027%
20	7.740	820	825	830	rVB7	9403	15714	0.35%	0.033%
21	7.863	840	846	850	rVB7	6419	9543	0.21%	0.020%
22	8.093	878	885	897	rBV	775915	1258547	27.71%	2.622%
23	8.522	950	958	969	rBV	853653	1384276	30.48%	2.883%
24	8.957	1028	1032	1039	rBV6	6303	11066	0.24%	0.023%
25	9.110	1054	1058	1062	rBV6	3485	5651	0.12%	0.012%
26	9.234	1071	1079	1094	rBV	724792	1195853	26.33%	2.491%
27	9.422	1107	1111	1112	rBV4	4782	5845	0.13%	0.012%
28	9.769	1162	1170	1179	rBV	1075475	1804499	39.74%	3.759%
29	10.134	1224	1232	1241	rBV	1071034	1803672	39.72%	3.757%
30	10.281	1249	1257	1276	rBV	883537	1559059	34.33%	3.247%
31	11.546	1466	1472	1480	rVB10	6704	15945	0.35%	0.033%
32	11.734	1499	1504	1511	rBV	16881	31833	0.70%	0.066%
33	12.640	1650	1658	1664	rVB5	5304	9714	0.21%	0.020%
34	12.746	1671	1676	1682	rBV10	3015	5756	0.13%	0.012%
35	13.457	1790	1797	1808	rBV	1877787	2538517	55.90%	5.288%
36	13.528	1808	1809	1816	rVB6	4536	5185	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
 Data File : BN034460.D
 Acq On : 08 Oct 2024 06:03
 Operator : RC/JU
 Sample : P4187-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EY045

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

37	13.716	1835	1841	1853	rBV2	1997897	2998152	66.02%	6.245%
38	13.963	1878	1883	1886	rBV7	4051	6008	0.13%	0.013%
39	14.028	1888	1894	1906	rBV	1530303	2234865	49.21%	4.655%
40	14.275	1929	1936	1950	rBV	116261	275359	6.06%	0.574%
41	14.487	1968	1972	1979	rVB9	5514	11591	0.26%	0.024%
42	14.734	2011	2014	2017	rBV5	3085	4623	0.10%	0.010%
43	14.863	2031	2036	2044	rBV4	10126	17481	0.38%	0.036%
44	15.034	2059	2065	2080	rBV	2687893	3717431	81.86%	7.743%
45	15.169	2082	2088	2102	rVV	691533	970862	21.38%	2.022%
46	15.275	2102	2106	2114	rVB2	15671	31950	0.70%	0.067%
47	15.416	2125	2130	2136	rBV	54151	75093	1.65%	0.156%
48	15.610	2159	2163	2167	rBV8	3302	5817	0.13%	0.012%
49	15.728	2179	2183	2187	rBV5	2554	5019	0.11%	0.010%
50	16.469	2305	2309	2313	rVB3	4979	7061	0.16%	0.015%
51	16.575	2324	2327	2331	rBV4	3266	5692	0.13%	0.012%
52	16.787	2356	2363	2373	rBV	1644464	2382697	52.47%	4.963%
53	16.887	2373	2380	2398	rVV2	2774164	3934939	86.65%	8.196%
54	17.057	2405	2409	2414	rBV2	4859	10571	0.23%	0.022%
55	17.110	2414	2418	2422	rVB	8138	12977	0.29%	0.027%
56	17.722	2517	2522	2530	rBV2	88332	151336	3.33%	0.315%
57	18.028	2570	2574	2578	rVB5	8963	11891	0.26%	0.025%
58	18.322	2622	2624	2630	rVB7	4386	6350	0.14%	0.013%
59	18.533	2658	2660	2663	rBV4	3744	4757	0.10%	0.010%
60	18.757	2693	2698	2703	rBV3	37763	54002	1.19%	0.112%
61	18.833	2706	2711	2715	rBV	34649	49495	1.09%	0.103%
62	18.928	2725	2727	2731	rVB5	6011	7795	0.17%	0.016%
63	19.022	2739	2743	2753	rBV3	53961	93647	2.06%	0.195%
64	19.198	2767	2773	2782	rBV	3134036	4220022	92.93%	8.790%
65	20.763	3036	3039	3044	rBV4	39762	52188	1.15%	0.109%
66	21.022	3078	3083	3095	rBV	1685011	2342922	51.59%	4.880%
67	23.545	3504	3512	3527	rBV	2111232	4541082	100.00%	9.459%
68	23.727	3536	3543	3560	rVB	1251010	2815445	62.00%	5.865%


Sum of corrected areas: 48008113

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034460.D
Acq On : 08 Oct 2024 06:03
Operator : RC/JU
Sample : P4187-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EY045

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

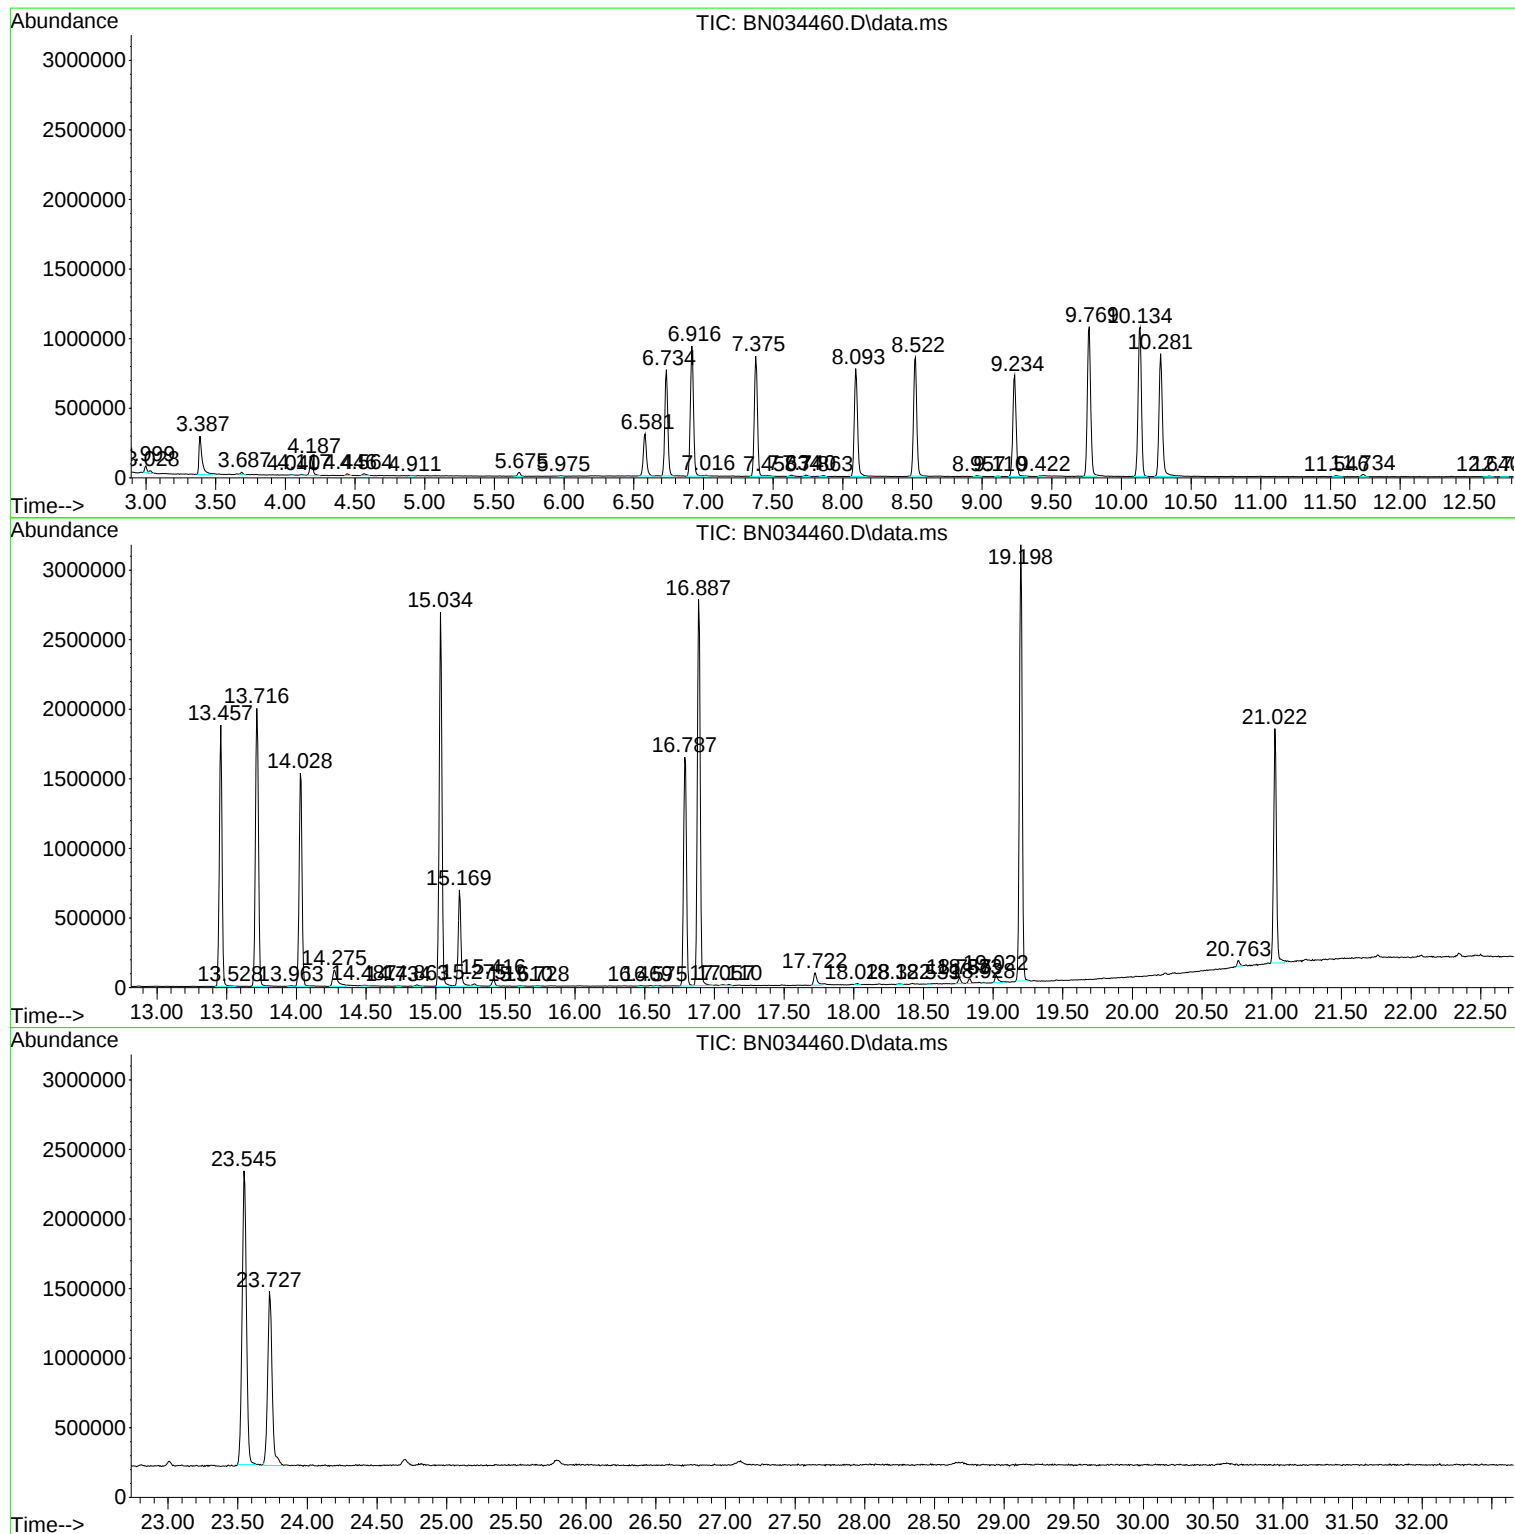

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034460.D
Acq On : 08 Oct 2024 06:03
Operator : RC/JU
Sample : P4187-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EY045










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.187	2.99 ng/ul	196862	1,4-Dichlorobenzene-d4	7.375

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	35

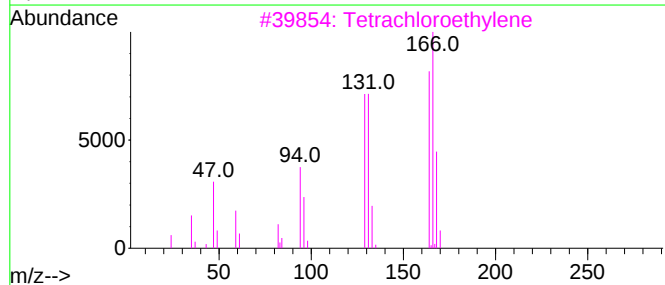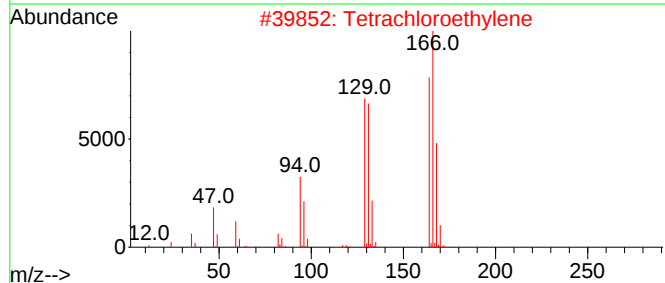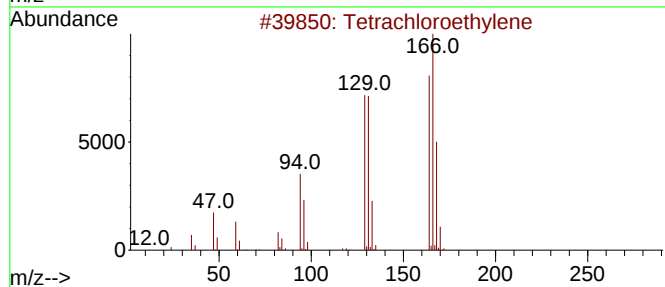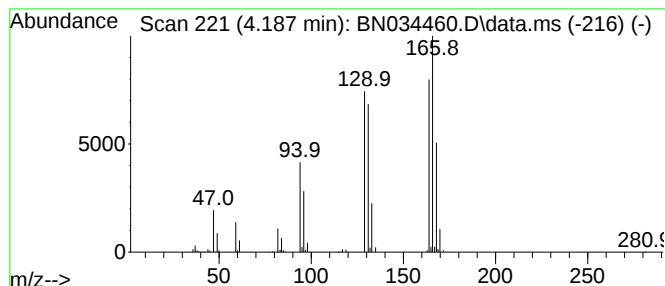

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100724\
Data File : BN034460.D
Acq On : 08 Oct 2024 06:03
Operator : RC/JU
Sample : P4187-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EY045

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.187	3.0	ng/u1	196862	1	7.375	1318630	20.0