

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100820\
 Data File : BN012108.D
 Acq On : 08 Oct 2020 18:32
 Operator : CG/JU
 Sample : L4209-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLWT0

Quant Time: Oct 09 01:16:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 08 15:35:30 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	262378	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1073700	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	684788	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1442646	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	1452421	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	1493721	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	8328	1.38	ng/uL	0.00
5) Phenol-d5	6.82	99	9471	0.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	327342	24.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	244101	13.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	30250	1.75	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	217819	25.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	221010	23.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	306456	17.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	1445	0.07	ng/ul	0.02
44) Dimethylphthalate-d6	13.70	166	1564937	29.13	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	543421	8.48	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	37382	3.78	ng/ul	0.00
58) Fluorene-d10	15.28	176	1236602	26.38	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	234002	25.41	ng/ul	0.00
71) Anthracene-d10	17.13	188	1171493	16.75	ng/ul	0.00
79) Pyrene-d10	19.43	212	1522783	19.93	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	1692541	20.19	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.75	163	126858	2.292	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100820\
Data File : BN012108.D
Acq On : 08 Oct 2020 18:32
Operator : CG/JU
Sample : L4209-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLWT0

Quant Time: Oct 09 01:16:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 08 15:35:30 2020
Response via : Initial Calibration

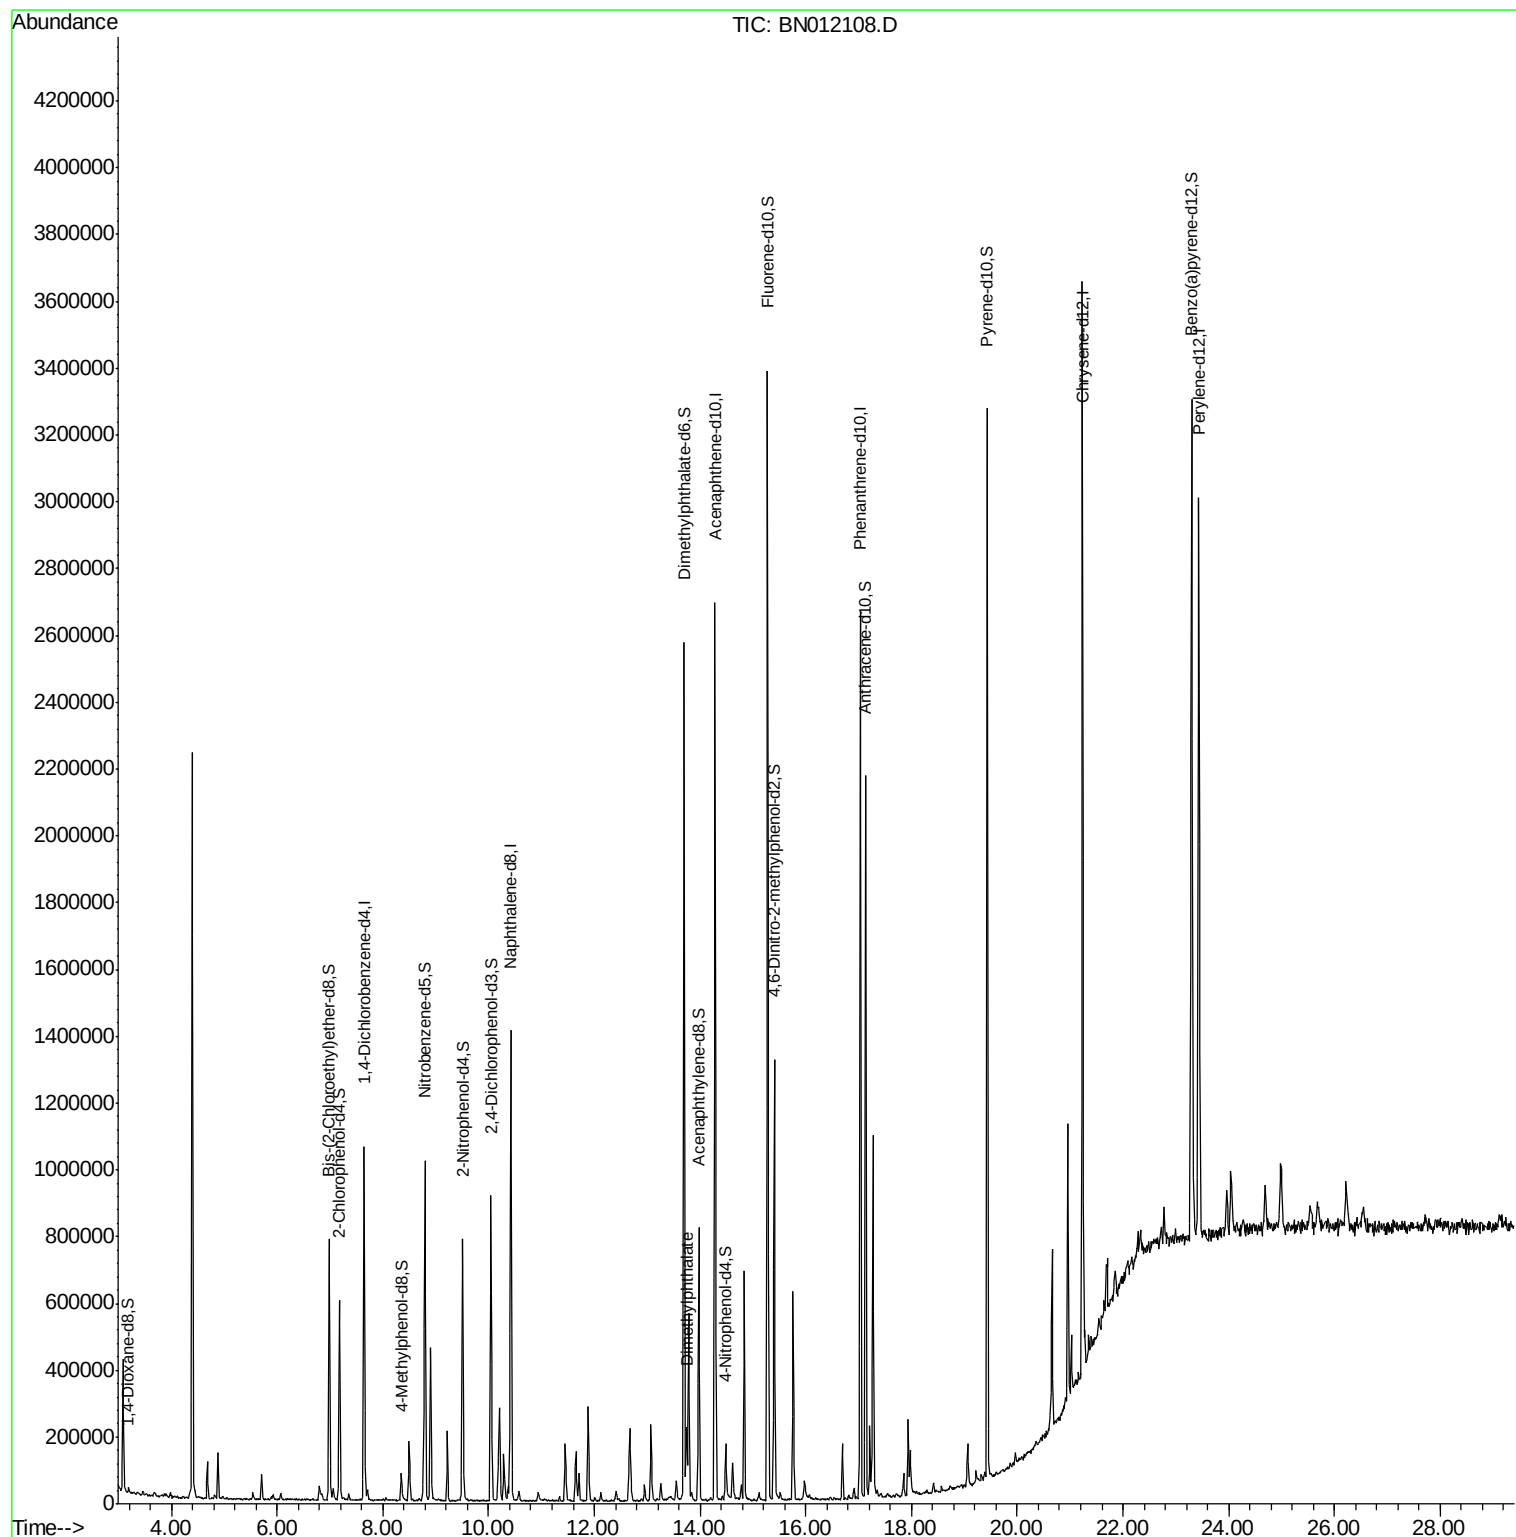

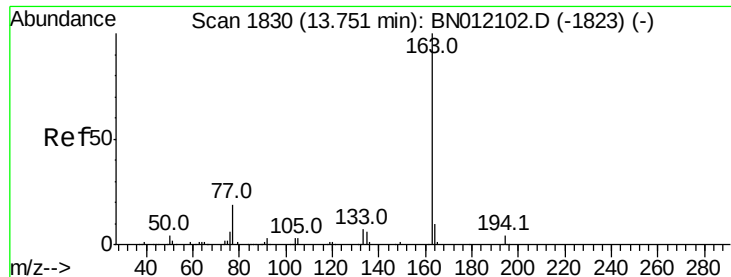

#45

Dimethylphthalate

Concen: 2.292 ng/ul

RT: 13.75 min Scan# 1829

Delta R.T. -0.01 min

Lab File: BN012108.D

Acq: 08 Oct 2020 18:32

Instrument :

BNA_N

ClientSampleId :

JLWT0


Tot Ion:163 Resp: 126858

Ion Ratio Lower Upper

163 100

194 3.5 3.4 5.0

164 10.8 7.8 11.8

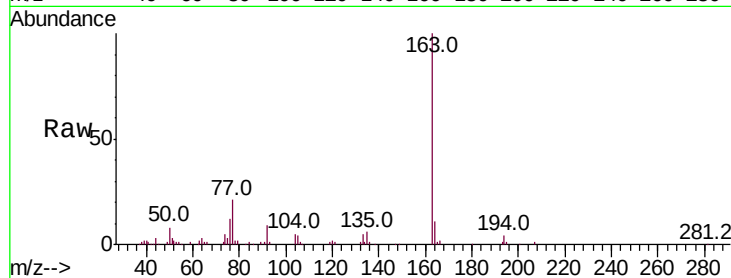

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

