

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100820\
 Data File : BN012108.D
 Acq On : 08 Oct 2020 18:32
 Operator : CG/JU
 Sample : L4209-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLWTO

Quant Time: Oct 09 01:15:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 08 15:35:30 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.646	152	262378	20.00	ng/ul	0.00
18) Naphthalene-d8	10.422	136	1073700	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.287	164	684788	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.033	188	1442646	20.00	ng/ul	0.00
78) Chrysene-d12	21.233	240	1452421	20.00	ng/ul	0.00
86) Perylene-d12	23.439	264	1493721	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	8328	1.38	ng/uL	0.00
5) Phenol-d5	6.822	99	9471	0.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	6.987	67	327342	24.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.181	132	244101	13.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.346	113	30250	1.75	ng/ul	0.00
19) Nitrobenzene-d5	8.793	128	217819	25.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.510	143	221010	23.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.046	165	306456	17.33	ng/ul	0.00
29) 4-Chloroaniline-d4	0.000	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	13.698	166	1564937	29.13	ng/ul	0.00
47) Acenaphthylene-d8	13.975	160	543421	8.48	ng/ul	0.00
52) 4-Nitrophenol-d4	14.487	143	37382	3.78	ng/ul	0.00
58) Fluorene-d10	15.281	176	1236602	26.38	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.404	200	234002	25.41	ng/ul	0.00
71) Anthracene-d10	17.133	188	1171493	16.75	ng/ul	0.00
79) Pyrene-d10	19.433	212	1522783	19.93	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.298	264	1692541	20.19	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.745	163	126858	2.29	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100820\
Data File : BN012108.D
Acq On : 08 Oct 2020 18:32
Operator : CG/JU
Sample : L4209-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLWTO

Quant Time: Oct 09 01:15:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 08 15:35:30 2020
Response via : Initial Calibration

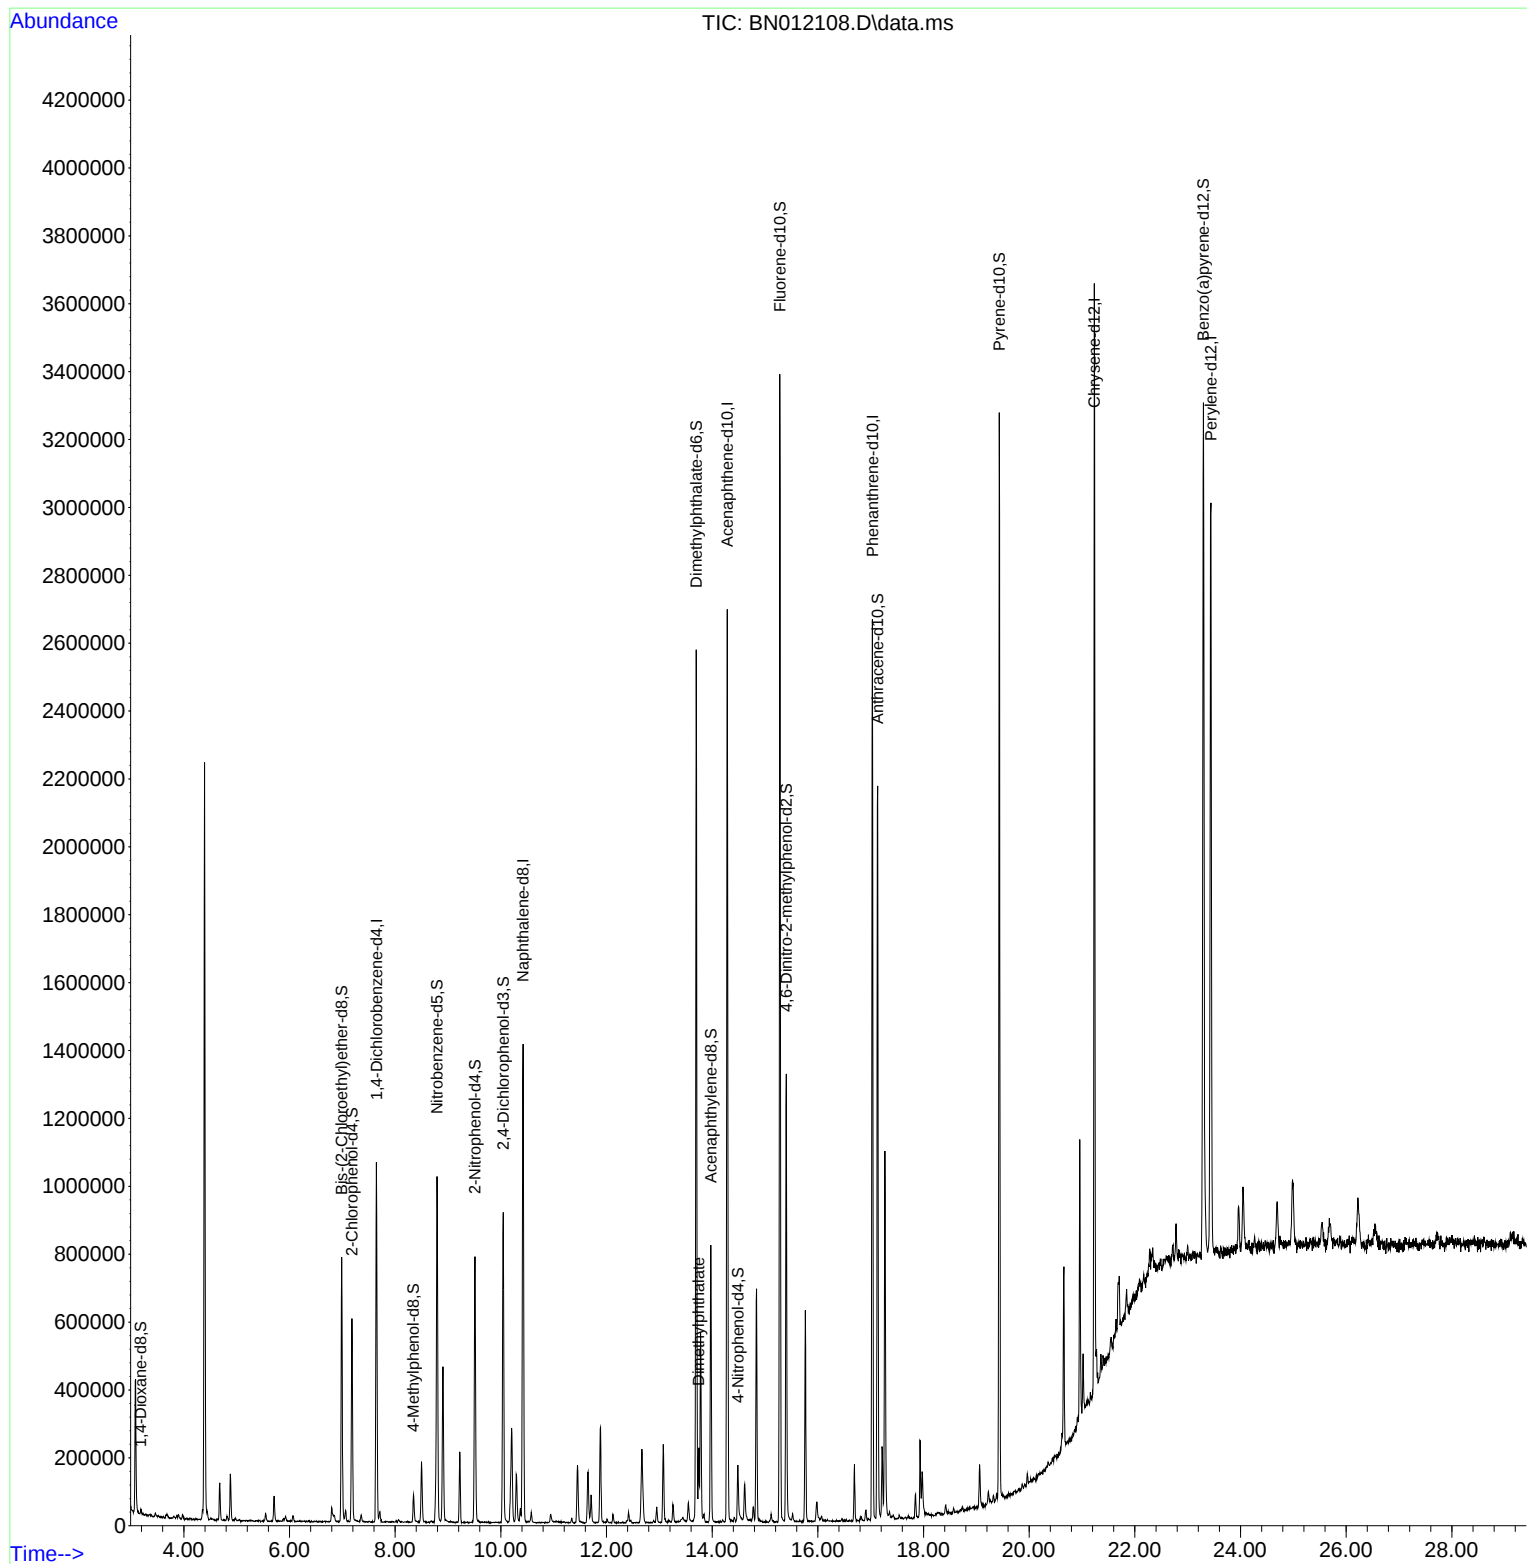

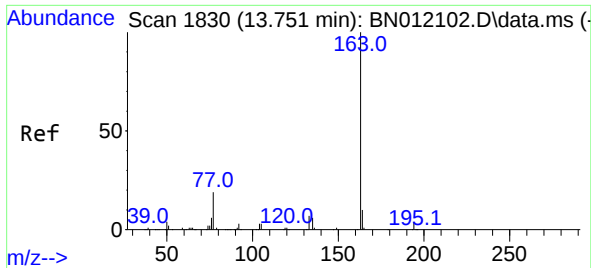

#45
 Dimethylphthalate
 Concen: 2.29 ng/ul
 RT: 13.745 min Scan# 1829
 Delta R.T. -0.006 min
 Lab File: BN012108.D
 Acq: 08 Oct 2020 18:32

Instrument :
 BNA_N
 ClientSampleId :
 JLWT0

Tgt Ion:163 Resp: 126858
 Ion Ratio Lower Upper
 163 100
 194 3.5 3.4 5.0
 164 10.8 7.8 11.8

