

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100820\
 Data File : BN012115.D
 Acq On : 08 Oct 2020 22:46
 Operator : CG/JU
 Sample : L4259-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C5CF8

Quant Time: Oct 09 01:16:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 08 15:35:30 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.645	152	244592	20.00	ng/ul	0.00
18) Naphthalene-d8	10.422	136	1026821	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.286	164	641840	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.033	188	1344488	20.00	ng/ul	0.00
78) Chrysene-d12	21.233	240	1334475	20.00	ng/ul	0.00
86) Perylene-d12	23.433	264	1423151	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	8296	1.48	ng/uL	0.00
5) Phenol-d5	6.822	99	137789	6.75	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	6.987	67	357124	28.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.181	132	392690	23.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.345	113	263473	16.40	ng/ul	0.00
19) Nitrobenzene-d5	8.792	128	245961	30.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.510	143	281757	31.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.039	165	492585	29.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.569	131	19058	0.96	ng/ul	0.01
44) Dimethylphthalate-d6	13.698	166	1856488	36.87	ng/ul	0.00
47) Acenaphthylene-d8	13.975	160	2027981	33.75	ng/ul	0.00
52) 4-Nitrophenol-d4	14.486	143	62362	6.73	ng/ul	0.00
58) Fluorene-d10	15.280	176	1507399	34.31	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.404	200	304700	35.51	ng/ul	0.00
71) Anthracene-d10	17.133	188	2459332	37.72	ng/ul	0.00
79) Pyrene-d10	19.433	212	2683854	38.24	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.298	264	2995728	37.51	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.745	163	62816	1.21	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100820\
Data File : BN012115.D
Acq On : 08 Oct 2020 22:46
Operator : CG/JU
Sample : L4259-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C5CF8


Quant Time: Oct 09 01:16:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 08 15:35:30 2020
Response via : Initial Calibration

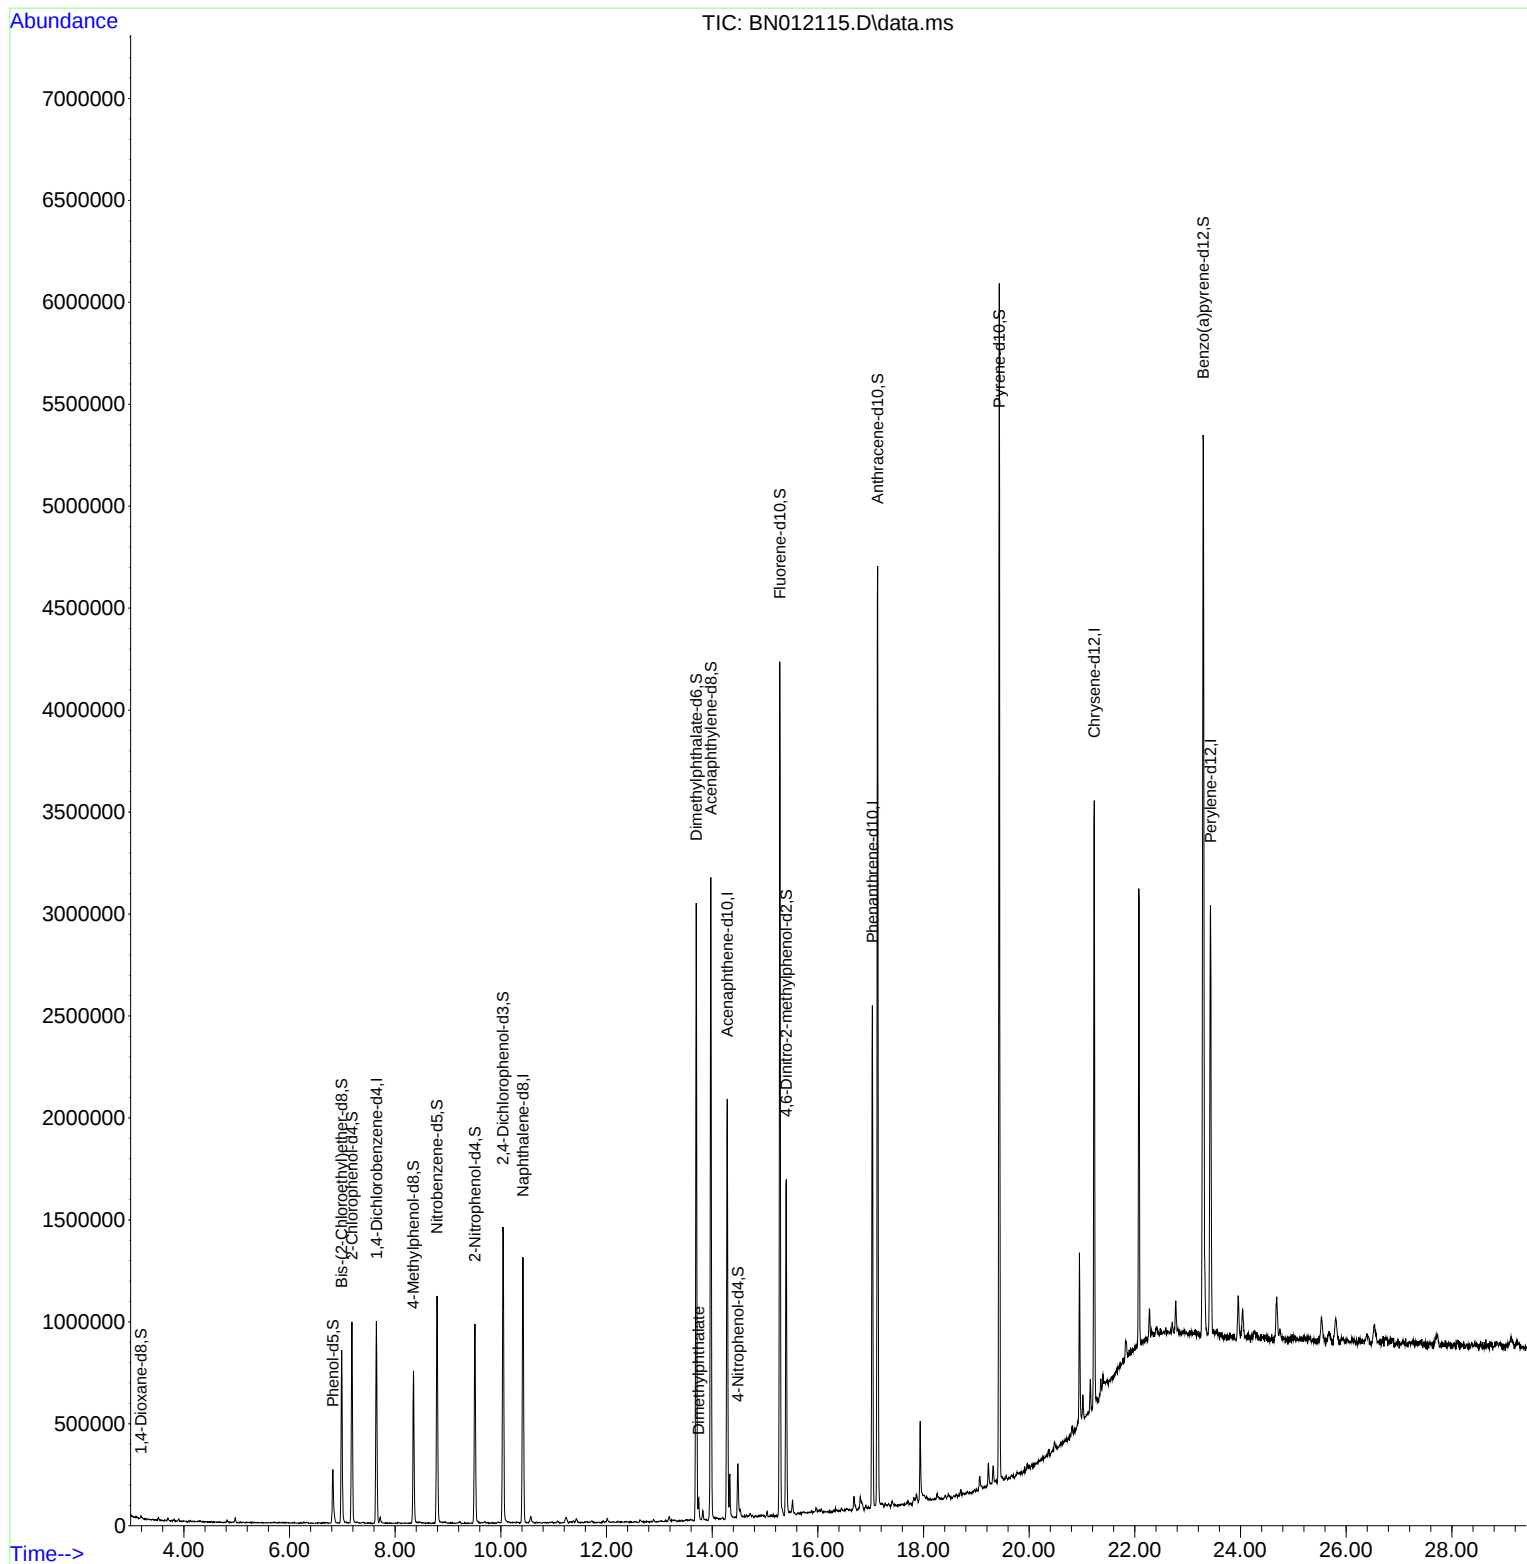

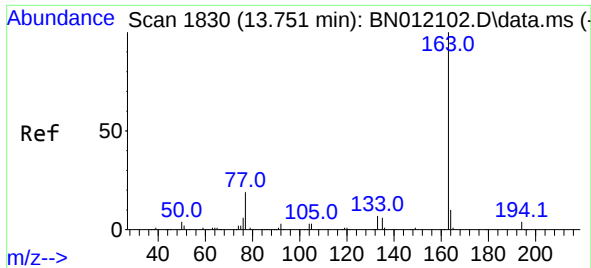

#45
Dimethylphthalate
Concen: 1.21 ng/ul
RT: 13.745 min Scan# 1829
Delta R.T. -0.006 min
Lab File: BN012115.D
Acq: 08 Oct 2020 22:46

Instrument :
BNA_N
ClientSampleId :
C5CF8

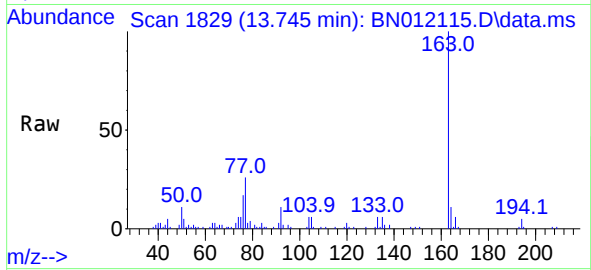

Tgt Ion:163 Resp: 62816
Ion Ratio Lower Upper
163 100
194 5.5 3.4 5.0#
164 11.5 7.8 11.8

