

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100820\
 Data File : BN012104.D
 Acq On : 08 Oct 2020 16:07
 Operator : CG/JU
 Sample : PB132115BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M

Title : SVOA CALIBRATION

Signal : TIC: BN012104.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	43	rVB	80517	120929	1.72%	0.174%
2	3.905	152	156	160	rVB	24306	33628	0.48%	0.048%
3	4.117	190	192	197	rVB5	7548	9046	0.13%	0.013%
4	4.517	254	260	265	rBV9	7728	14105	0.20%	0.020%
5	4.893	320	324	328	rBV7	6856	10383	0.15%	0.015%
6	6.822	645	652	661	rBV	1291027	1962884	27.98%	2.824%
7	6.987	673	680	692	rVB	961862	1470657	20.96%	2.116%
8	7.181	706	713	723	rBV	1336406	2069224	29.50%	2.977%
9	7.646	785	792	801	rBV	961116	1495827	21.32%	2.152%
10	8.346	904	911	920	rBV	1489543	2361778	33.67%	3.398%
11	8.793	978	987	997	rBV	1154980	1913687	27.28%	2.753%
12	9.510	1102	1109	1118	rBV	1018307	1647833	23.49%	2.370%
13	10.046	1192	1200	1214	rBV	1486091	2413784	34.41%	3.472%
14	10.422	1257	1264	1273	rBV	1256498	2039443	29.07%	2.934%
15	10.557	1280	1287	1301	rBV	1372384	2413112	34.40%	3.471%
16	12.022	1530	1536	1542	rBV6	19626	37143	0.53%	0.053%
17	13.698	1815	1821	1835	rVB	2682180	3615432	51.54%	5.201%
18	13.975	1861	1868	1878	rBV	2917705	4229902	60.30%	6.085%
19	14.287	1915	1921	1933	rBV	1939359	2741494	39.08%	3.944%
20	14.487	1949	1955	1970	rBV	1173224	1752782	24.99%	2.521%
21	15.281	2082	2090	2102	rBV	3619482	5098110	72.67%	7.334%
22	15.404	2105	2111	2126	rVV	1369735	1870956	26.67%	2.691%
23	15.522	2127	2131	2136	rVB2	44634	57637	0.82%	0.083%
24	15.951	2200	2204	2205	rBV4	6590	7821	0.11%	0.011%
25	16.069	2221	2224	2229	rBV5	14774	16381	0.23%	0.024%
26	16.798	2343	2348	2349	rBV3	5242	7594	0.11%	0.011%
27	16.822	2349	2352	2358	rVB7	10254	19255	0.27%	0.028%
28	17.034	2381	2388	2398	rBV	2324979	3197405	45.58%	4.600%
29	17.134	2398	2405	2419	rVV	3961915	5576520	79.49%	8.022%
30	17.534	2469	2473	2477	rVB7	5781	12102	0.17%	0.017%
31	17.598	2483	2484	2488	rBV4	6391	7210	0.10%	0.010%
32	17.663	2490	2495	2497	rBV6	7981	12530	0.18%	0.018%
33	17.933	2537	2541	2545	rBV7	12303	20496	0.29%	0.029%
34	18.010	2552	2554	2557	rVB2	12330	11385	0.16%	0.016%
35	18.463	2629	2631	2635	rVB6	8138	10176	0.15%	0.015%
36	19.069	2730	2734	2740	rBV2	42218	57645	0.82%	0.083%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100820\
 Data File : BN012104.D
 Acq On : 08 Oct 2020 16:07
 Operator : CG/JU
 Sample : PB132115BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK15

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Title : SVOA CALIBRATION

37	19.228	2759	2761	2764	rBV3	10574	11894	0.17%	0.017%
38	19.322	2774	2777	2780	rBV	34812	39927	0.57%	0.057%
39	19.433	2790	2796	2803	rBV2	5028712	6490688	92.52%	9.337%
40	21.022	3062	3066	3070	rBV	199791	270861	3.86%	0.390%
41	21.233	3097	3102	3108	rBV	2909997	3591375	51.20%	5.166%
42	23.298	3446	3453	3467	rVB	3764403	7015075	100.00%	10.091%
43	23.433	3470	3476	3486	rVB	2056609	3758637	53.58%	5.407%


Sum of corrected areas: 69514753

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100820\
Data File : BN012104.D
Acq On : 08 Oct 2020 16:07
Operator : CG/JU
Sample : PB132115BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK15

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

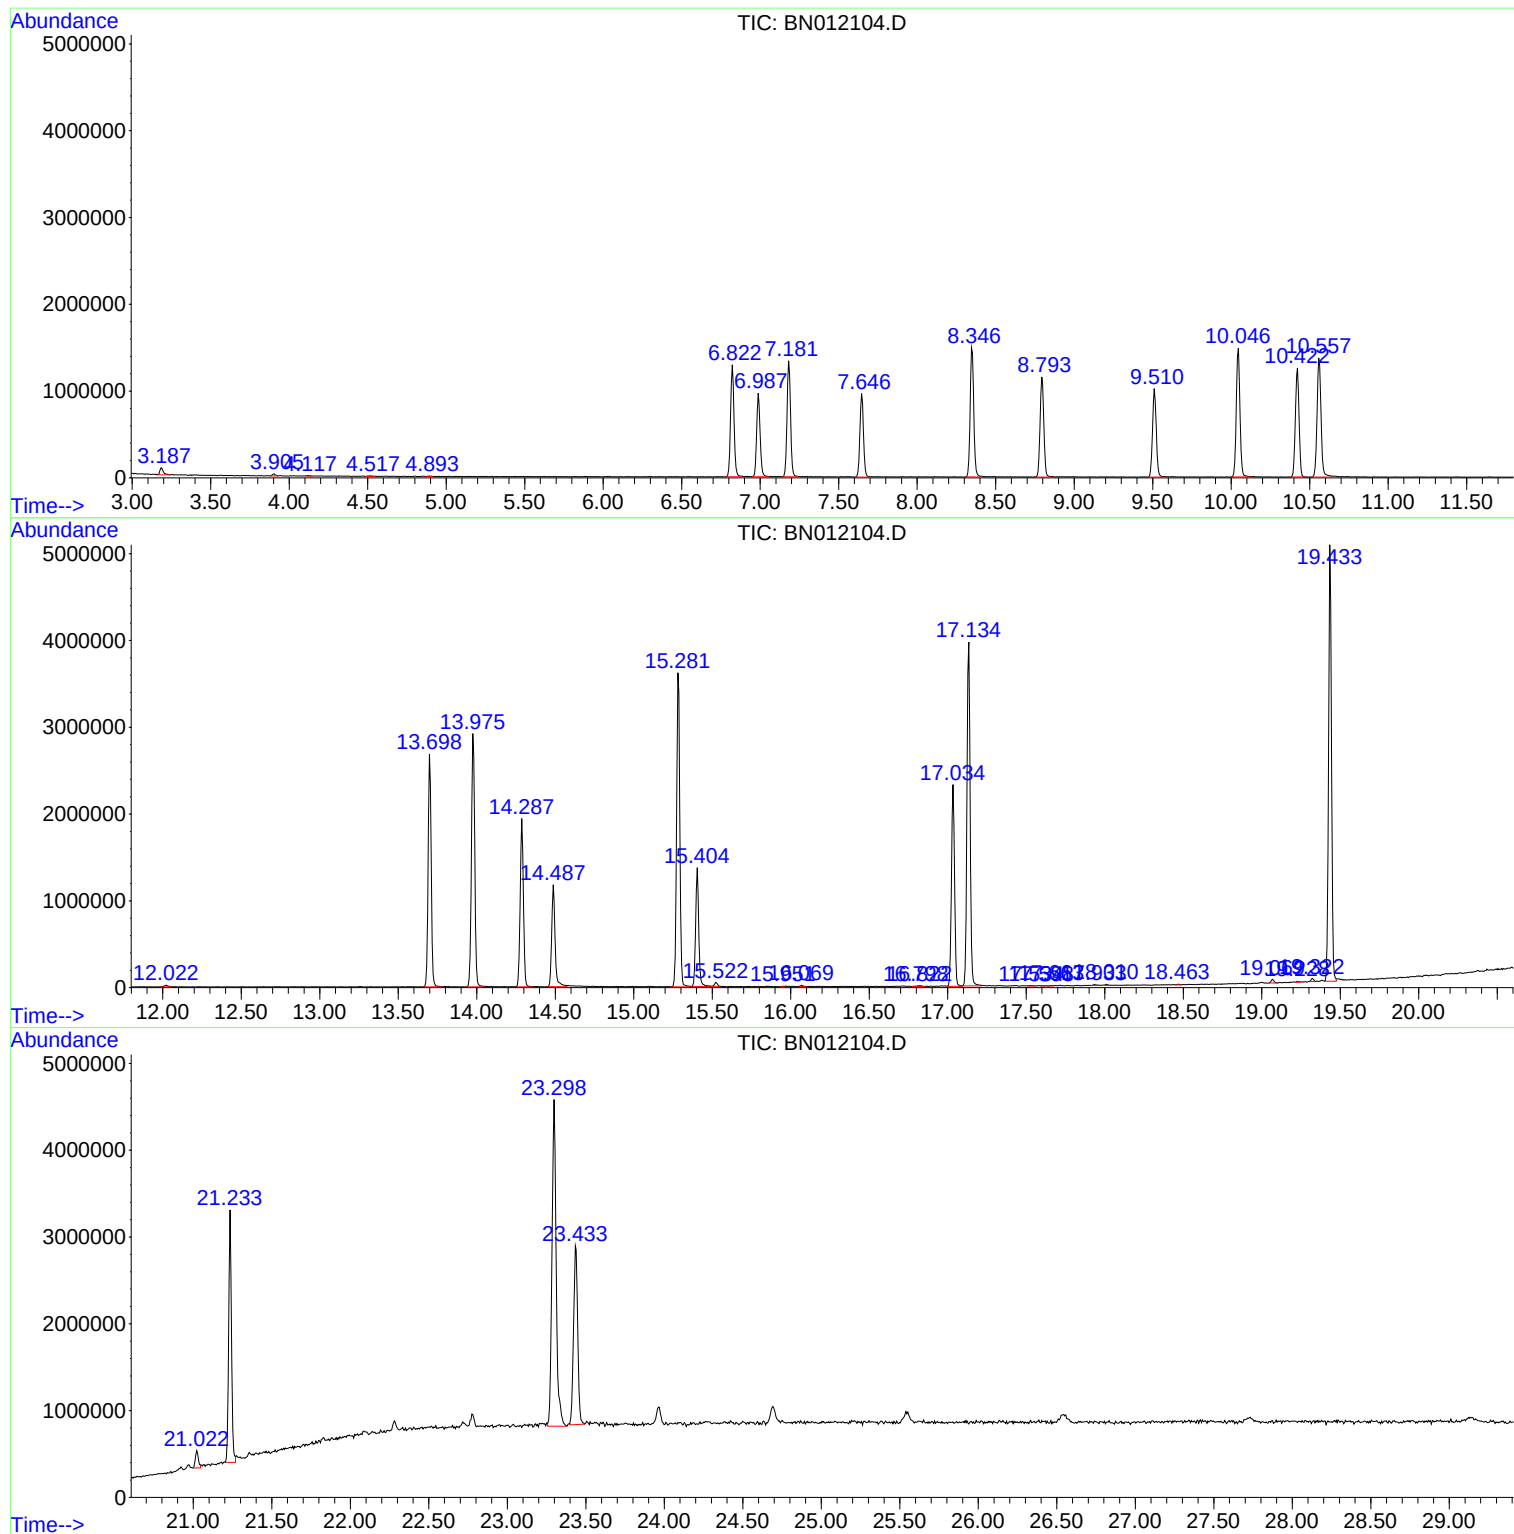

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100820\
Data File : BN012104.D
Acq On : 08 Oct 2020 16:07
Operator : CG/JU
Sample : PB132115BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK15

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100820\
Data File : BN012104.D
Acq On : 08 Oct 2020 16:07
Operator : CG/JU
Sample : PB132115BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK15

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
