
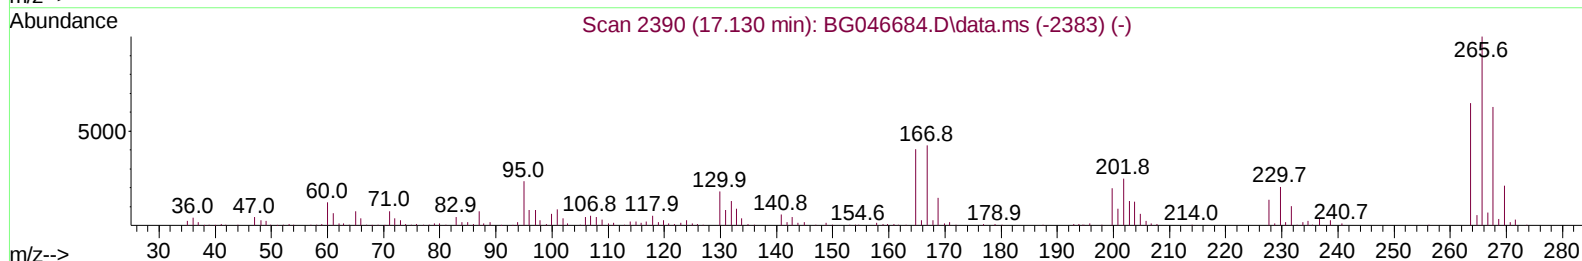
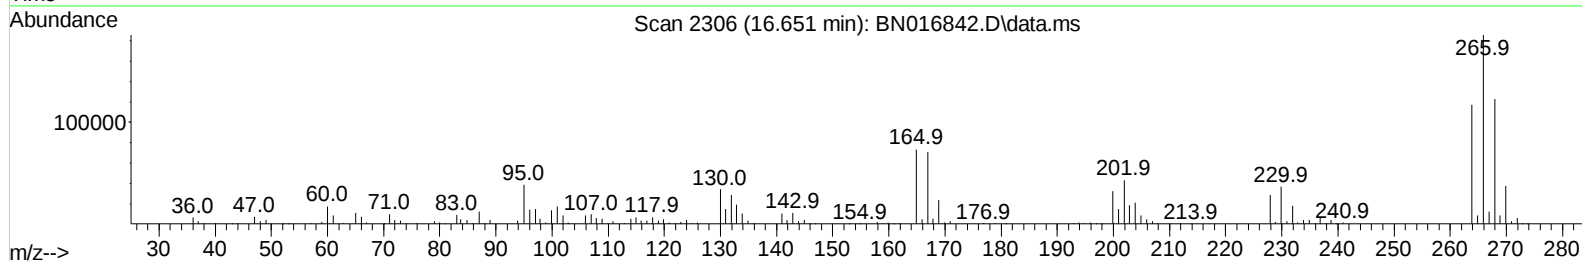


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN100821\  
Data File : BN016842.D  
Acq On : 08 Oct 2021 13:41  
Operator : CG/JU  
Sample : DFTTP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 15:41:22 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Sep 30 18:14:09 2021  
Response via : Initial Calibration

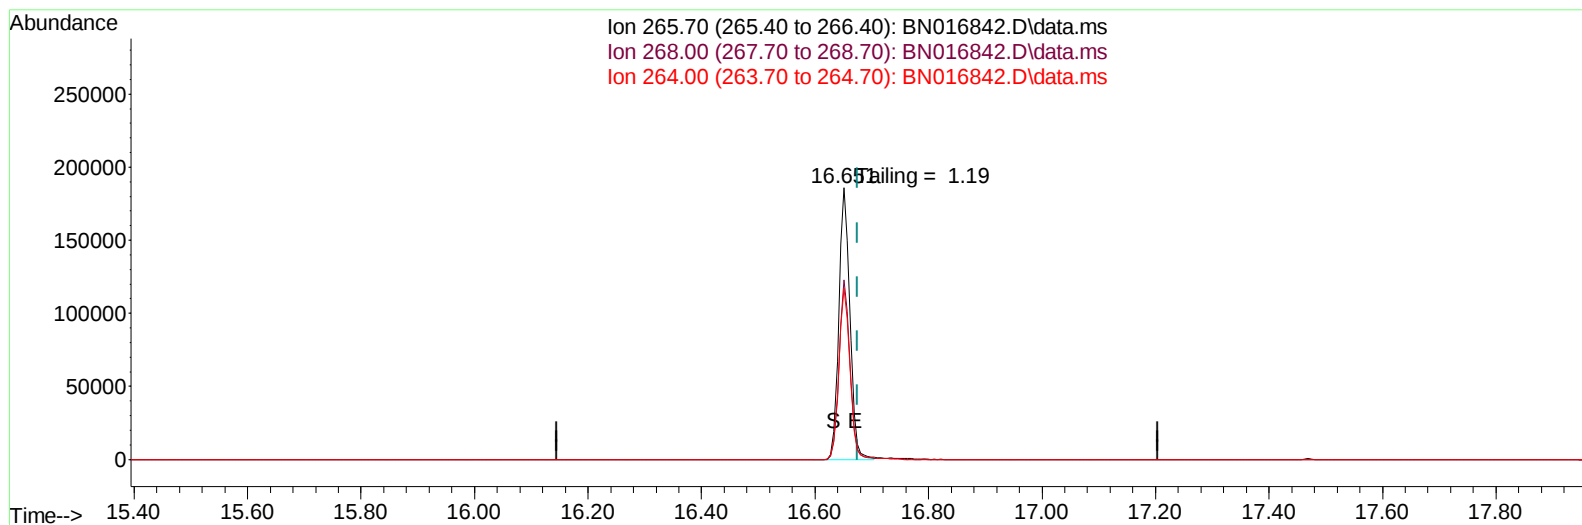

TIC: BN016842.D\data.ms




**(70) Pentachlorophenol (C)**

**16.651min (-0.023) 34018.21 ng**

**response 254152**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 66.09  |
| 264.00 | 61.60  | 63.20  |
| 0.00   | 0.00   | 0.00   |

Quant Time: Oct 08 15:41:22 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Sep 30 18:14:09 2021  
Response via : Initial Calibration

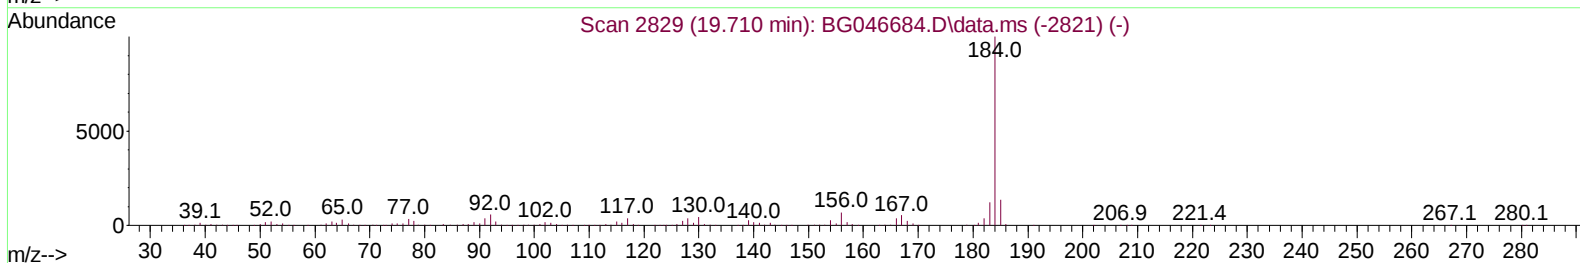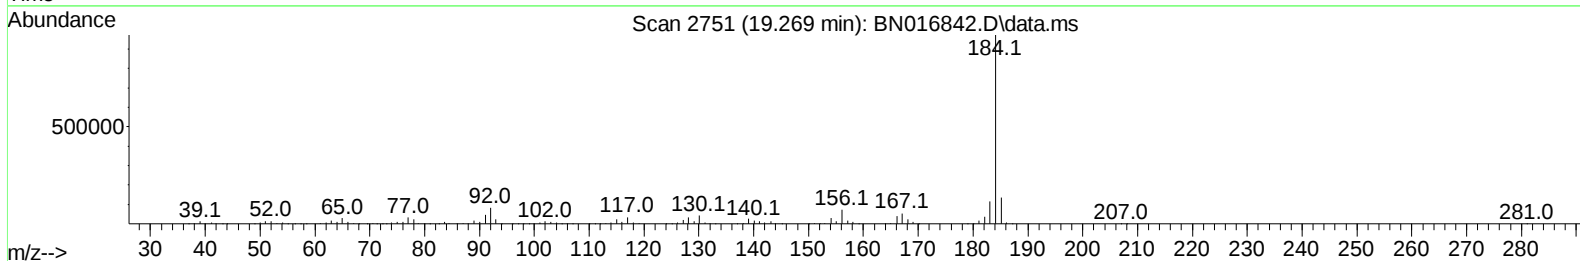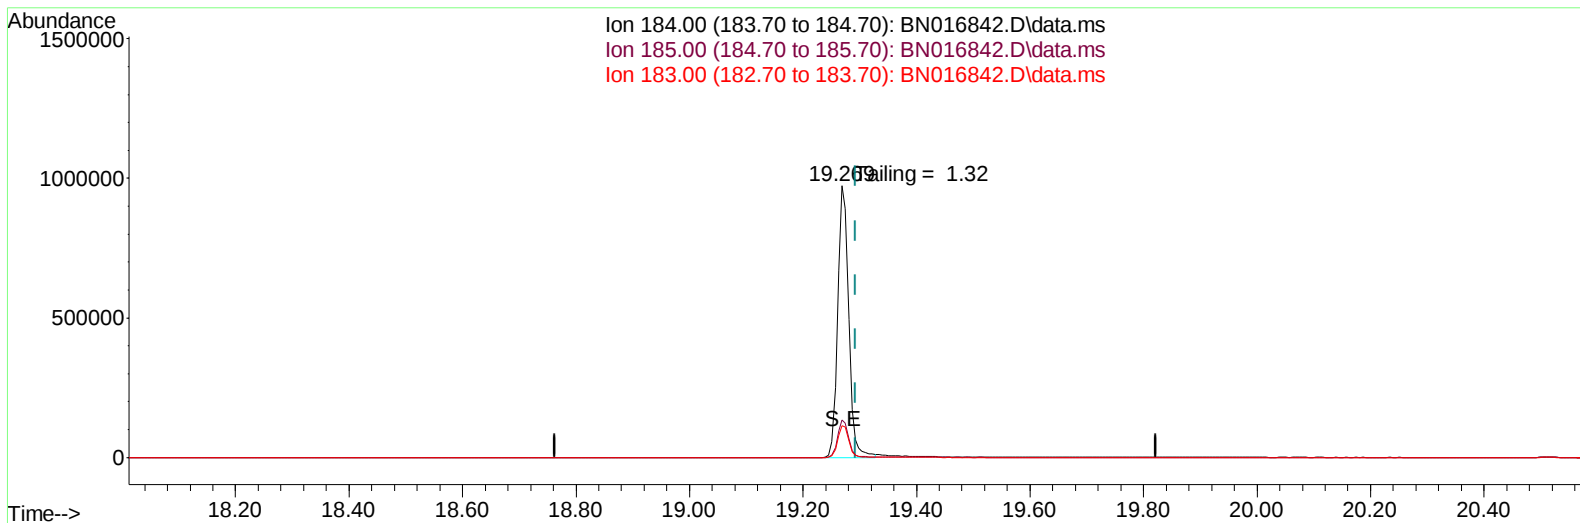

TIC: BN016842.D\data.ms

(77) Benzidine

**19.269min (-0.023) 0.00 ng**

**response**      **1339233**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.83  |
| 183.00 | 13.20  | 11.77  |
| 0.00   | 0.00   | 0.00   |