
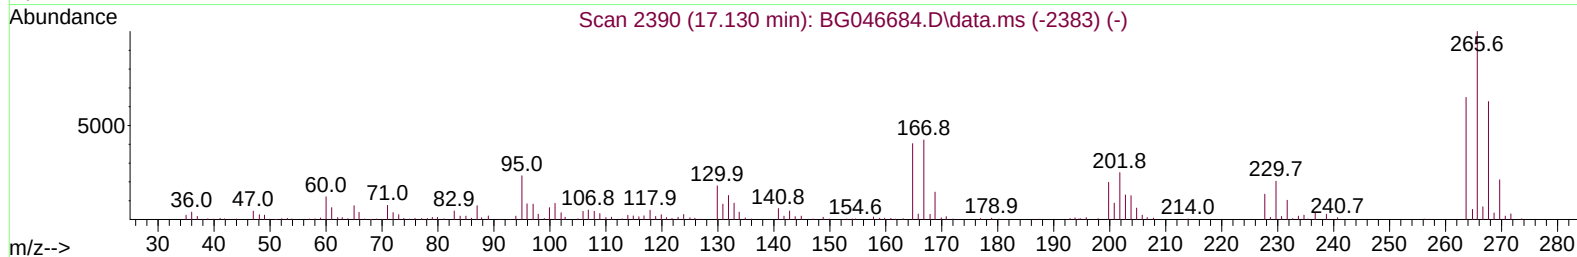
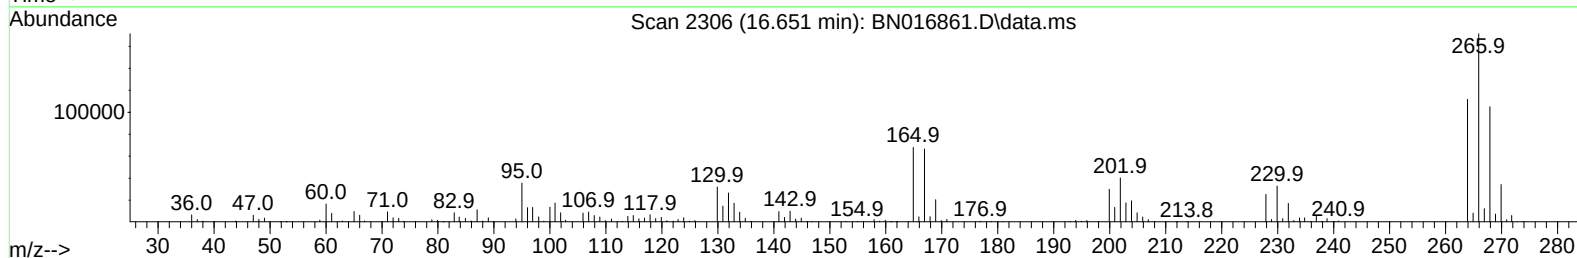


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100821\
Data File : BN016861.D
Acq On : 09 Oct 2021 02:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 07:22:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

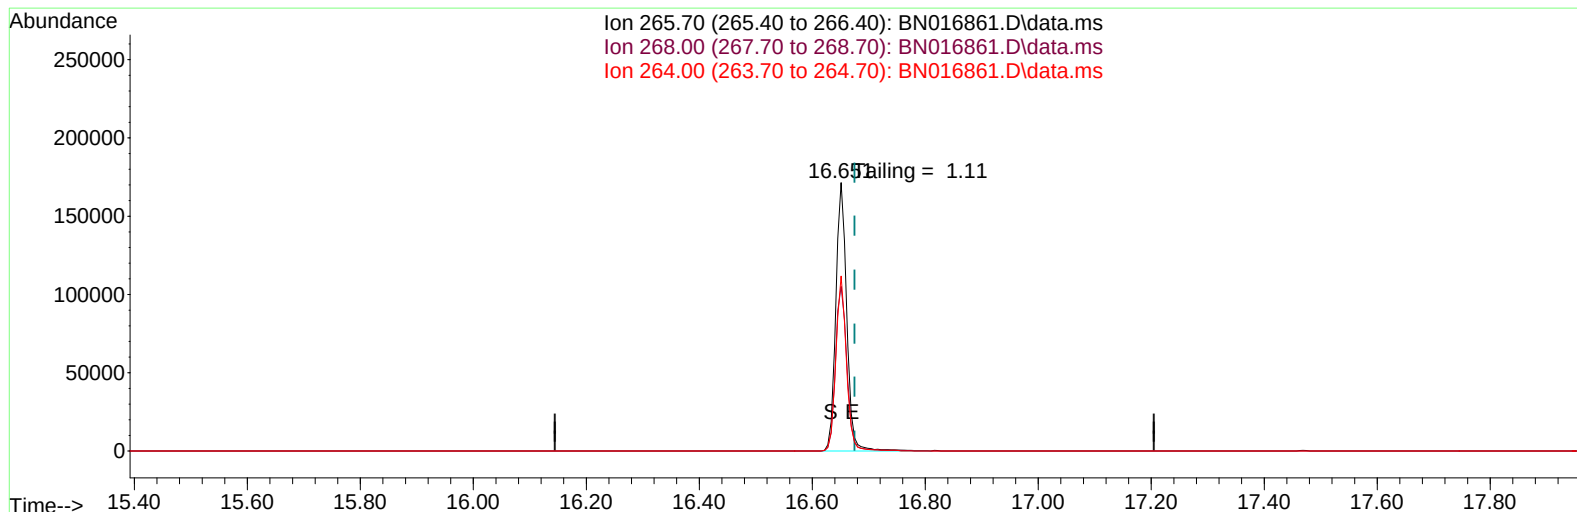

TIC: BN016861.D\data.ms

(70) Pentachlorophenol (C)




16.651min (-0.024) 29881.57 ng

response 230282

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.29
264.00	61.60	65.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100821\
Data File : BN016861.D
Acq On : 09 Oct 2021 02:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 07:22:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

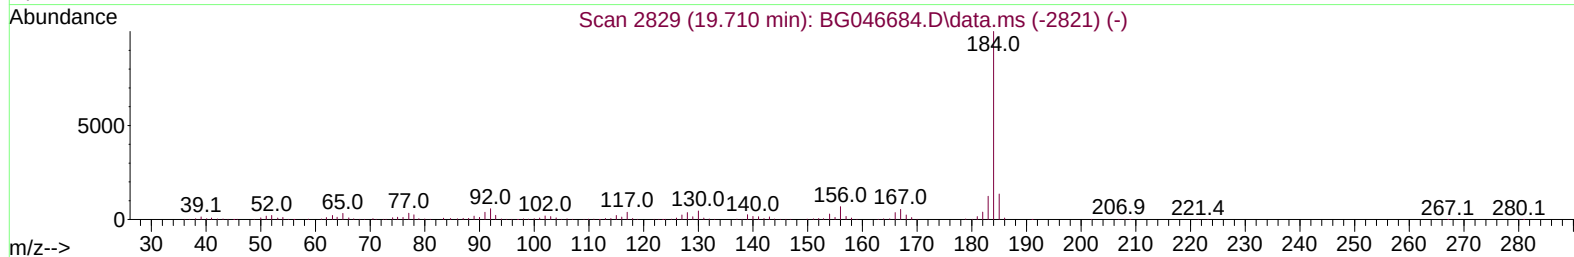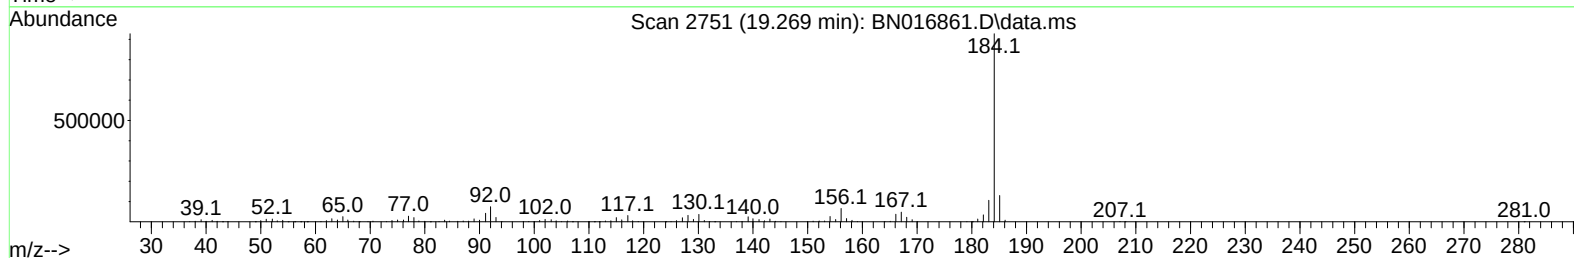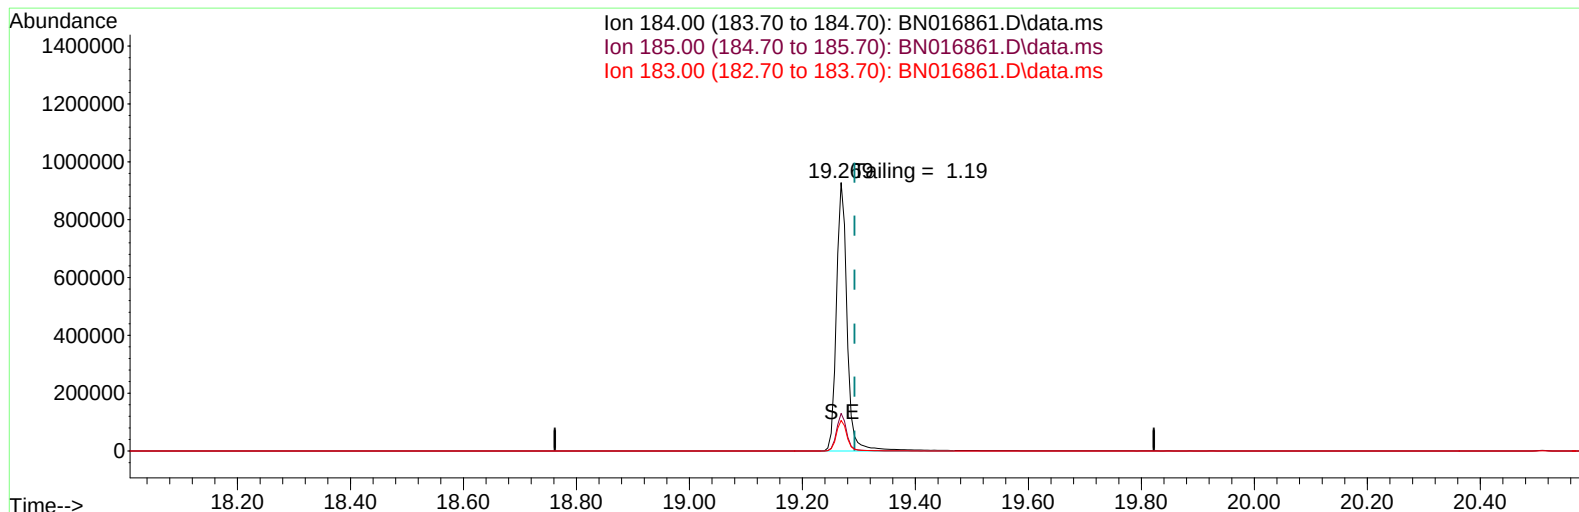

TIC: BN016861.D\data.ms

(77) Benzidine

19.269min (-0.024) 0.00 ng

response 1225669

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.00
183.00	13.20	11.43
0.00	0.00	0.00