
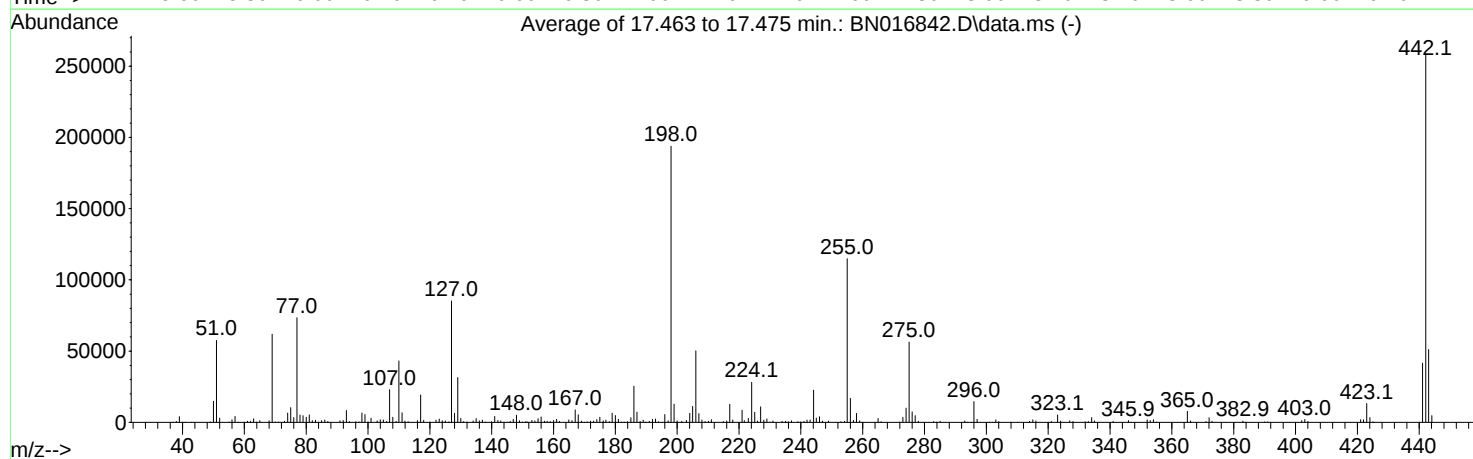


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100821\
 Data File : BN016842.D
 Acq On : 08 Oct 2021 13:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 08 15:46:07 2021

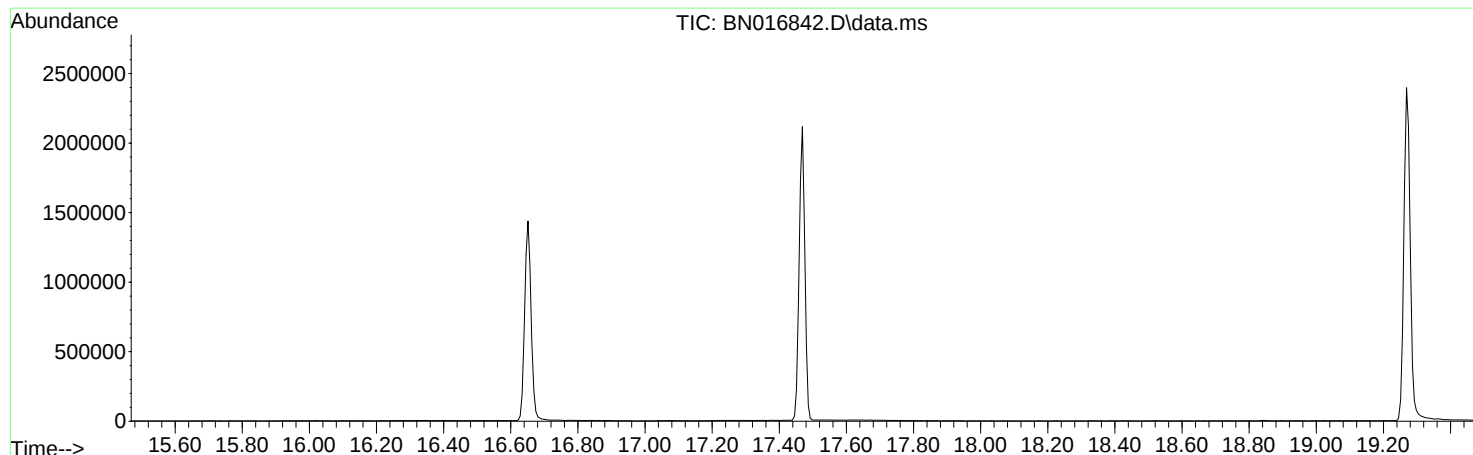

AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	57560	PASS
68	69	0.00	2	1.9	1144	PASS
69	198	0.00	100	31.9	61829	PASS
70	69	0.00	2	0.6	346	PASS
127	198	10	80	44.0	85272	PASS
197	198	0.00	2	0.6	1150	PASS
198	198	100	100	100.0	193877	PASS
199	198	5	9	6.6	12811	PASS
275	198	10	60	29.1	56360	PASS
365	198	1	100	4.0	7741	PASS
441	198	0.01	100	21.4	41515	PASS
442	442	50	100	100.0	258176	PASS
443	442	15	24	19.8	51128	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/8/2021	BNA_N	<u>BN016842.D</u>
Compound Name	Response	Retention Time
DDT	658146	20.516
DDD	10125	20.075
DDE	0	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10125	668271	1.52

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100821\
Data File : BN016842.D
Acq On : 08 Oct 2021 13:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 08 15:41:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

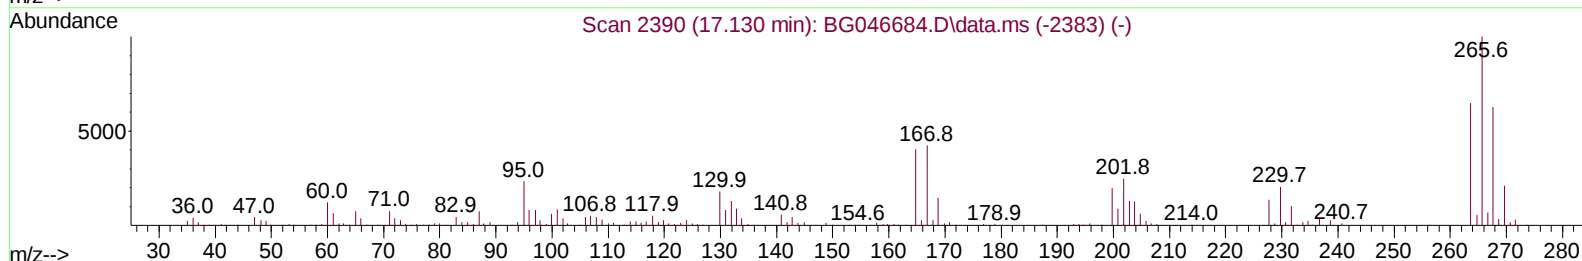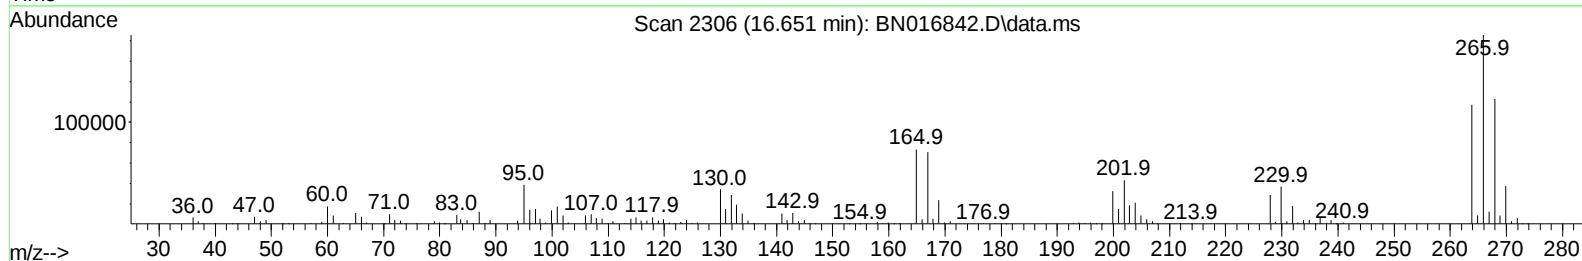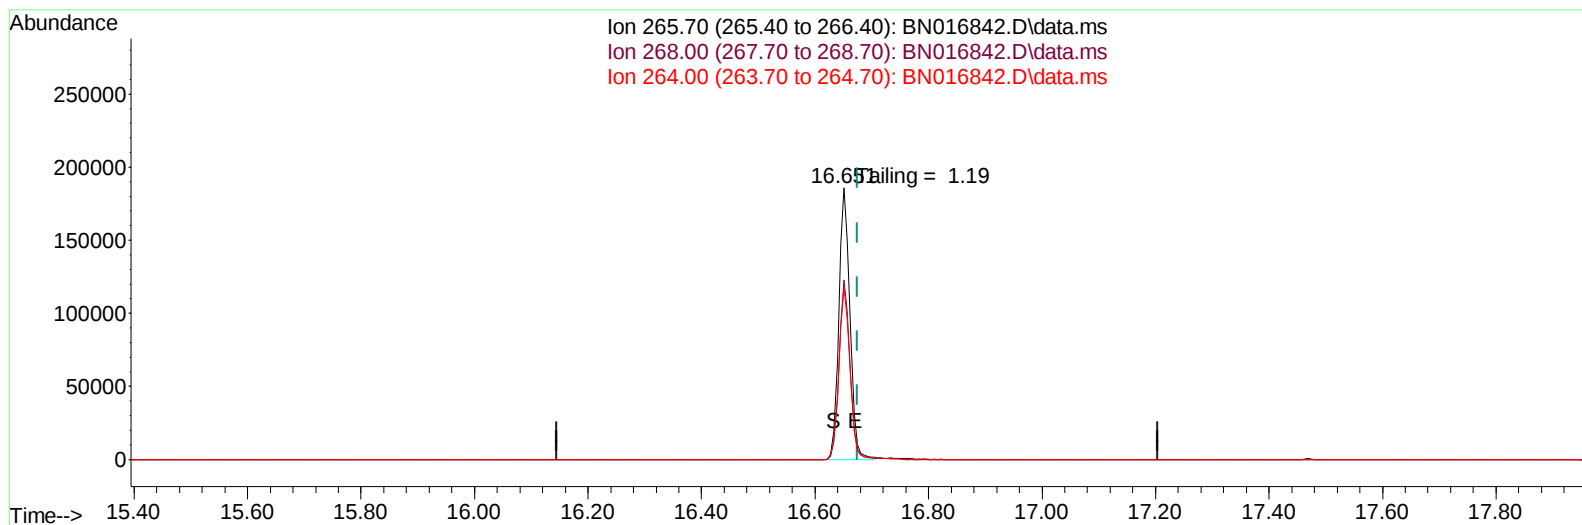

TIC: BN016842.D\data.ms

(70) Pentachlorophenol (C)

16.651min (-0.023) 34018.21 ng




response 254152

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.09
264.00	61.60	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100821\
Data File : BN016842.D
Acq On : 08 Oct 2021 13:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 08 15:41:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

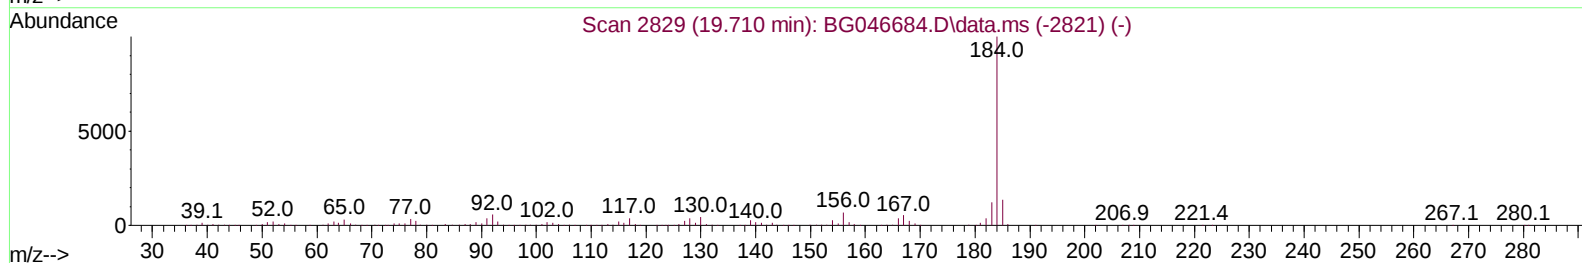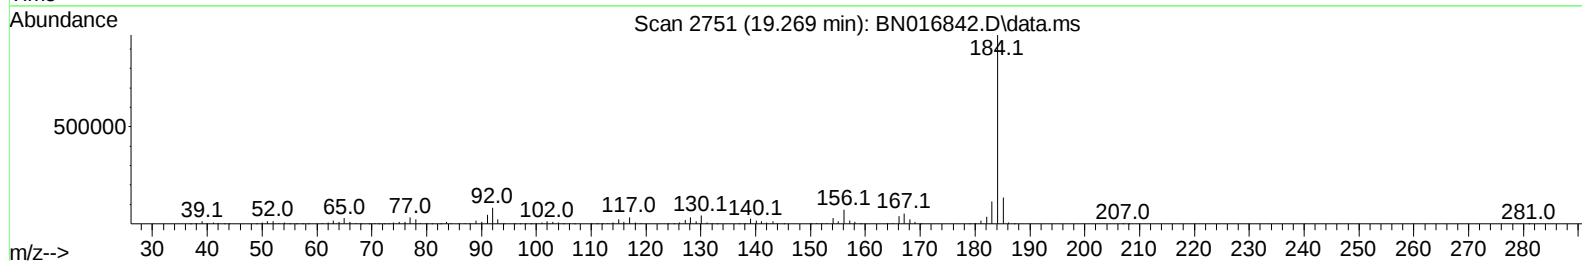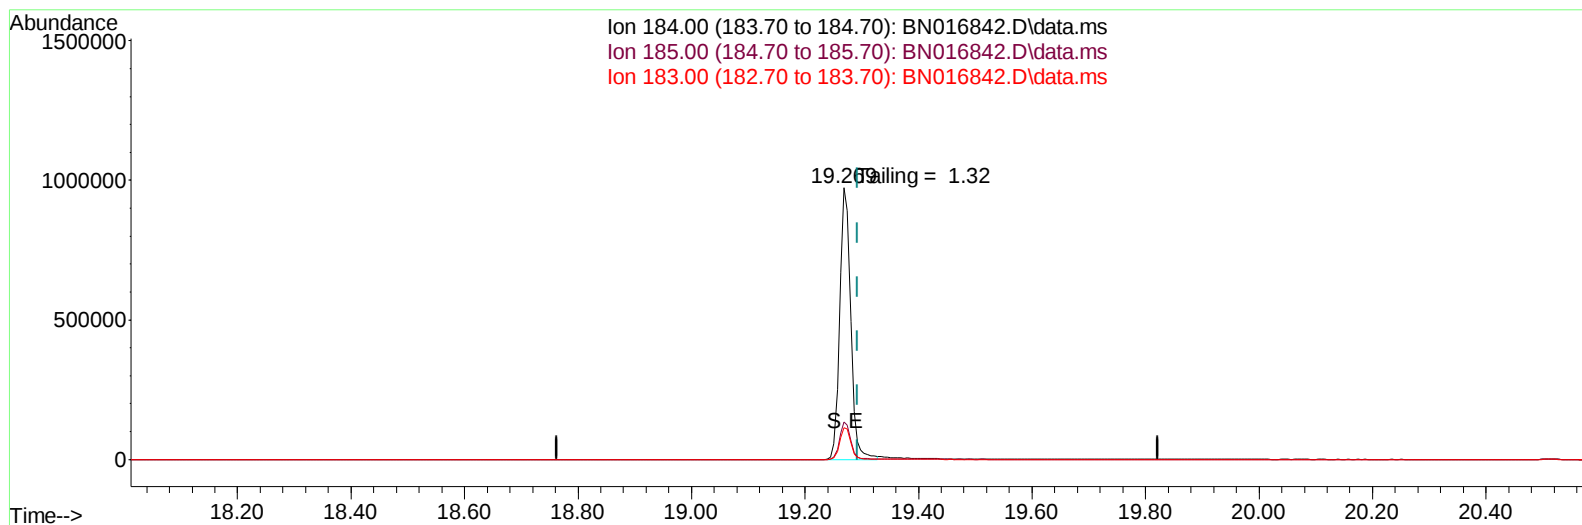

TIC: BN016842.D\data.ms

(77) Benzidine

19.269min (-0.023) 0.00 ng

response 1339233

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.83
183.00	13.20	11.77
0.00	0.00	0.00