
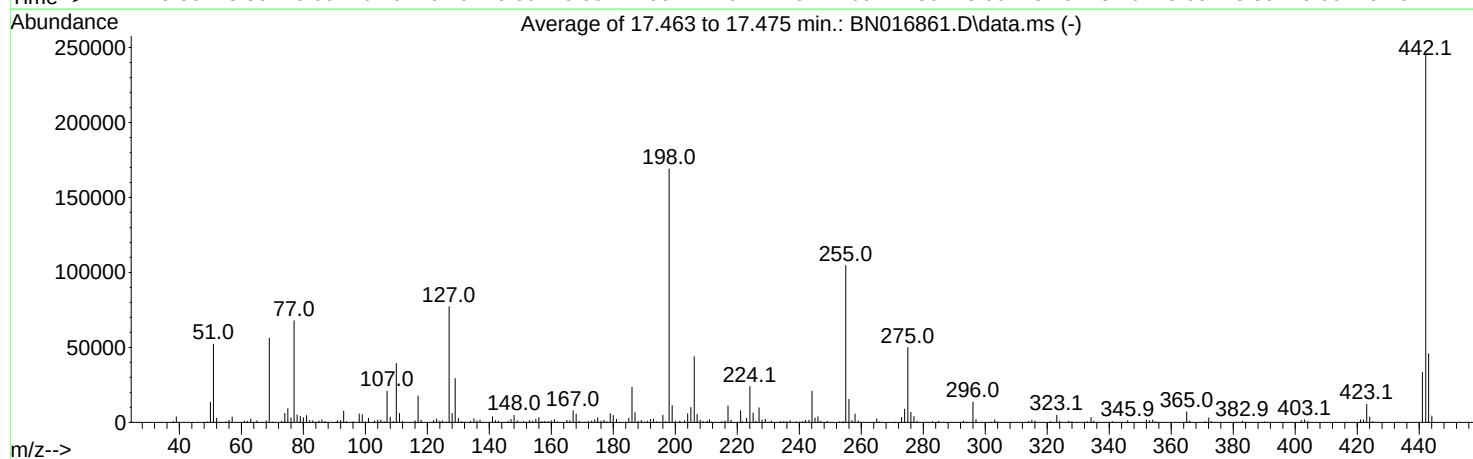


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100821\
 Data File : BN016861.D
 Acq On : 09 Oct 2021 02:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 08 15:46:07 2021

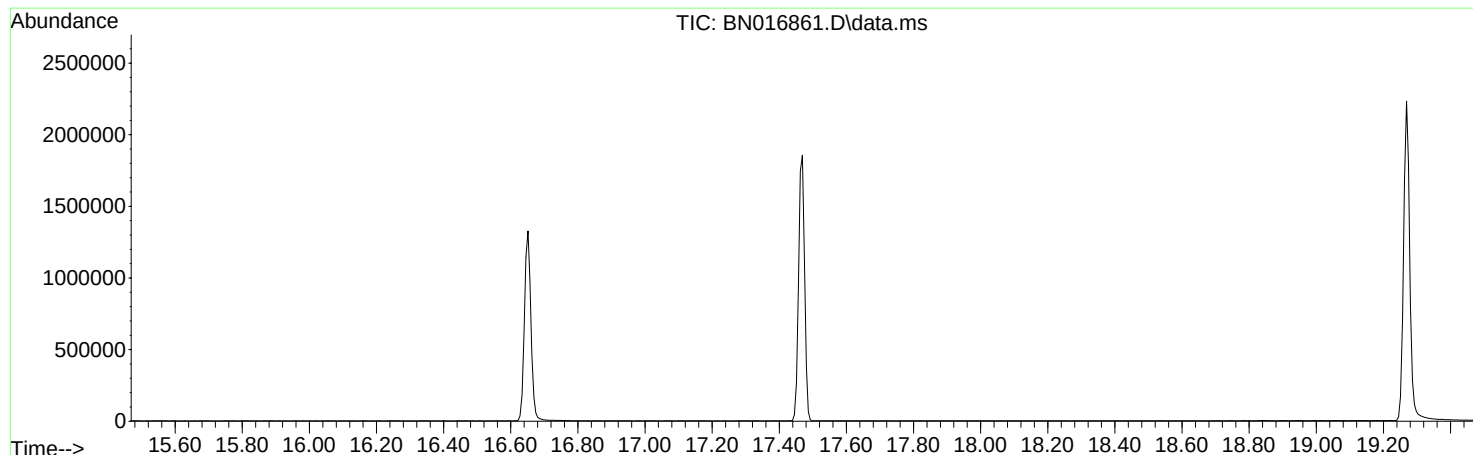

AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	52176	PASS
68	69	0.00	2	1.8	1030	PASS
69	198	0.00	100	33.2	56091	PASS
70	69	0.00	2	0.4	249	PASS
127	198	10	80	45.7	77195	PASS
197	198	0.00	2	0.4	679	PASS
198	198	100	100	100.0	169021	PASS
199	198	5	9	6.7	11244	PASS
275	198	10	60	29.6	49968	PASS
365	198	1	100	4.1	6977	PASS
441	198	0.01	100	19.7	33331	PASS
442	442	50	100	100.0	245355	PASS
443	442	15	24	18.7	45795	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/8/2021	BNA_N	<u>BN016861.D</u>
Compound Name	Response	Retention Time
DDT	607713	20.51
DDD	25292	20.069
DDE	439	19.563
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25731	633444	4.06

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100821\
Data File : BN016861.D
Acq On : 09 Oct 2021 02:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 09 07:22:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

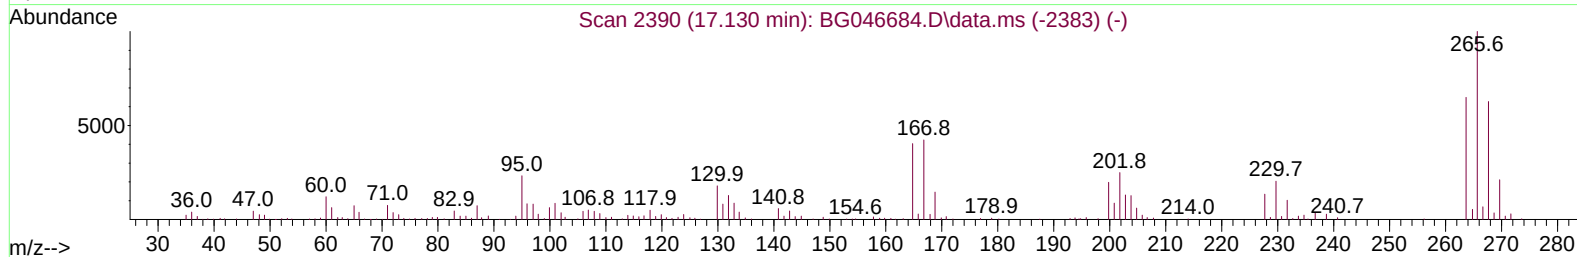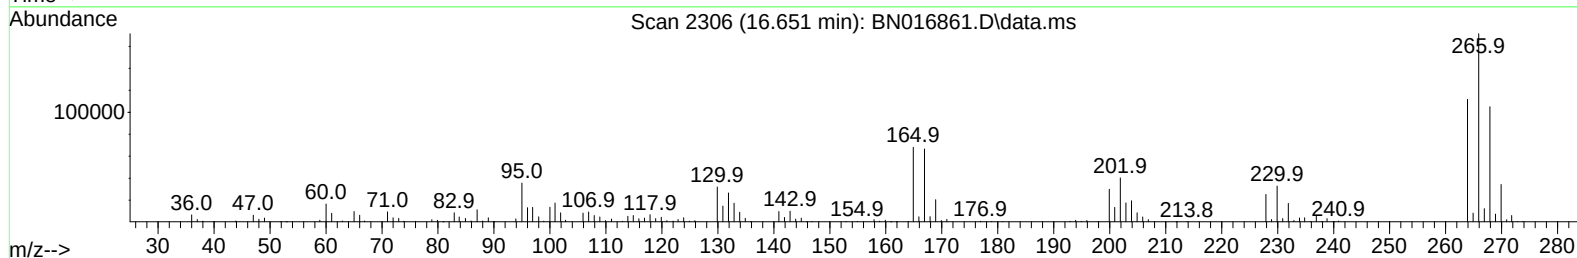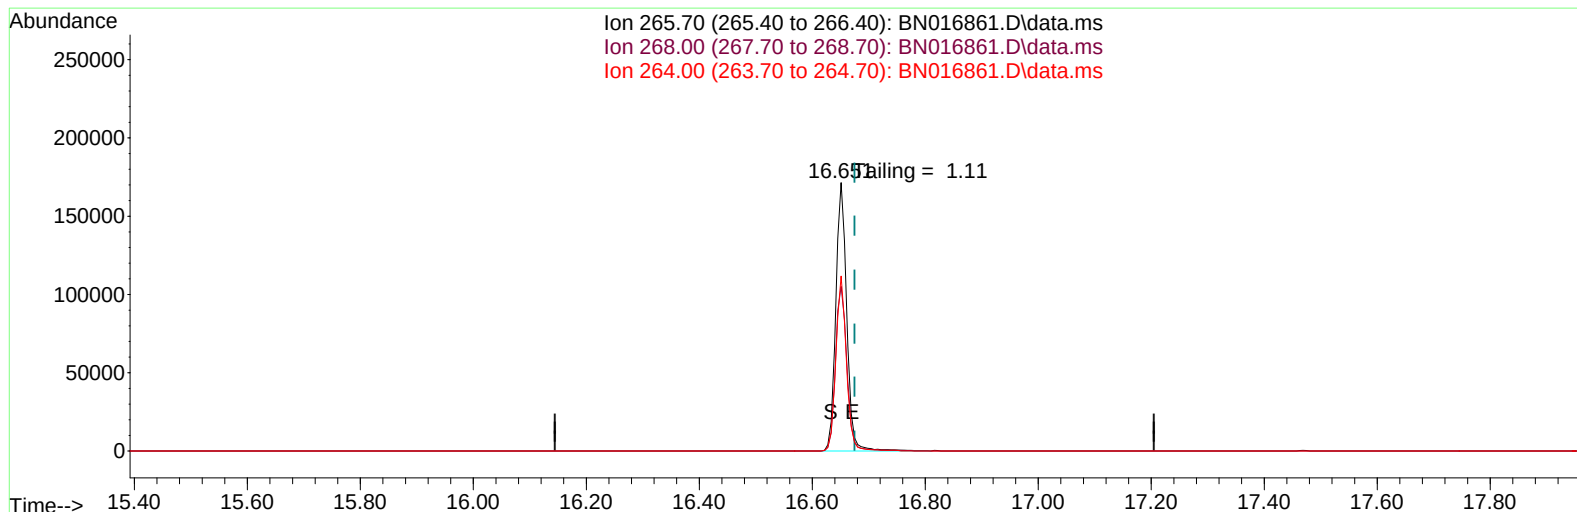

TIC: BN016861.D\data.ms

(70) Pentachlorophenol (C)

16.651min (-0.024) 29881.57 ng




response 230282

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.29
264.00	61.60	65.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100821\
Data File : BN016861.D
Acq On : 09 Oct 2021 02:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 09 07:22:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

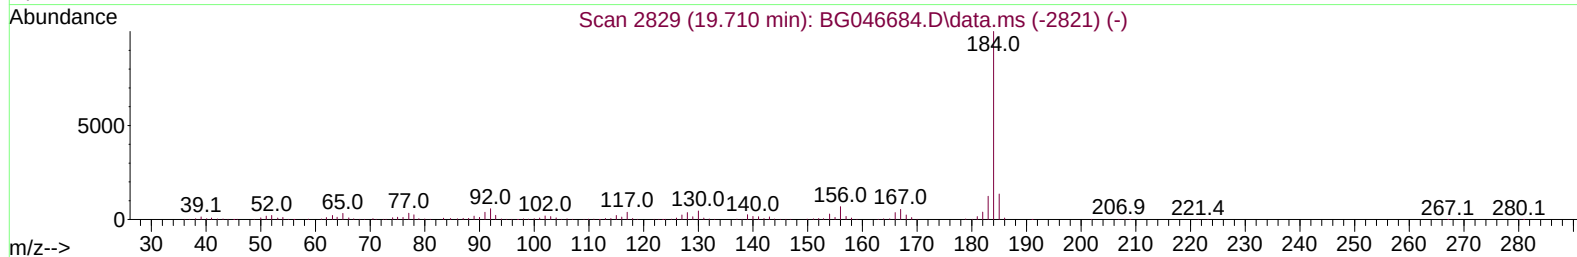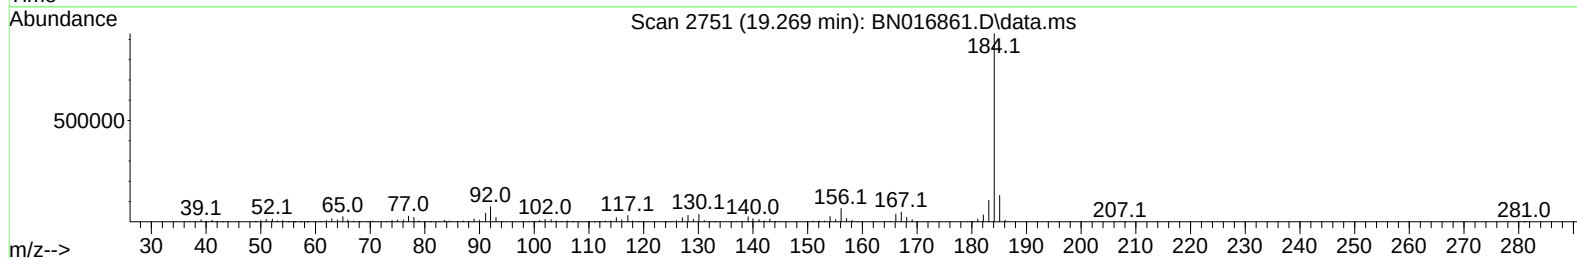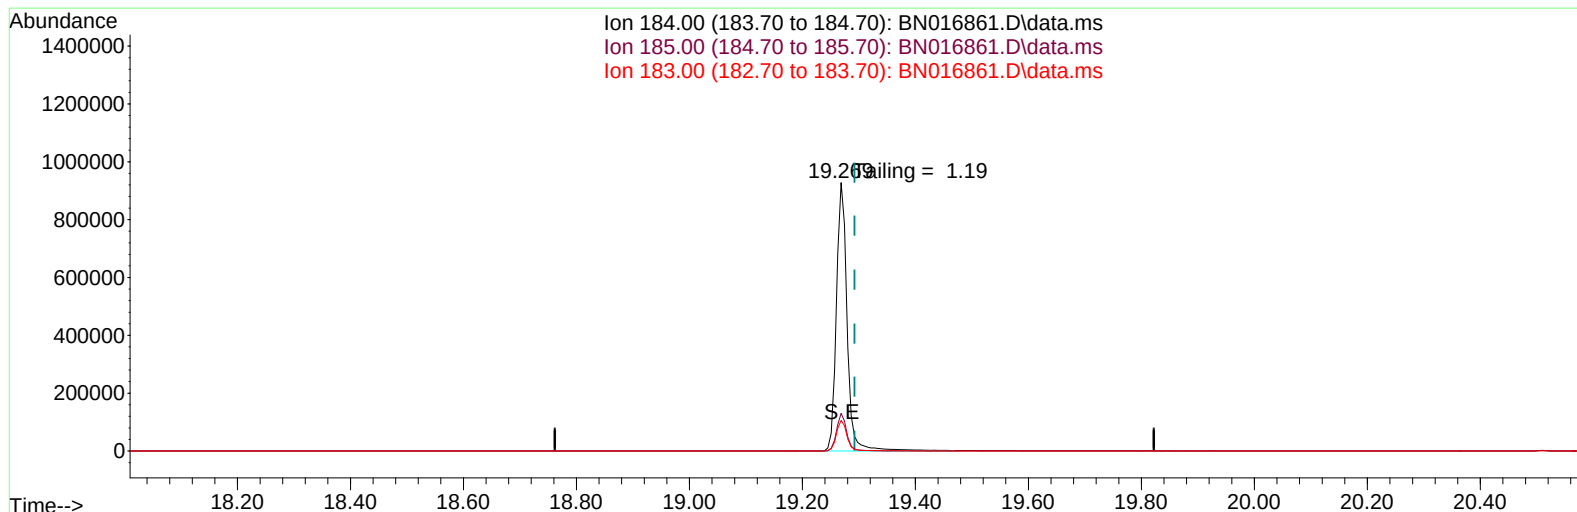

TIC: BN016861.D\data.ms

(77) Benzidine

19.269min (-0.024) 0.00 ng

response 1225669

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.00
183.00	13.20	11.43
0.00	0.00	0.00