
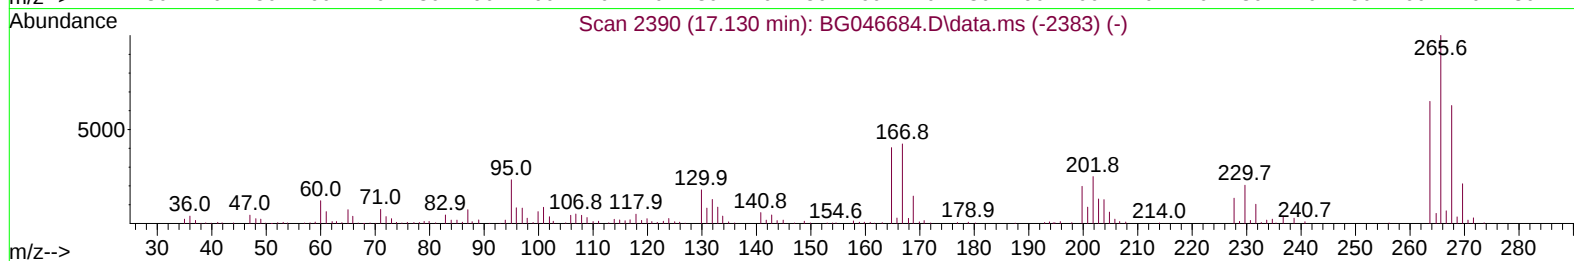
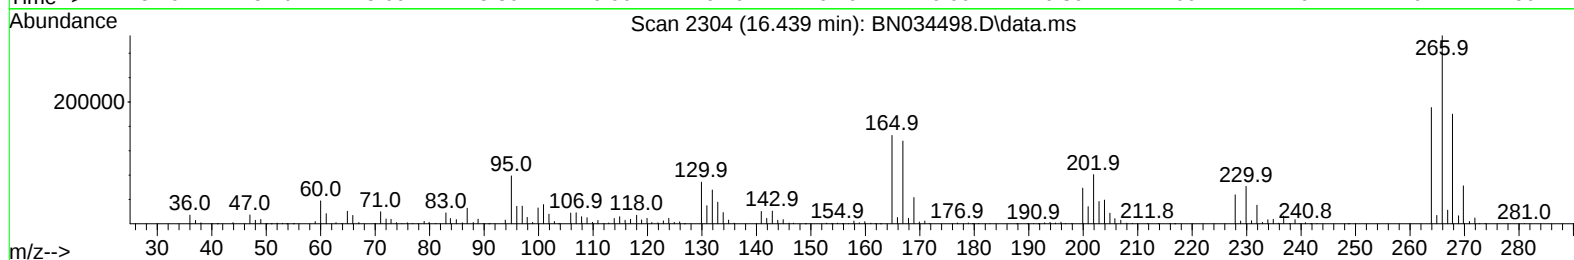


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100924\
Data File : BN034498.D
Acq On : 09 Oct 2024 10:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 73 Sample Multiplier: 1

Quant Time: Oct 10 05:23:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 10 05:23:17 2024
Response via : Initial Calibration

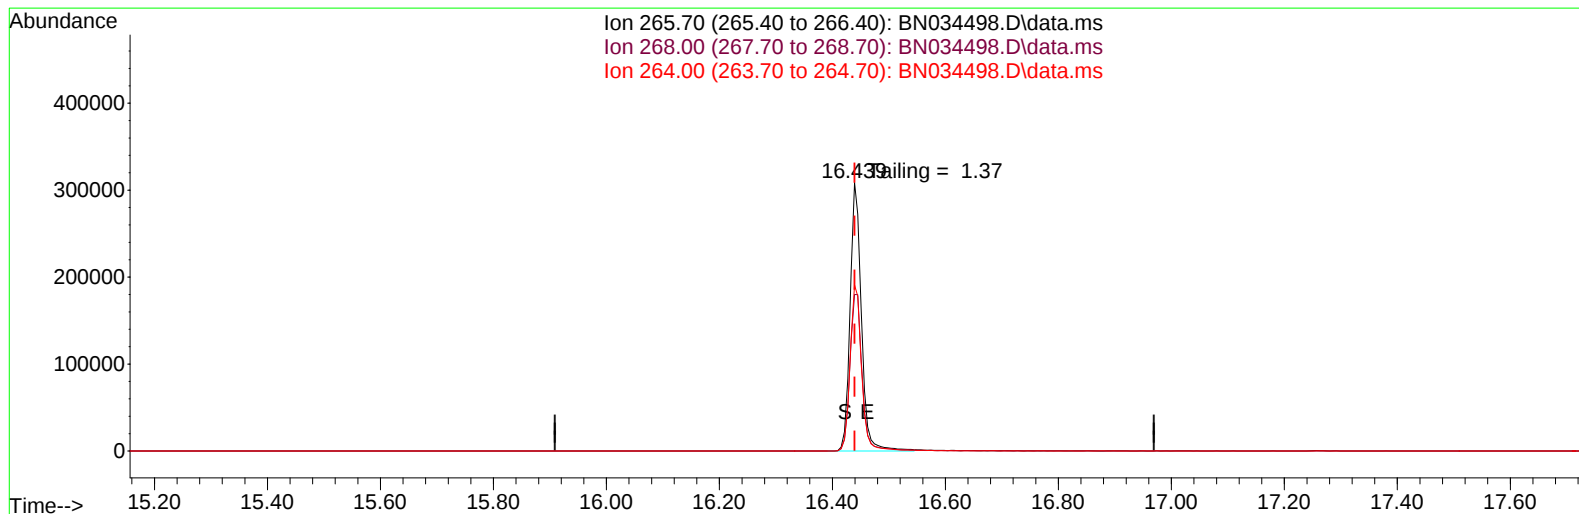

TIC: BN034498.D\data.ms

(70) Pentachlorophenol (C)




16.439min (0.000) 39510.53 ng

response 433166

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.32
264.00	61.60	61.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100924\
Data File : BN034498.D
Acq On : 09 Oct 2024 10:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 73 Sample Multiplier: 1

Quant Time: Oct 10 05:23:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 10 05:23:17 2024
Response via : Initial Calibration

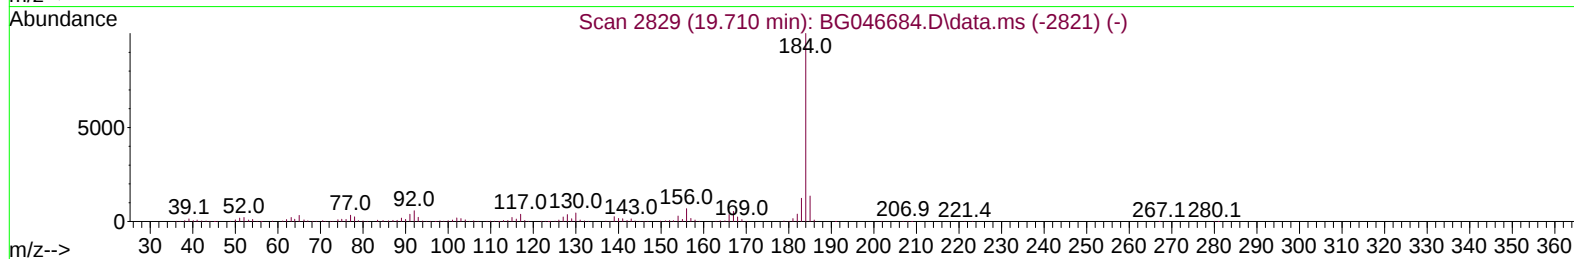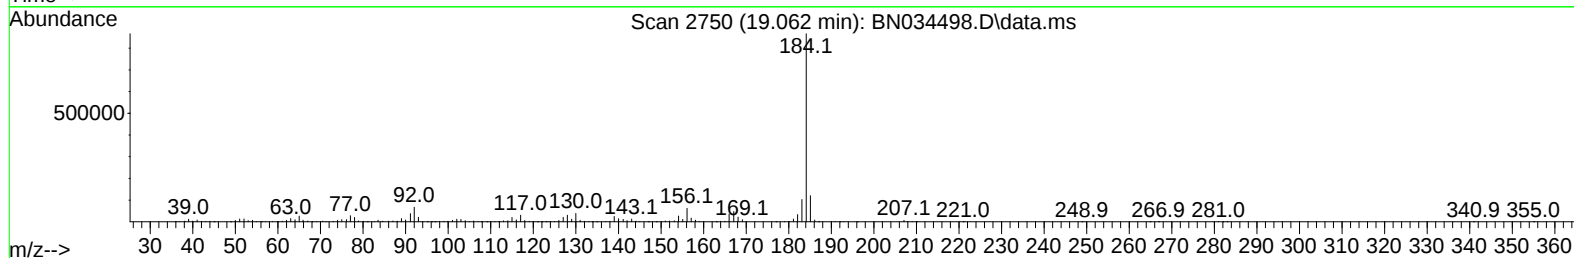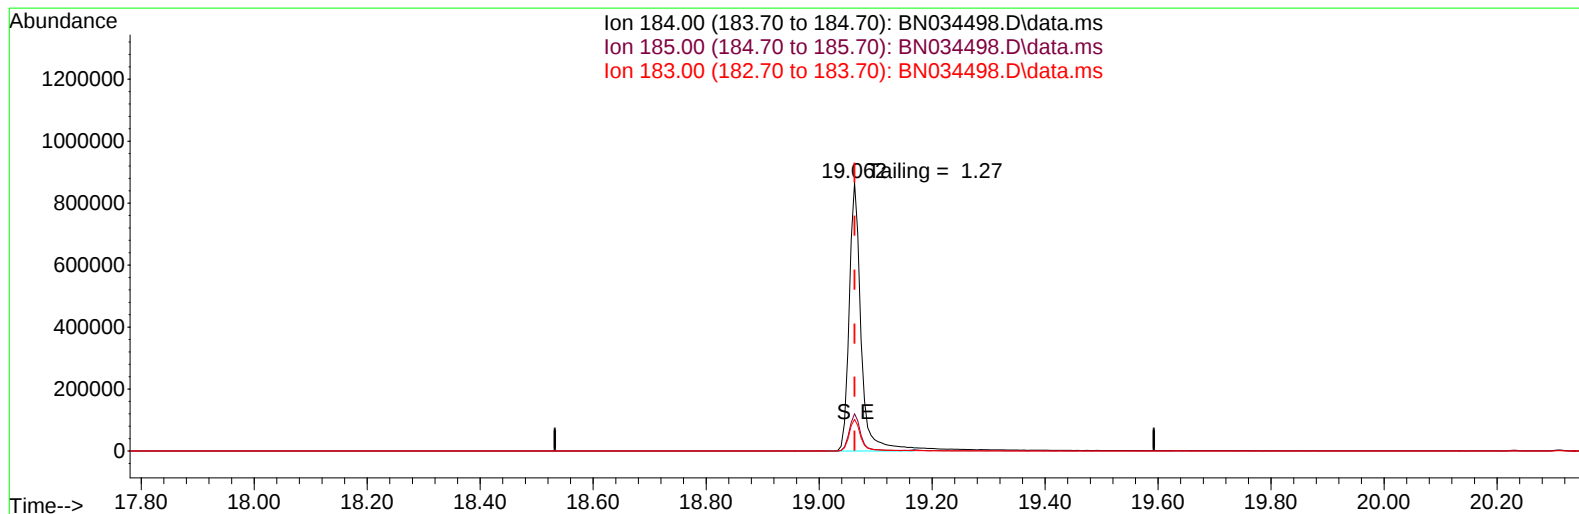

TIC: BN034498.D\data.ms

(77) Benzidine

19.062min (0.000) 0.00 ng

response 1287716

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	11.85
0.00	0.00	0.00