


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100924\
Data File : BN034498.D
Acq On : 09 Oct 2024 10:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 26 14:44:02 2024

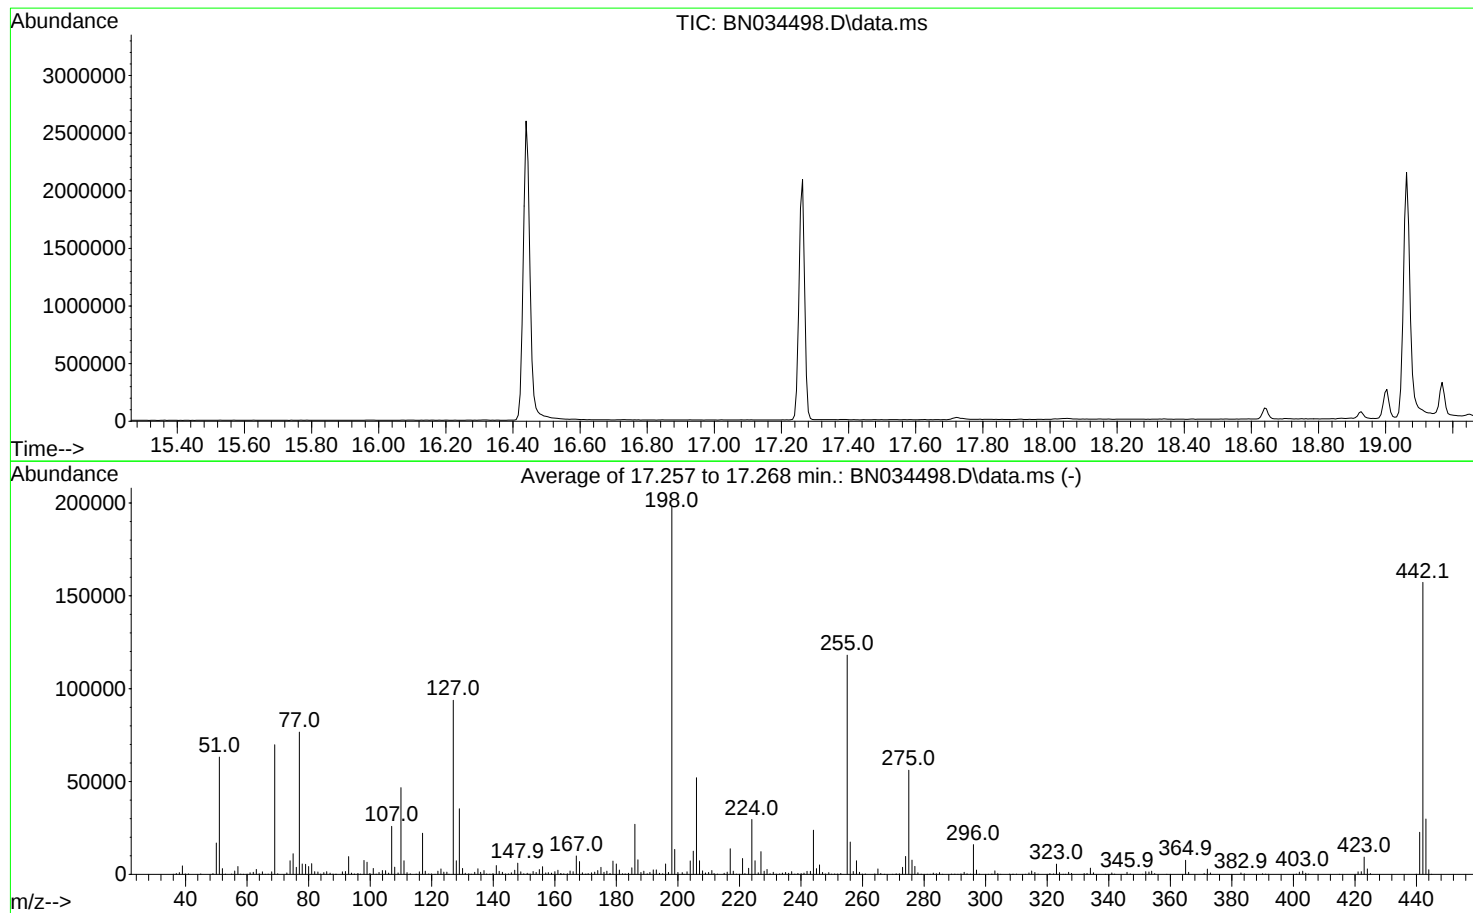

AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2436

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	63173	PASS
68	69	0.00	2	2.0	1391	PASS
69	198	0.00	100	35.2	69811	PASS
70	69	0.00	2	0.5	349	PASS
127	198	10	80	47.3	93787	PASS
197	198	0.00	2	0.5	1043	PASS
198	198	100	100	100.0	198123	PASS
199	198	5	9	6.8	13446	PASS
275	198	10	60	28.3	56107	PASS
365	198	1	100	3.8	7620	PASS
441	198	0.01	100	11.4	22664	PASS
442	442	50	100	100.0	157269	PASS
443	442	15	24	19.0	29813	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/9/2024	BNA_N	<u>BN034498.D</u>
Compound Name	Response	Retention Time
DDT	729416	20.309
DDD	64451	19.868
DDE	1287	19.357
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
65738	795154	8.27

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100924\
Data File : BN034498.D
Acq On : 09 Oct 2024 10:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 10 05:23:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 10 05:23:17 2024
Response via : Initial Calibration

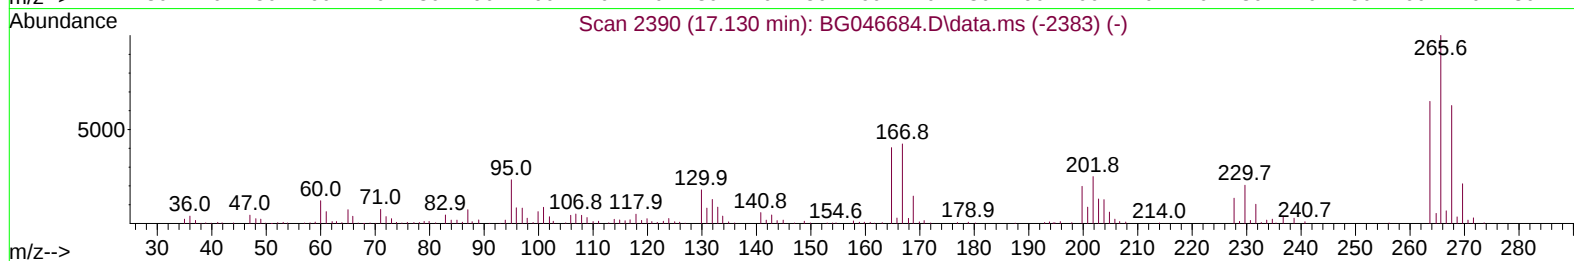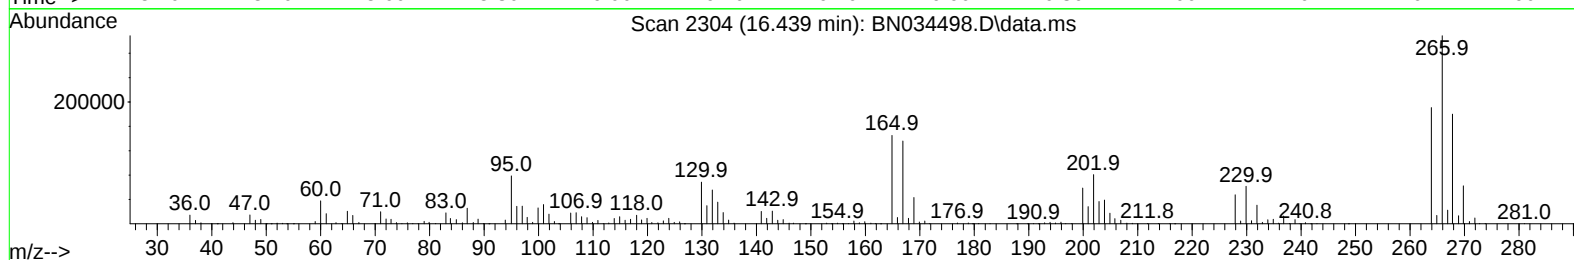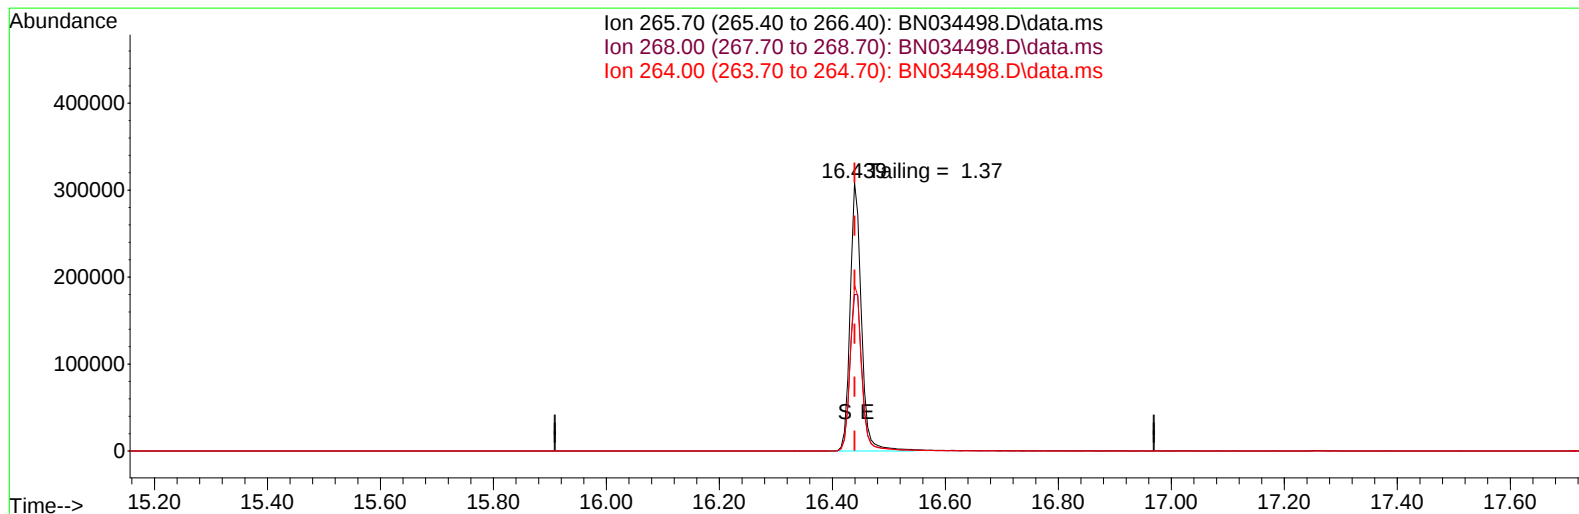

TIC: BN034498.D\data.ms

(70) Pentachlorophenol (C)

16.439min (0.000) 39510.53 ng




response 433166

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.32
264.00	61.60	61.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100924\
Data File : BN034498.D
Acq On : 09 Oct 2024 10:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 10 05:23:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 10 05:23:17 2024
Response via : Initial Calibration

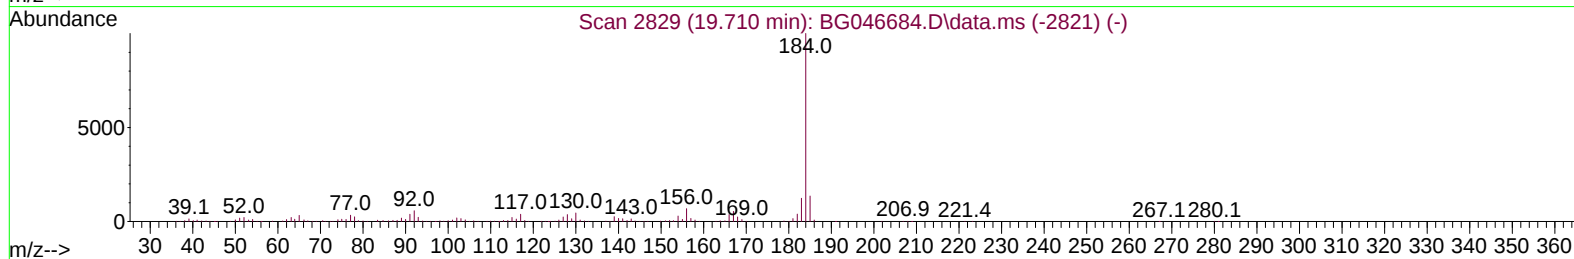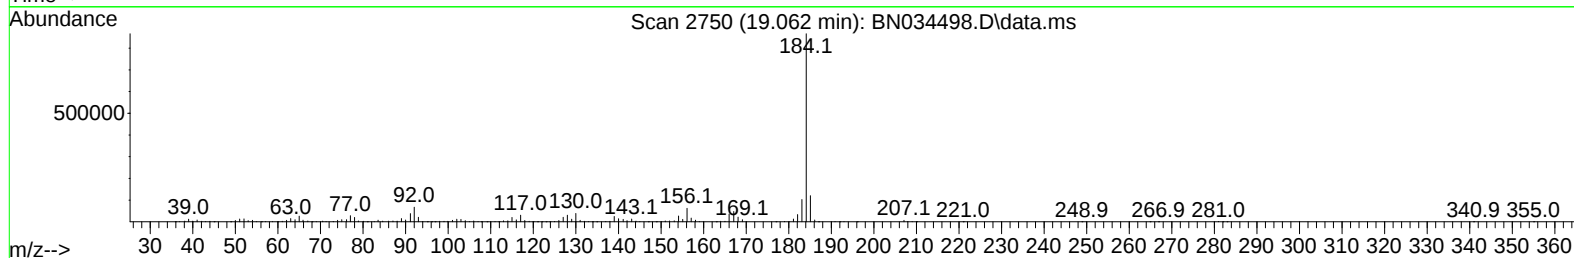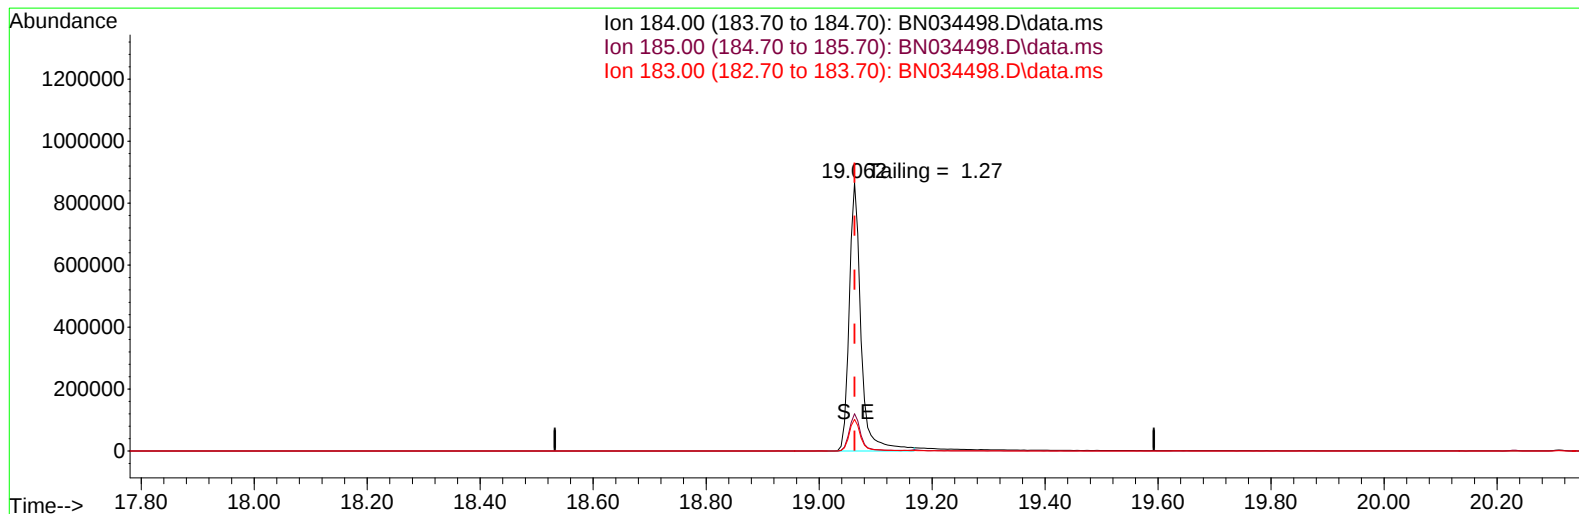

TIC: BN034498.D\data.ms

(77) Benzidine

19.062min (0.000) 0.00 ng

response 1287716

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	11.85
0.00	0.00	0.00