
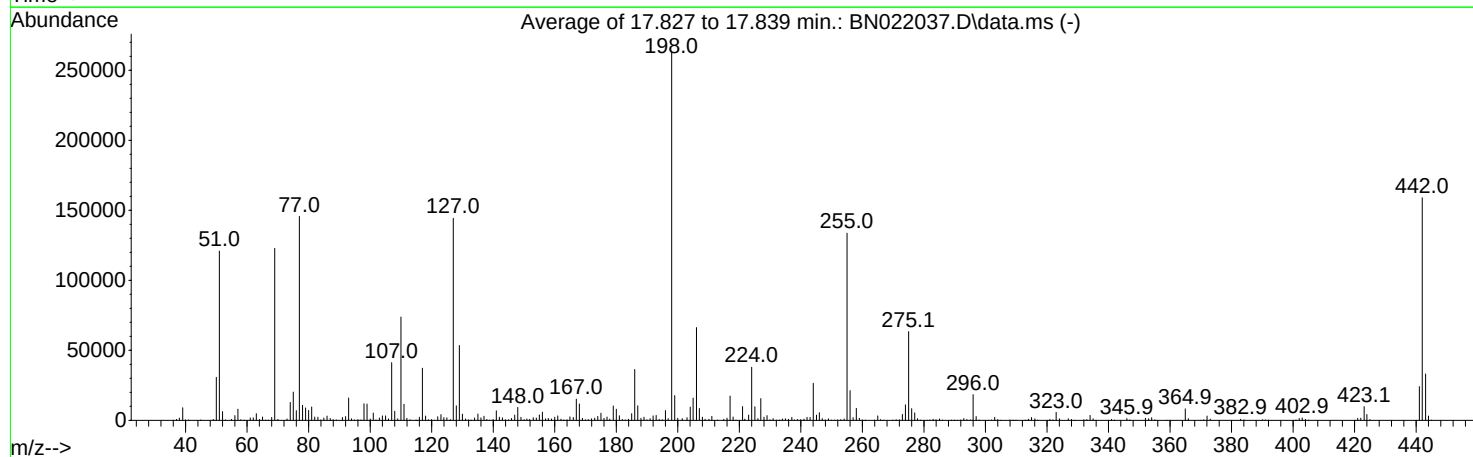


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101022\
 Data File : BN022037.D
 Acq On : 10 Oct 2022 12:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 11 04:42:07 2022

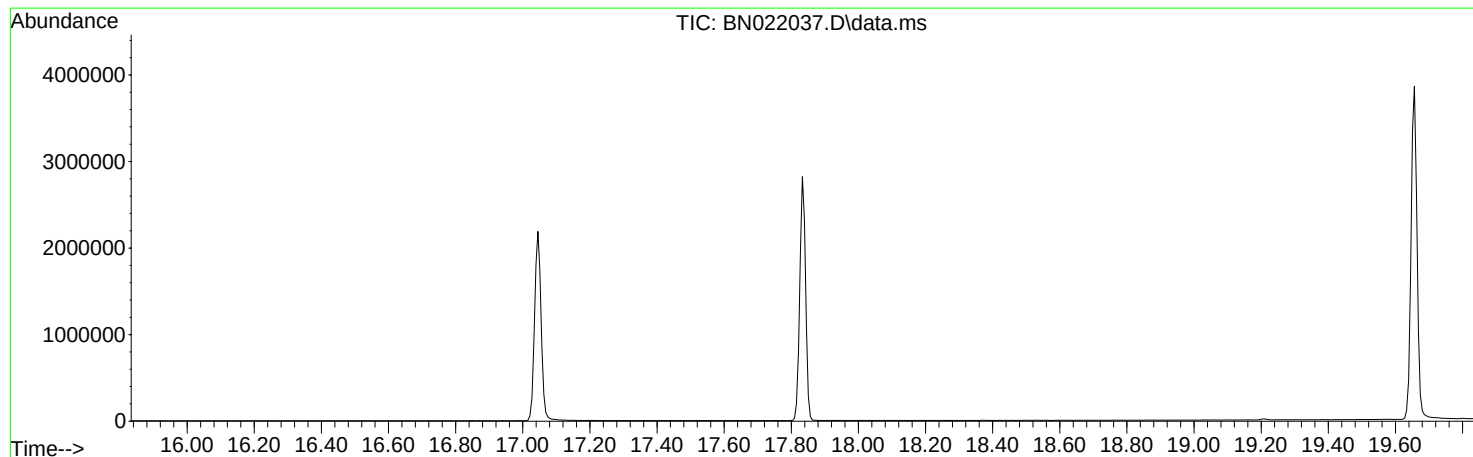




AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	120856	PASS
68	69	0.00	2	1.7	2049	PASS
69	198	0.00	100	46.7	122797	PASS
70	69	0.00	2	0.5	636	PASS
127	198	10	80	54.9	144341	PASS
197	198	0.00	2	0.5	1191	PASS
198	198	100	100	100.0	262763	PASS
199	198	5	9	6.7	17631	PASS
275	198	10	60	24.1	63411	PASS
365	198	1	100	3.1	8165	PASS
441	198	0.01	100	9.2	24063	PASS
442	442	50	100	100.0	158885	PASS
443	442	15	24	20.8	33064	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101022\
Data File : BN022037.D
Acq On : 10 Oct 2022 12:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 11 05:43:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 05:43:06 2022
Response via : Initial Calibration

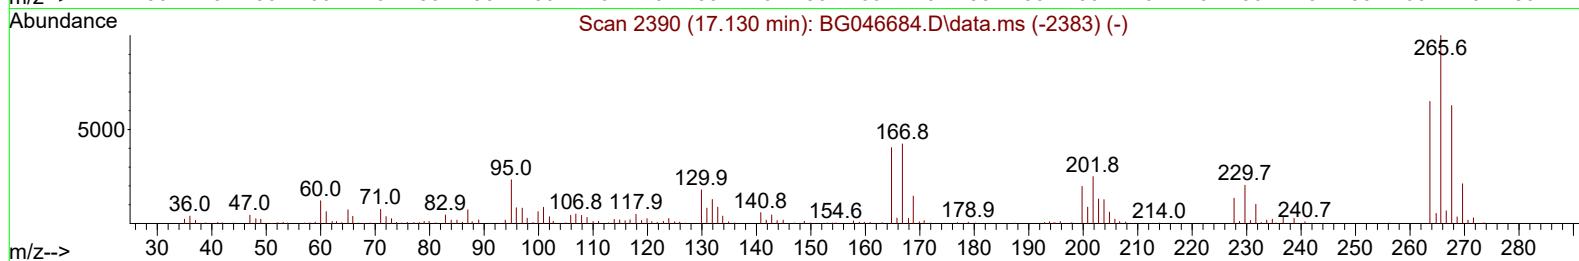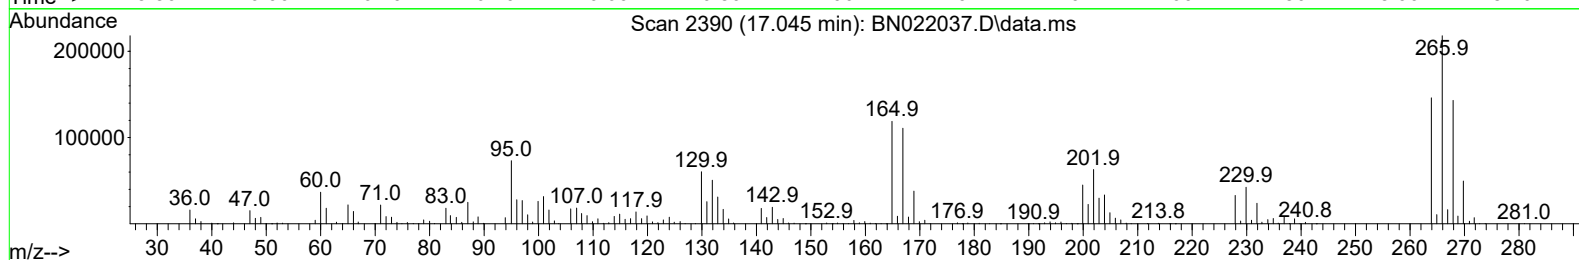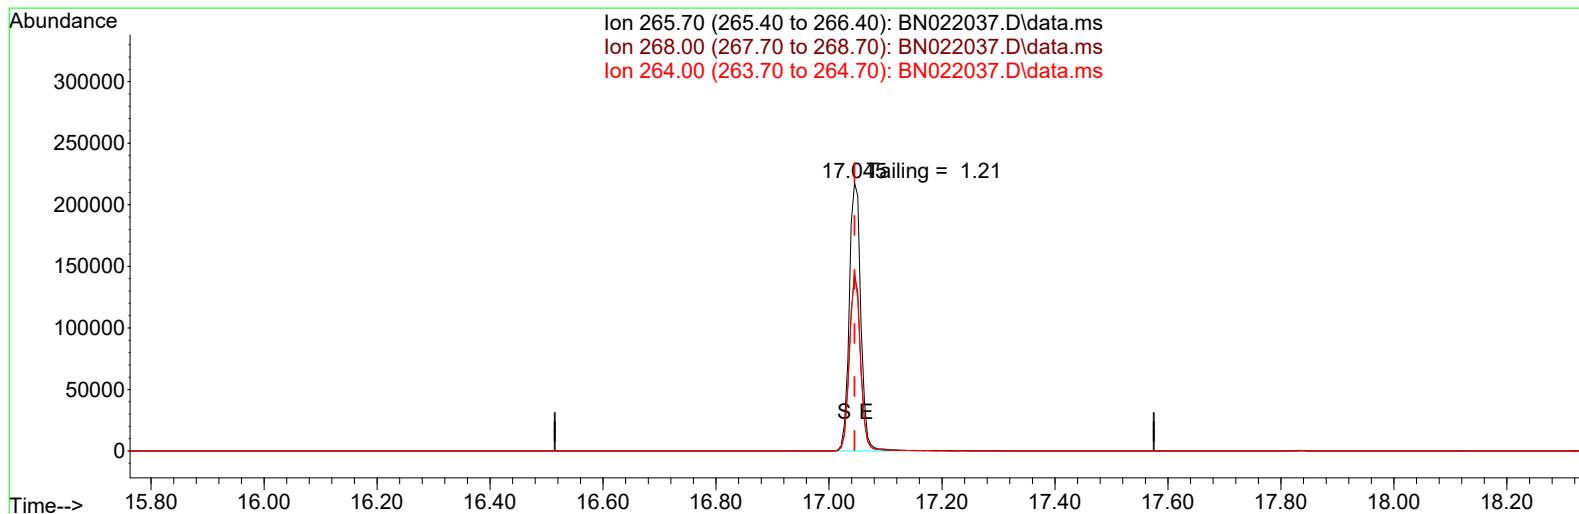

TIC: BN022037.D\data.ms

(70) Pentachlorophenol (C)

17.045min (0.000) 20209.66 ng




response 310698

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.65
264.00	61.60	66.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101022\
Data File : BN022037.D
Acq On : 10 Oct 2022 12:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 11 05:43:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 05:43:06 2022
Response via : Initial Calibration

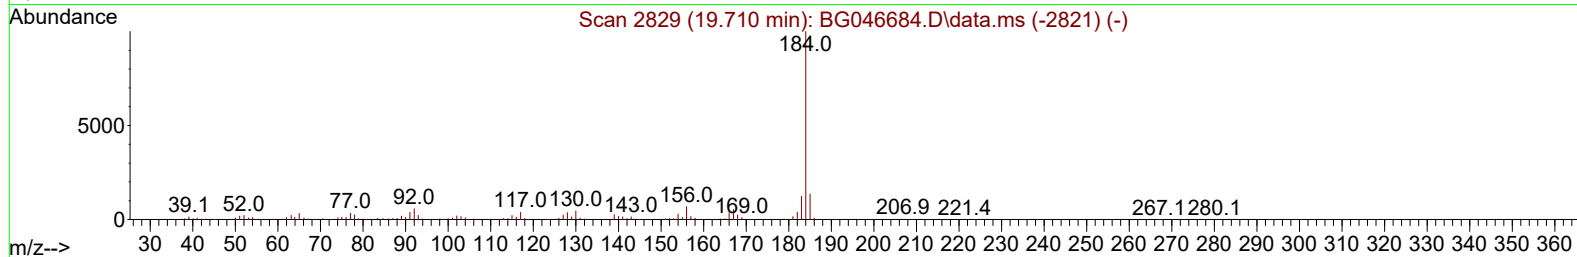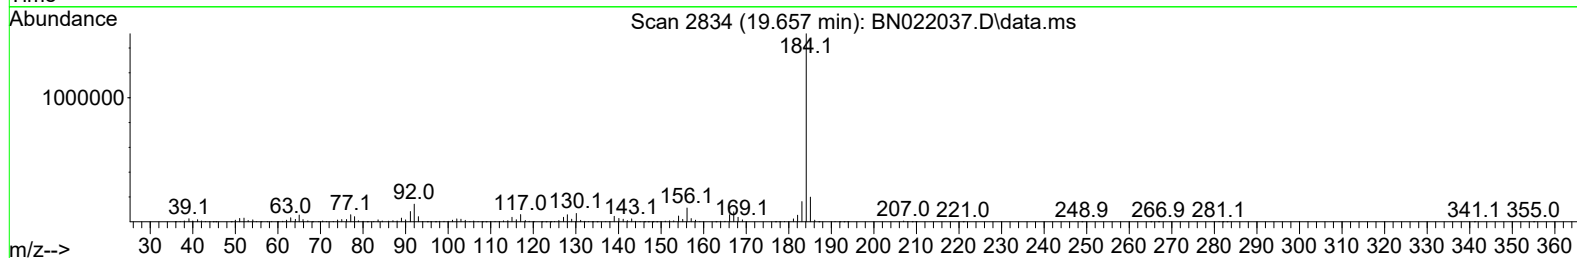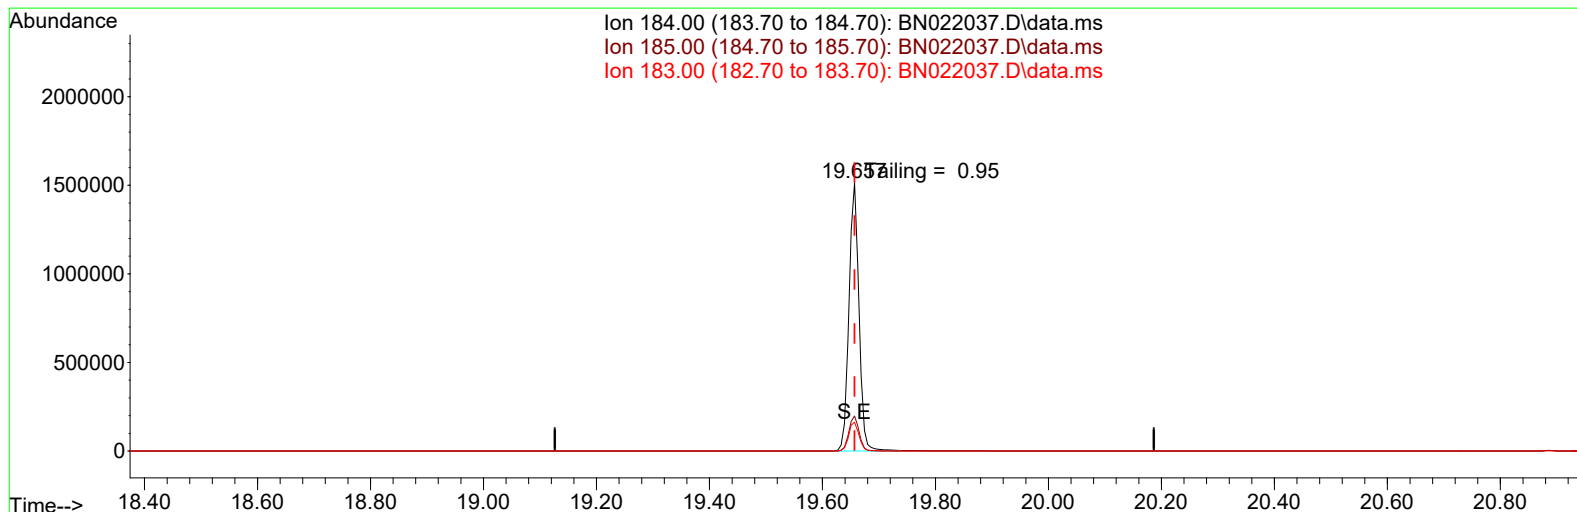

TIC: BN022037.D\data.ms

(77) Benzidine

19.657min (0.000) 0.00 ng

response 1873894

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.09
183.00	13.20	10.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/10/2022	BNA_N	<u>BN022037.D</u>
Compound Name	Response	Retention Time
DDT	874553	20.886
DDD	8351	20.445
DDE	914	19.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9265	883818	1.05

Instrument :
BNA_N
ClientSampleId :
DFTPP