
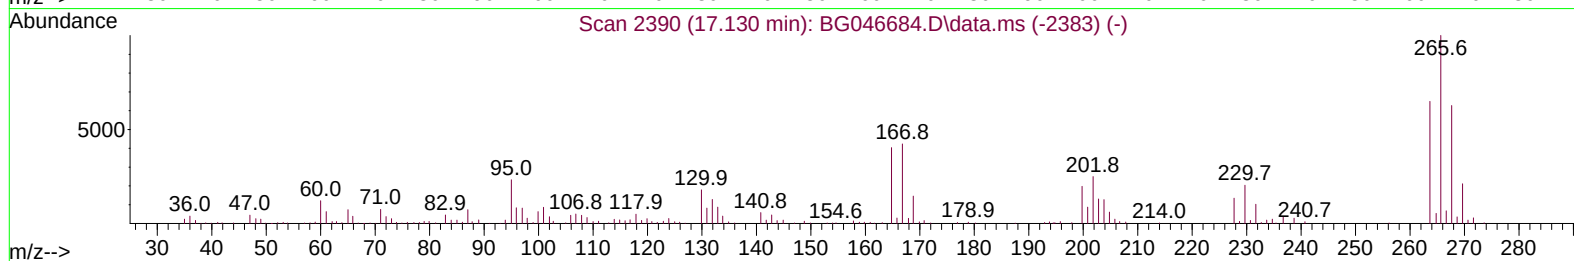
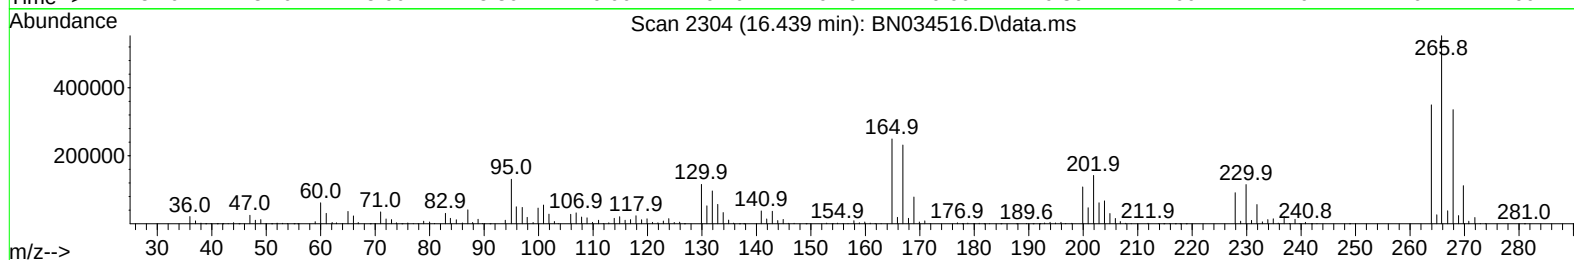


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101024\
Data File : BN034516.D
Acq On : 10 Oct 2024 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 92 Sample Multiplier: 1

Quant Time: Oct 11 04:32:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 11 04:32:47 2024
Response via : Initial Calibration

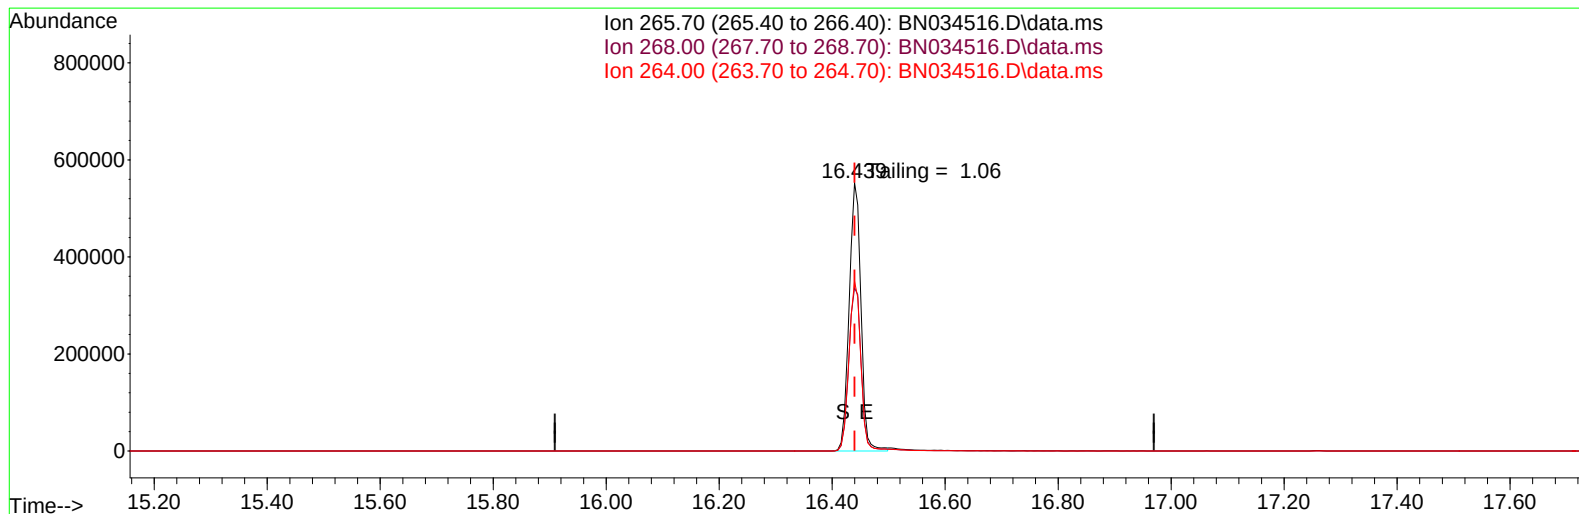

TIC: BN034516.D\data.ms

(70) Pentachlorophenol (C)




16.439min (0.000) 421660.19 ng

response 797489

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.68
264.00	61.60	63.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101024\
Data File : BN034516.D
Acq On : 10 Oct 2024 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 92 Sample Multiplier: 1

Quant Time: Oct 11 04:32:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 11 04:32:47 2024
Response via : Initial Calibration

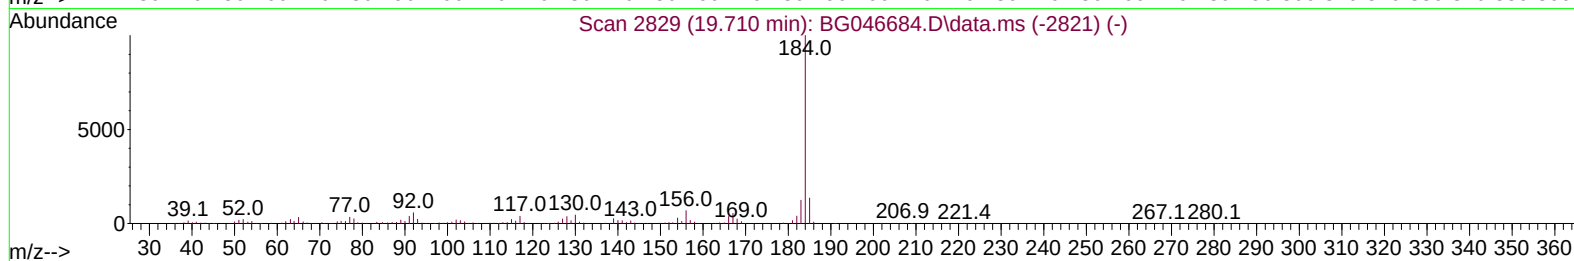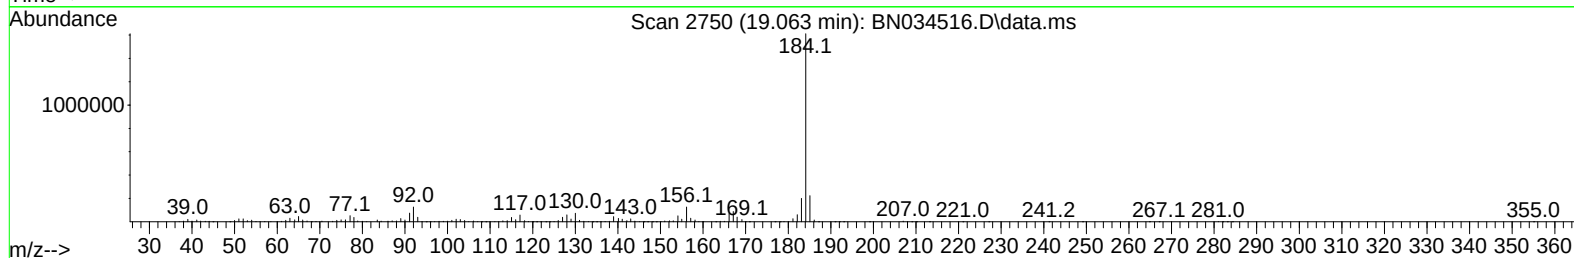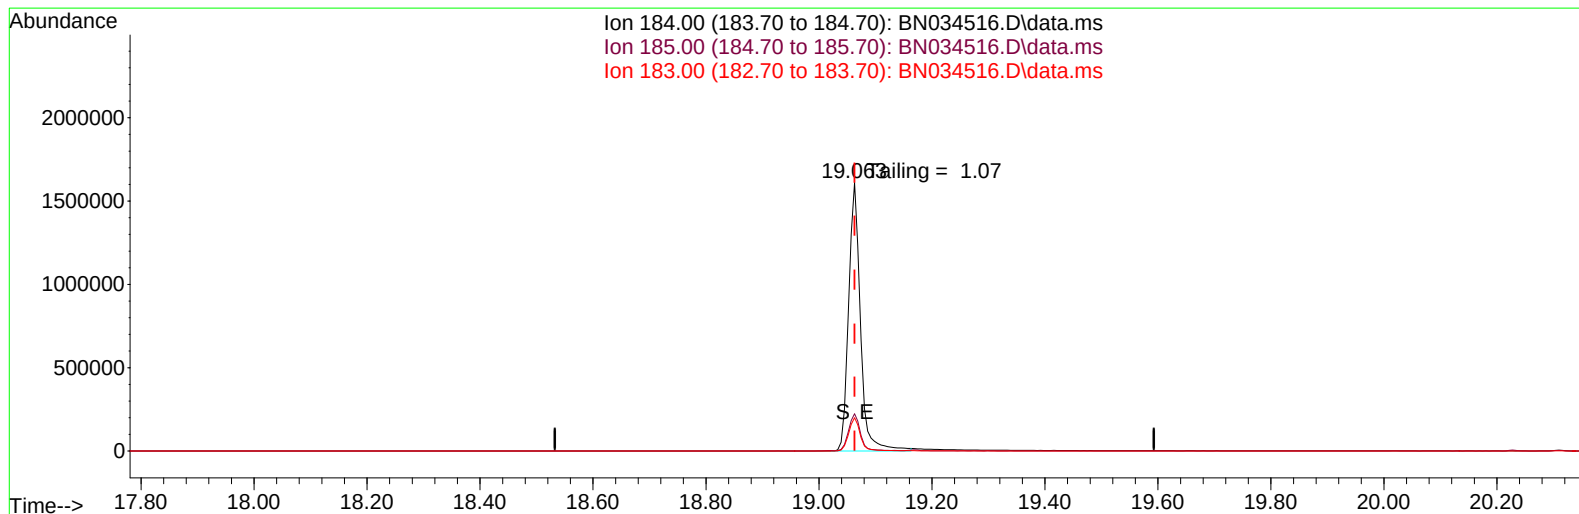

TIC: BN034516.D\data.ms

(77) Benzidine**19.063min (0.000) 134287.98 ng****response 2405036**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.88
183.00	13.20	12.42
0.00	0.00	0.00