

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101024\
 Data File : BN034537.D
 Acq On : 11 Oct 2024 02:02
 Operator : RC/JU
 Sample : PB163903BL
 Misc :
 ALS Vial : 113 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB163903BL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 10/11/2024
 Supervised By :mohammad ahmed 10/14/2024

Quant Time: Oct 11 02:31:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 00:21:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.380	152	3859	0.400	ng	0.00
7) Naphthalene-d8	10.148	136	10903	0.400	ng	0.02
13) Acenaphthene-d10	14.030	164	6019	0.400	ng	0.01
19) Phenanthrene-d10	16.808	188	10284	0.400	ng	# 0.03
29) Chrysene-d12	21.017	240	6672	0.400	ng	0.01
35) Perylene-d12	23.119	264	8124	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.018	112	3793	0.346	ng	0.00
5) Phenol-d6	6.614	99	3439m	0.270	ng	0.04
8) Nitrobenzene-d5	8.557	82	2354m	0.282	ng	0.04
11) 2-Methylnaphthalene-d10	11.761	152	5813m	0.361	ng	0.03
14) 2,4,6-Tribromophenol	15.567	330	638m	0.234	ng	0.03
15) 2-Fluorobiphenyl	12.661	172	8252m	0.337	ng	0.03
27) Fluoranthene-d10	18.839	212	9697	0.374	ng	0.01
31) Terphenyl-d14	19.456	244	6149	0.461	ng	0.00

Target Compounds Qvalue

 (#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101024\
Data File : BN034537.D
Acq On : 11 Oct 2024 02:02
Operator : RC/JU
Sample : PB163903BL
Misc :
ALS Vial : 113 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB163903BL

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 10/11/2024
Supervised By :mohammad ahmed 10/14/2024


Quant Time: Oct 11 02:31:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 11 00:21:08 2024
Response via : Initial Calibration

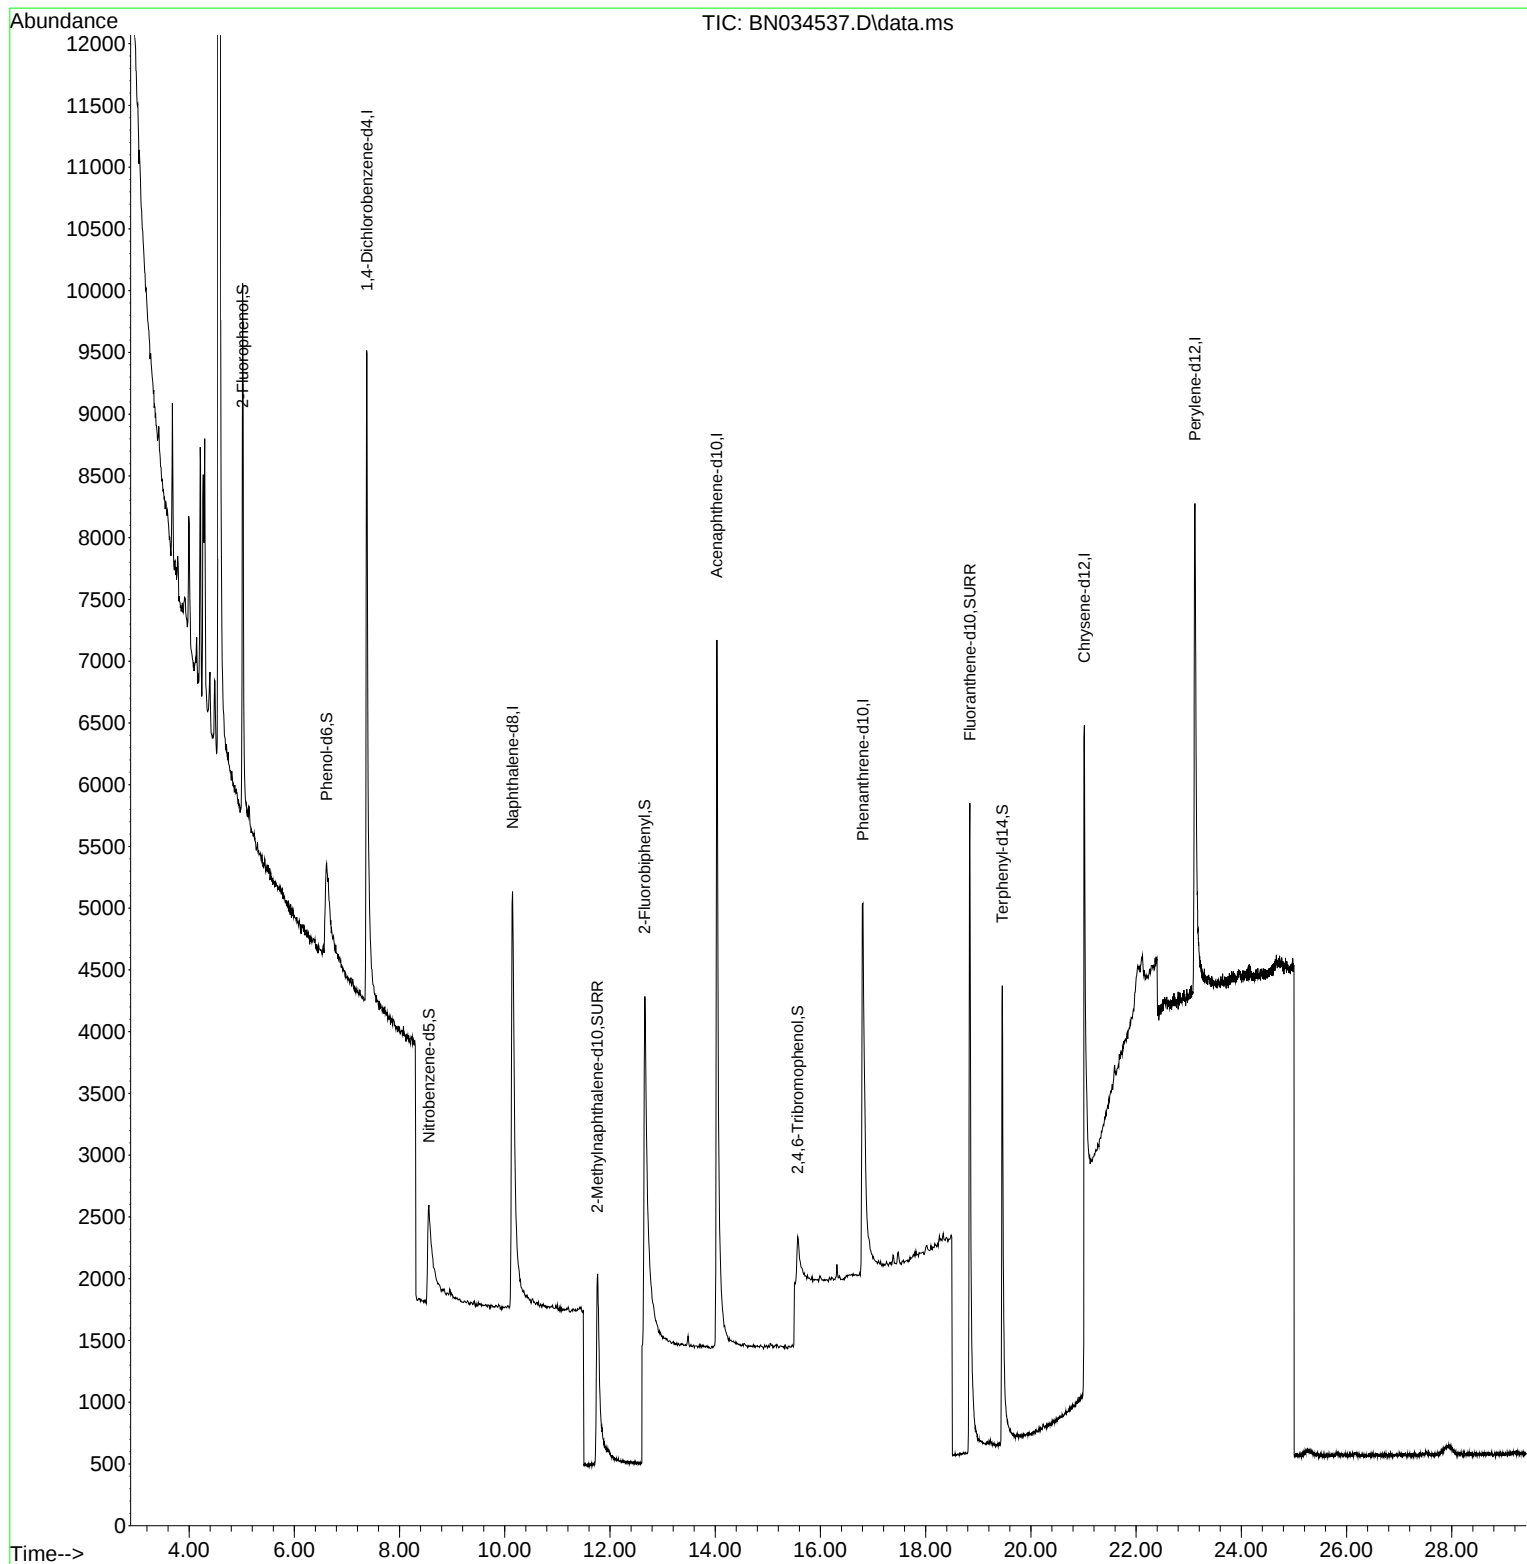



#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.380 min Scan# 617
Delta R.T. 0.007 min
Lab File: BN034537.D
Acq: 11 Oct 2024 02:02




Instrument :
BNA_N
ClientSampleId :
PB163903BL

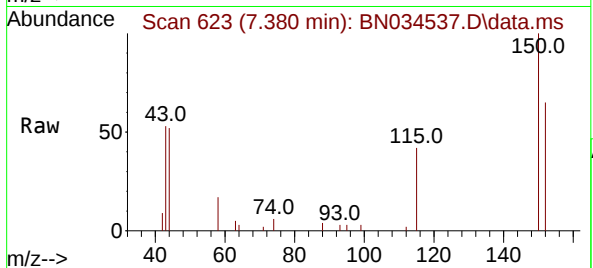


Tgt Ion:152 Resp: 3859
Ion Ratio Lower Upper
152 100
150 154.0 124.6 187.0
115 64.4 50.0 75.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 10/11/2024
Supervised By :mohammad ahmed 10/14/2024

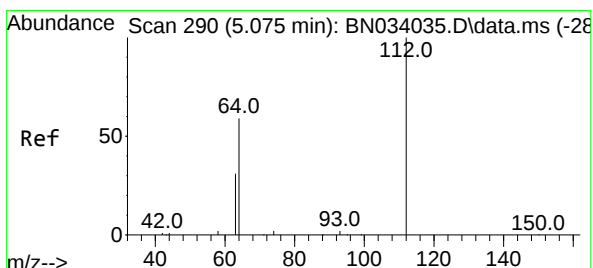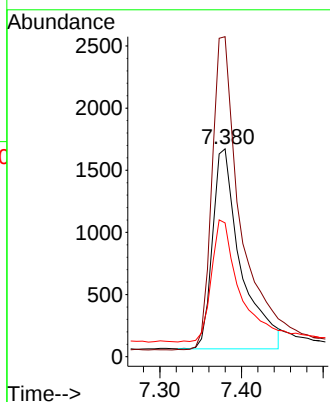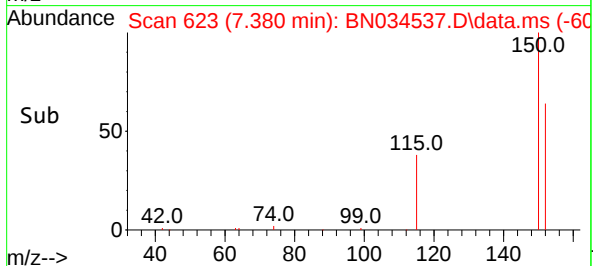


#4
2-Fluorophenol
Concen: 0.346 ng
RT: 5.018 min Scan# 296
Delta R.T. 0.007 min
Lab File: BN034537.D
Acq: 11 Oct 2024 02:02

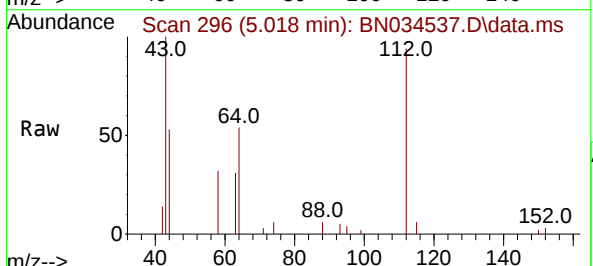


Tgt Ion:112 Resp: 3793
Ion Ratio Lower Upper
112 100
64 55.5 48.6 72.8
63 30.0 25.6 38.4

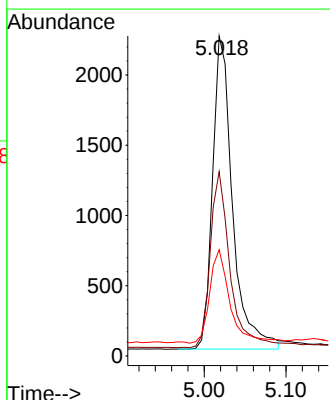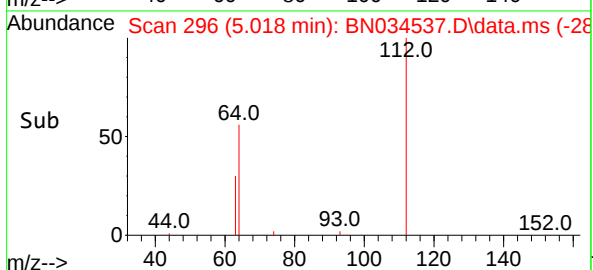

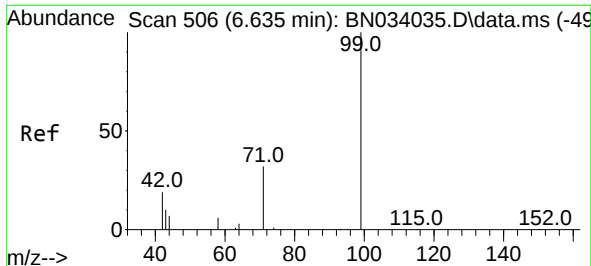

#5
Phenol-d6
Concen: 0.270 ng m
RT: 6.614 min Scan# 517
Delta R.T. 0.043 min
Lab File: BN034537.D
Acq: 11 Oct 2024 02:02




Instrument :
BNA_N
ClientSampleId :
PB163903BL

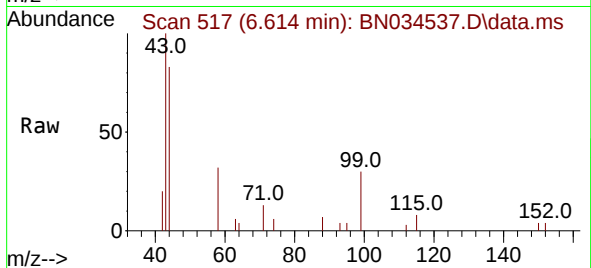

Tgt Ion: 99 Resp: 3439
Ion Ratio Lower Upper
99 100
42 8.9 17.8 26.8
71 17.7 26.2 39.2




Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 10/11/2024
Supervised By :mohammad ahmed 10/14/2024

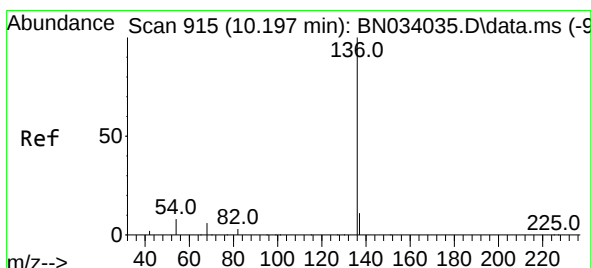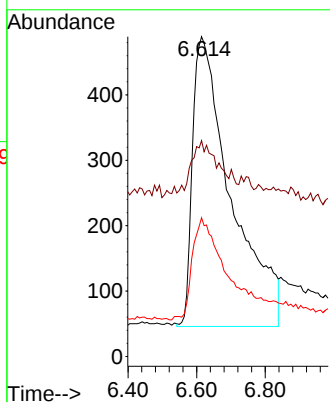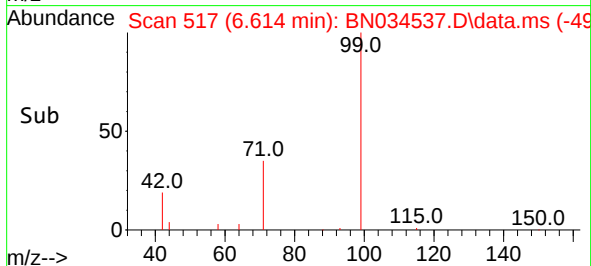

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.148 min Scan# 924
Delta R.T. 0.021 min
Lab File: BN034537.D
Acq: 11 Oct 2024 02:02


Tgt Ion:136 Resp: 10903
Ion Ratio Lower Upper
136 100
137 12.6 9.0 13.6
54 9.4 6.8 10.2
68 7.3 5.0 7.6

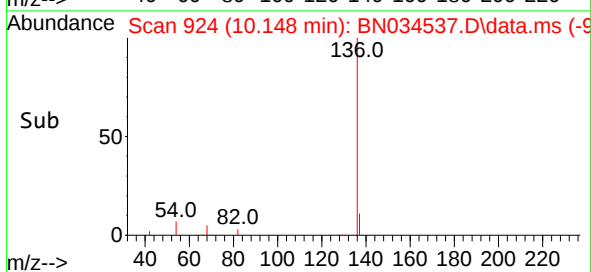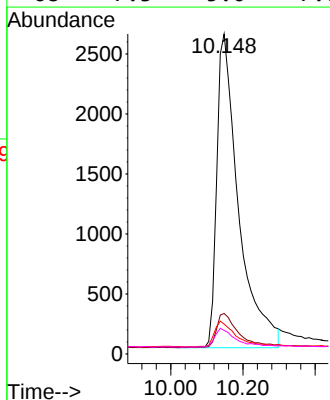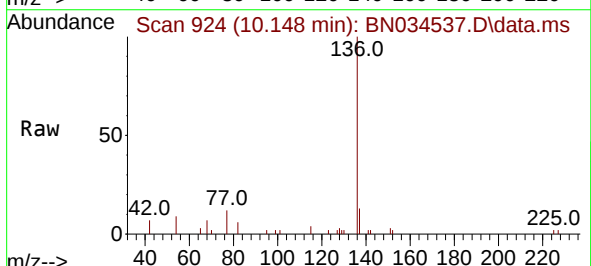



#8
Nitrobenzene-d5
Concen: 0.282 ng m
RT: 8.557 min Scan# 71
Delta R.T. 0.043 min
Lab File: BN034537.D
Acq: 11 Oct 2024 02:02




Instrument :
BNA_N
ClientSampleId :
PB163903BL

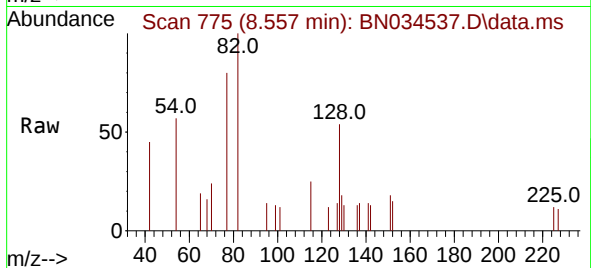

Tgt Ion: 82 Resp: 2354
Ion Ratio Lower Upper
82 100
128 54.5 31.4 47.2
54 56.9 47.4 71.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/11/2024
Supervised By :mohammad ahmed 10/14/2024

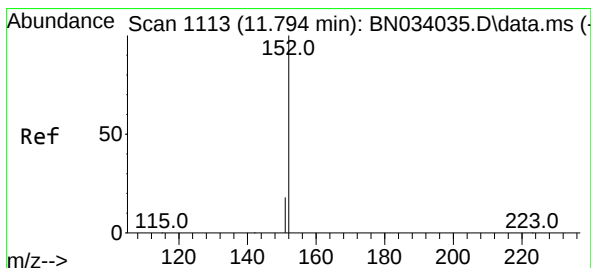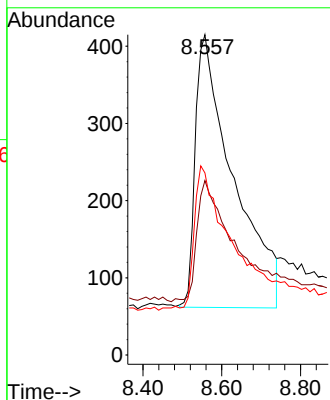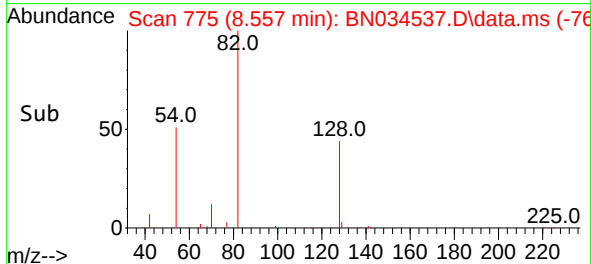

#11
2-Methylnaphthalene-d10
Concen: 0.361 ng m
RT: 11.761 min Scan# 1119
Delta R.T. 0.034 min
Lab File: BN034537.D
Acq: 11 Oct 2024 02:02


Tgt Ion:152 Resp: 5813
Ion Ratio Lower Upper
152 100
151 17.5 16.8 25.2

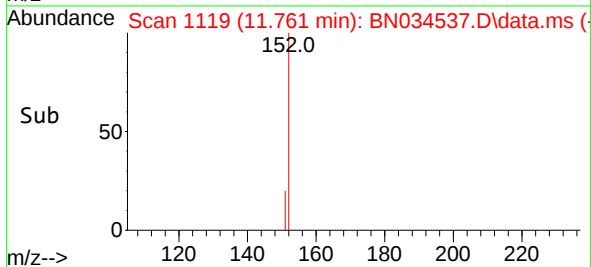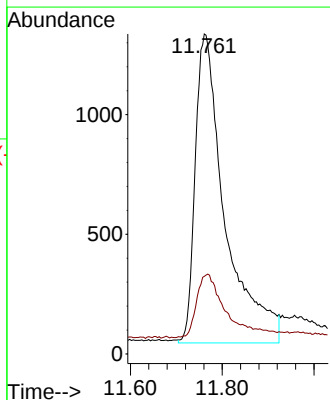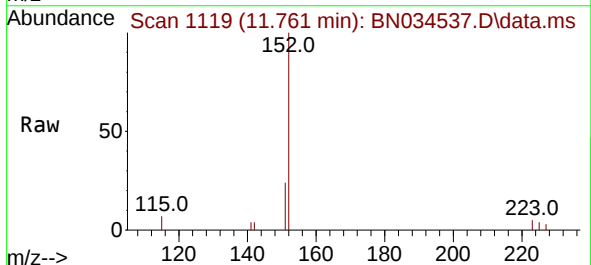

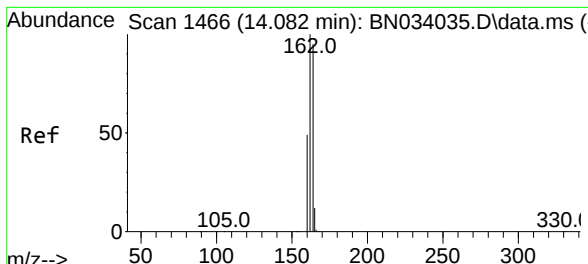

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.030 min Scan# 1466
 Delta R.T. 0.014 min
 Lab File: BN034537.D
 Acq: 11 Oct 2024 02:02




Instrument :
 BNA_N
 ClientSampleId :
 PB163903BL

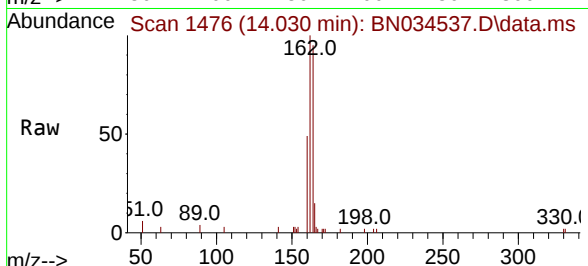


Tgt Ion:164 Resp: 6019
 Ion Ratio Lower Upper
 164 100
 162 105.4 84.2 126.2
 160 51.3 41.7 62.5

Manual Integrations
 APPROVED



Reviewed By :Jagrut Upadhyay 10/11/2024
 Supervised By :mohammad ahmed 10/14/2024

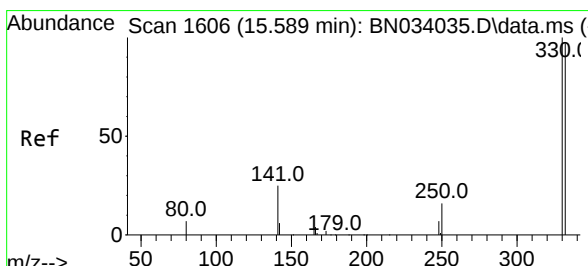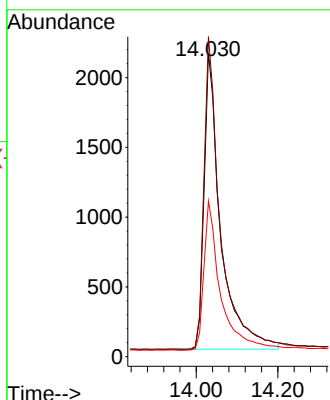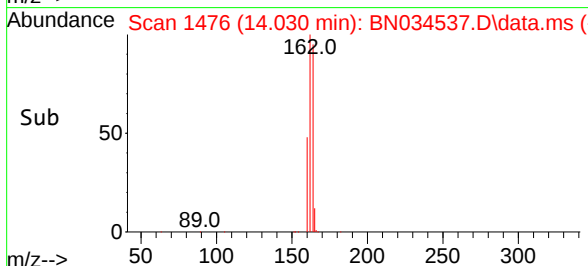


#14
 2,4,6-Tribromophenol
 Concen: 0.234 ng m
 RT: 15.567 min Scan# 1619
 Delta R.T. 0.030 min
 Lab File: BN034537.D
 Acq: 11 Oct 2024 02:02

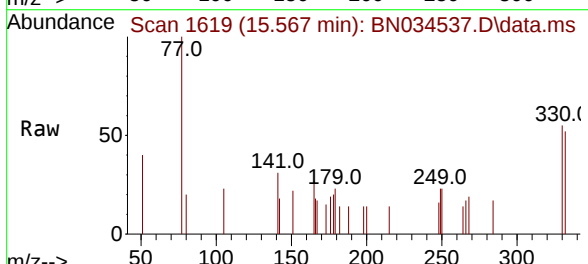


Tgt Ion:330 Resp: 638
 Ion Ratio Lower Upper
 330 100
 332 146.6 77.4 116.0#
 141 30.6 35.9 53.9#

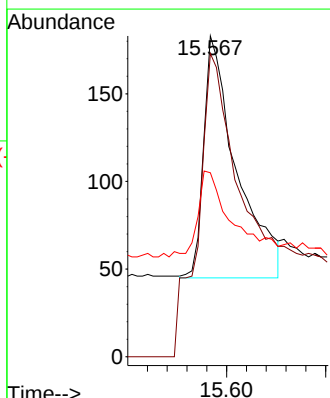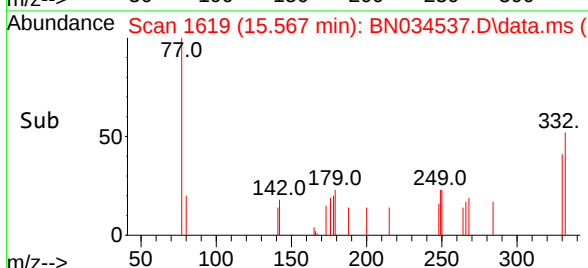

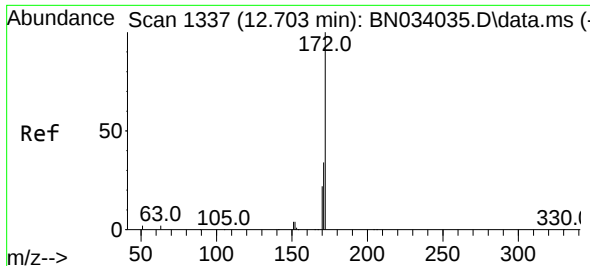

#15
2-Fluorobiphenyl
Concen: 0.337 ng m
RT: 12.661 min Scan# 11
Delta R.T. 0.025 min
Lab File: BN034537.D
Acq: 11 Oct 2024 02:02




Instrument :
BNA_N
ClientSampleId :
PB163903BL

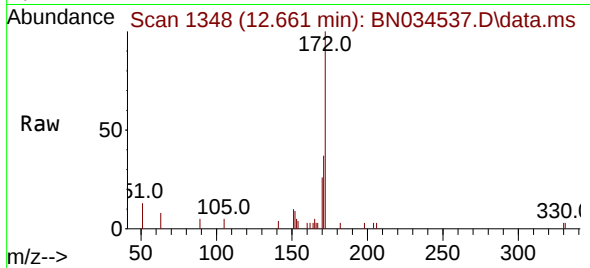


Tgt Ion:172 Resp: 825
Ion Ratio Lower Upper
172 100
171 36.8 27.3 40.9
170 26.4 18.1 27.1

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 10/11/2024
Supervised By :mohammad ahmed 10/14/2024

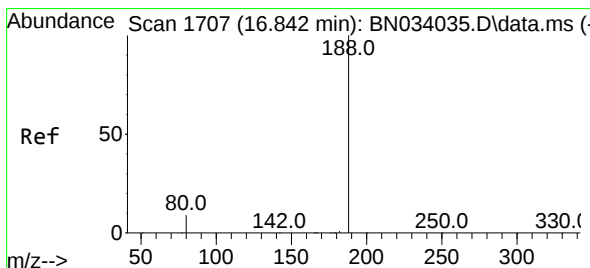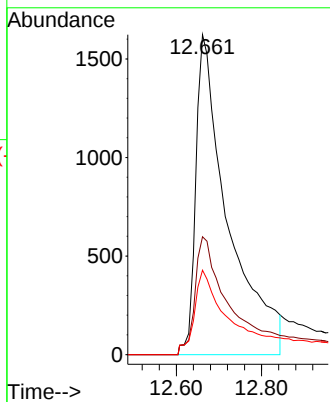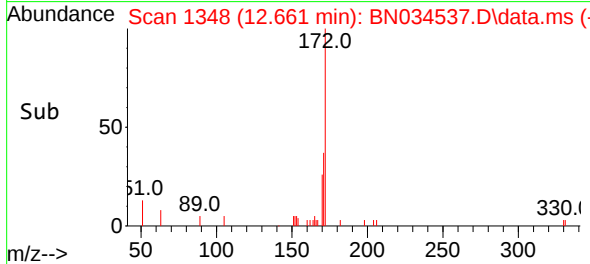


#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.808 min Scan# 1719
Delta R.T. 0.030 min
Lab File: BN034537.D
Acq: 11 Oct 2024 02:02

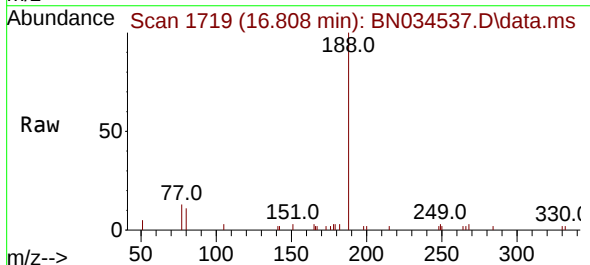

Tgt Ion:188 Resp: 10284
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.3 7.4 11.0#

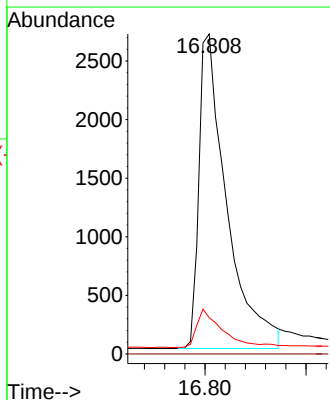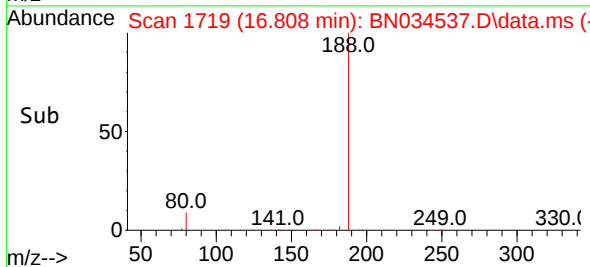

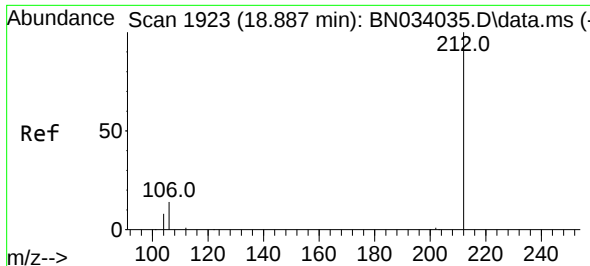


#27
Fluoranthene-d10
Concen: 0.374 ng
RT: 18.839 min Scan# 1927
Delta R.T. 0.012 min
Lab File: BN034537.D
Acq: 11 Oct 2024 02:02

Instrument :

BNA_N

ClientSampleId :

PB163903BL



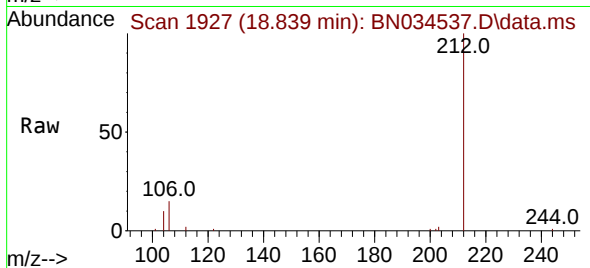


Tgt Ion:212 Resp: 969
Ion Ratio Lower Upper
212 100
106 14.8 13.4 20.2
104 8.8 7.8 11.6


Manual Integrations

APPROVED



Reviewed By :Jagrut Upadhyay 10/11/2024
Supervised By :mohammad ahmed 10/14/2024

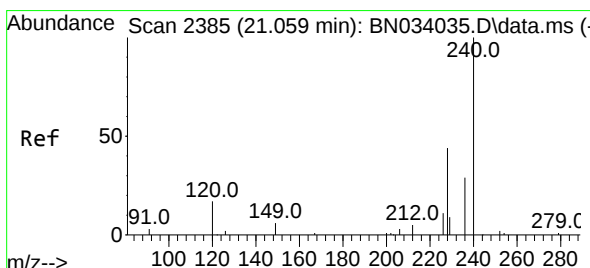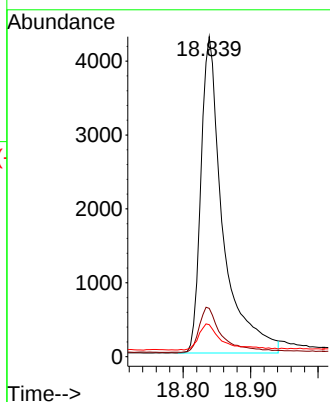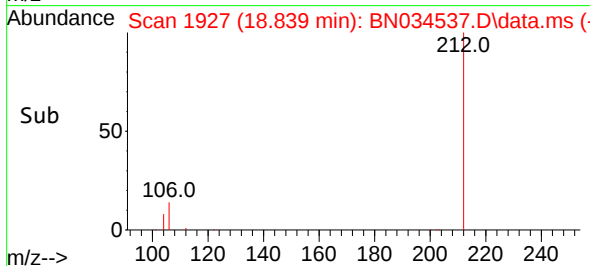


#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.017 min Scan# 2395
Delta R.T. 0.011 min
Lab File: BN034537.D
Acq: 11 Oct 2024 02:02

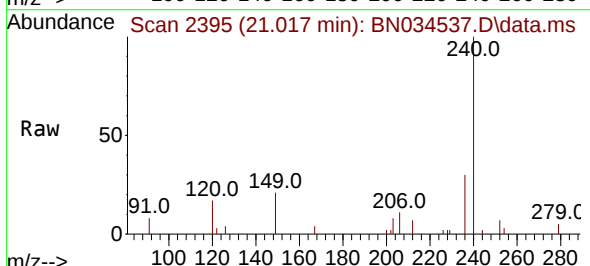

Tgt Ion:240 Resp: 6672
Ion Ratio Lower Upper
240 100
120 17.4 13.5 20.3
236 30.1 23.4 35.0

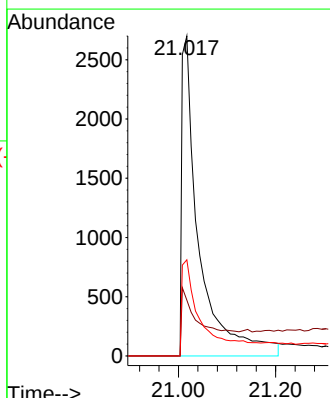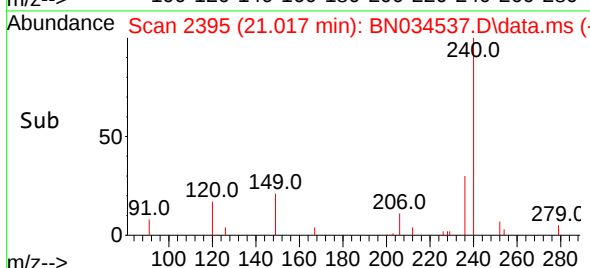

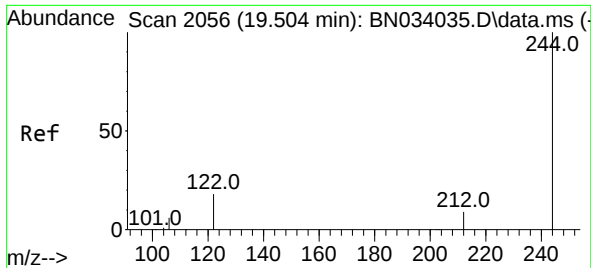

#31
 Terphenyl-d14
 Concen: 0.461 ng
 RT: 19.456 min Scan# 2056
 Delta R.T. 0.007 min
 Lab File: BN034537.D
 Acq: 11 Oct 2024 02:02

Instrument :

BNA_N

ClientSampleId :





PB163903BL

Tgt Ion:244 Resp: 6149
 Ion Ratio Lower Upper
 244 100
 212 10.2 7.8 11.6
 122 17.1 14.8 22.2

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 10/11/2024
 Supervised By :mohammad ahmed 10/14/2024

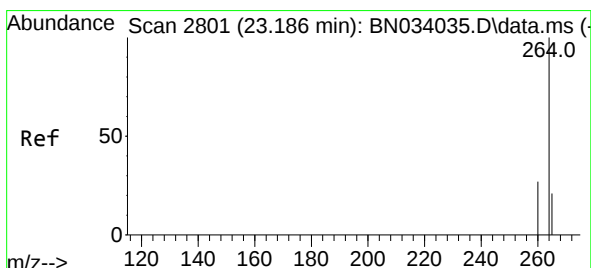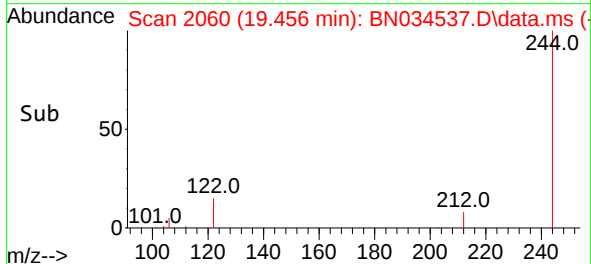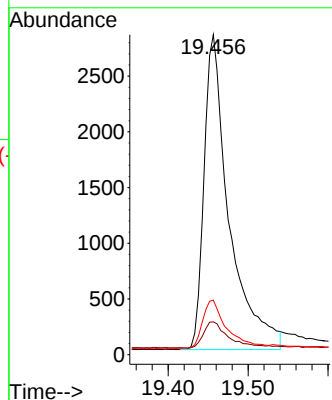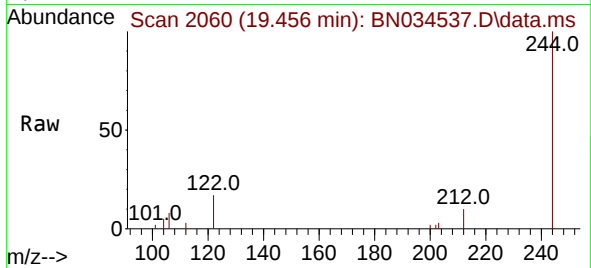

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.119 min Scan# 2794
 Delta R.T. 0.005 min
 Lab File: BN034537.D
 Acq: 11 Oct 2024 02:02

Tgt Ion:264 Resp: 8124
 Ion Ratio Lower Upper
 264 100
 260 27.6 21.7 32.5
 265 118.2 52.1 78.1#

