


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101024\
Data File : BN034516.D
Acq On : 10 Oct 2024 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 11 00:21:08 2024

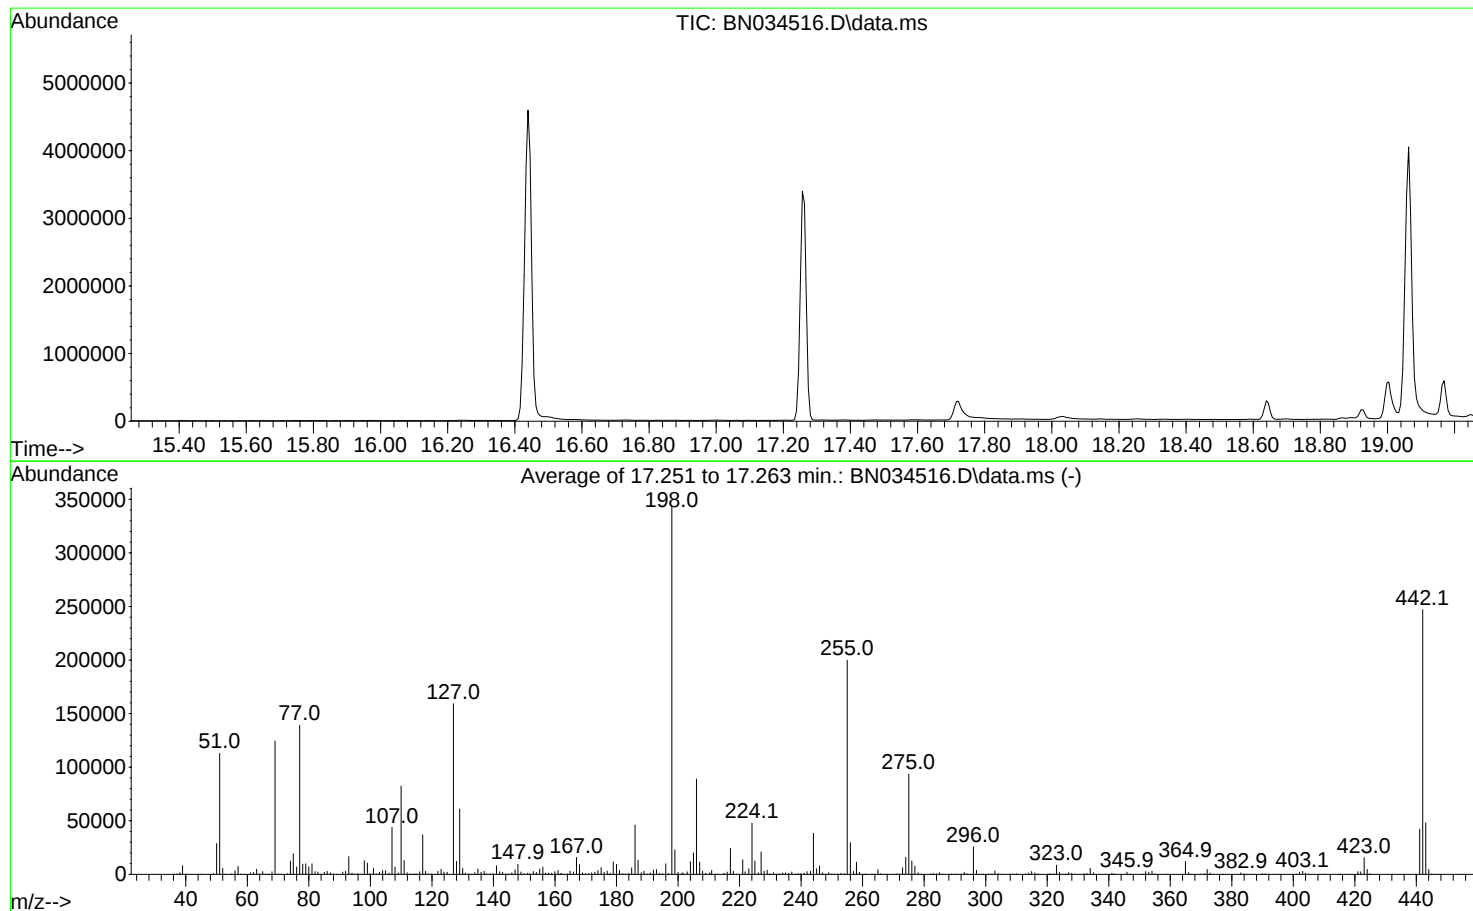




AutoFind: Scans 2442, 2443, 2444; Background Corrected with Scan 2436

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	112952	PASS
68	69	0.00	2	1.9	2421	PASS
69	198	0.00	100	36.3	124460	PASS
70	69	0.00	2	0.4	496	PASS
127	198	10	80	46.4	159387	PASS
197	198	0.00	2	0.2	778	PASS
198	198	100	100	100.0	343275	PASS
199	198	5	9	6.7	22845	PASS
275	198	10	60	27.2	93501	PASS
365	198	1	100	3.5	11904	PASS
441	198	0.01	100	12.3	42184	PASS
442	442	50	100	100.0	247189	PASS
443	442	15	24	19.4	48032	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101024\
Data File : BN034516.D
Acq On : 10 Oct 2024 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 11 04:32:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 11 04:32:47 2024
Response via : Initial Calibration

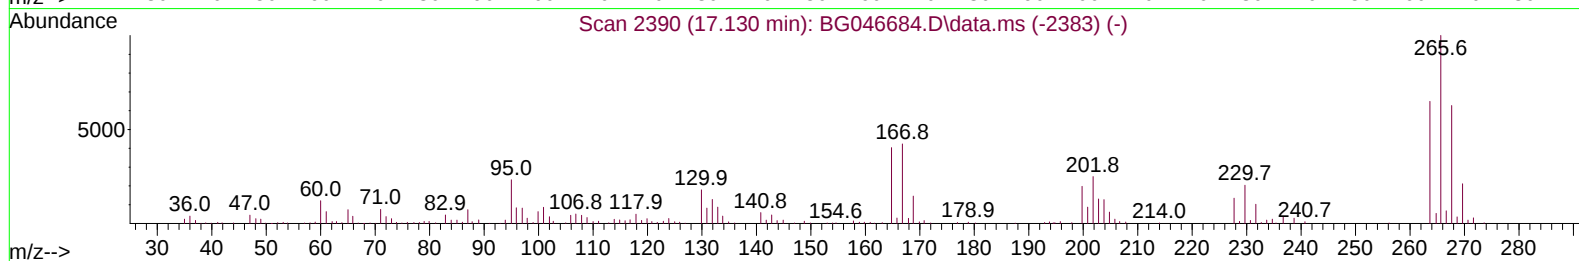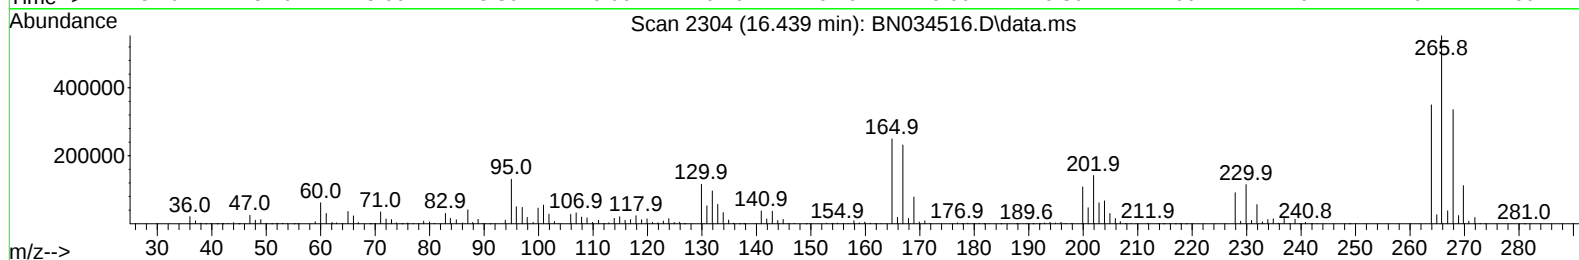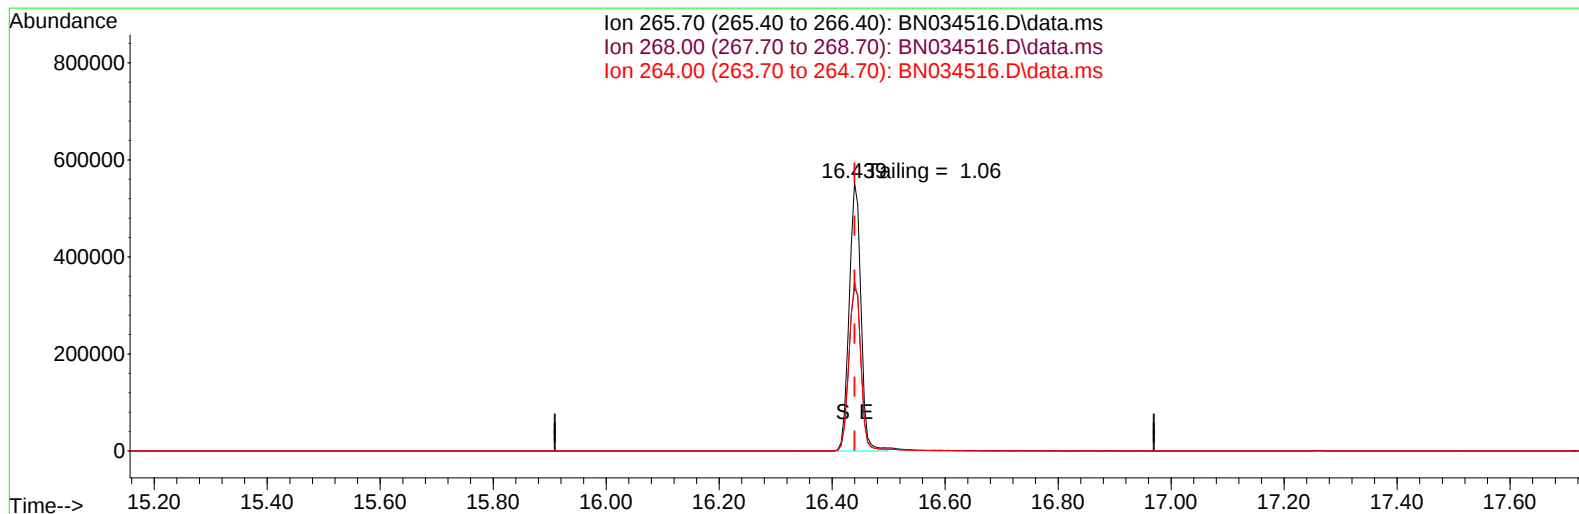

TIC: BN034516.D\data.ms

(70) Pentachlorophenol (C)

16.439min (0.000) 421660.19 ng




response 797489

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.68
264.00	61.60	63.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101024\
Data File : BN034516.D
Acq On : 10 Oct 2024 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 11 04:32:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 11 04:32:47 2024
Response via : Initial Calibration

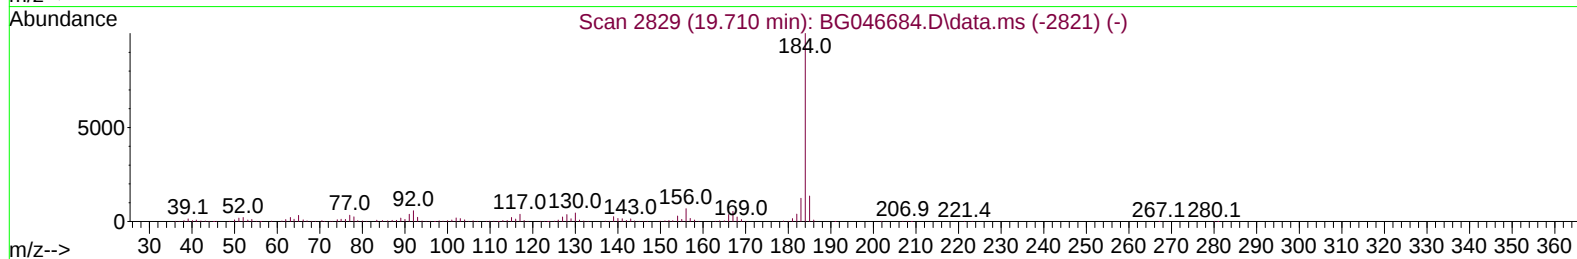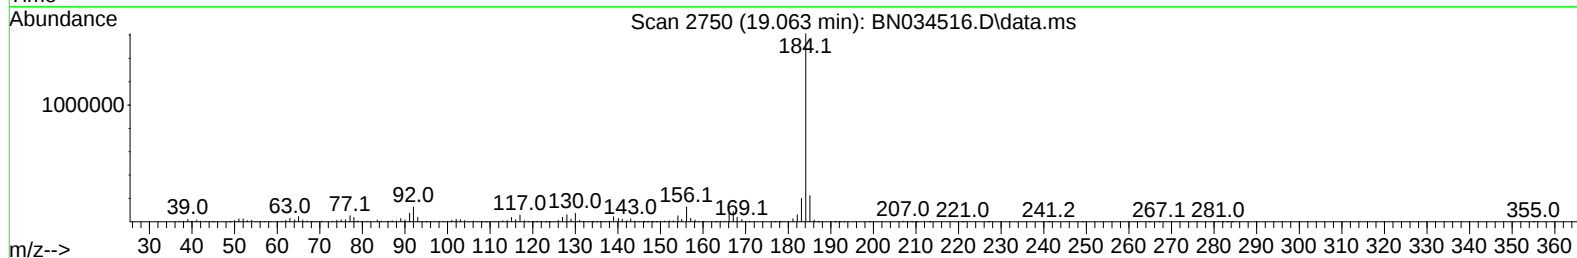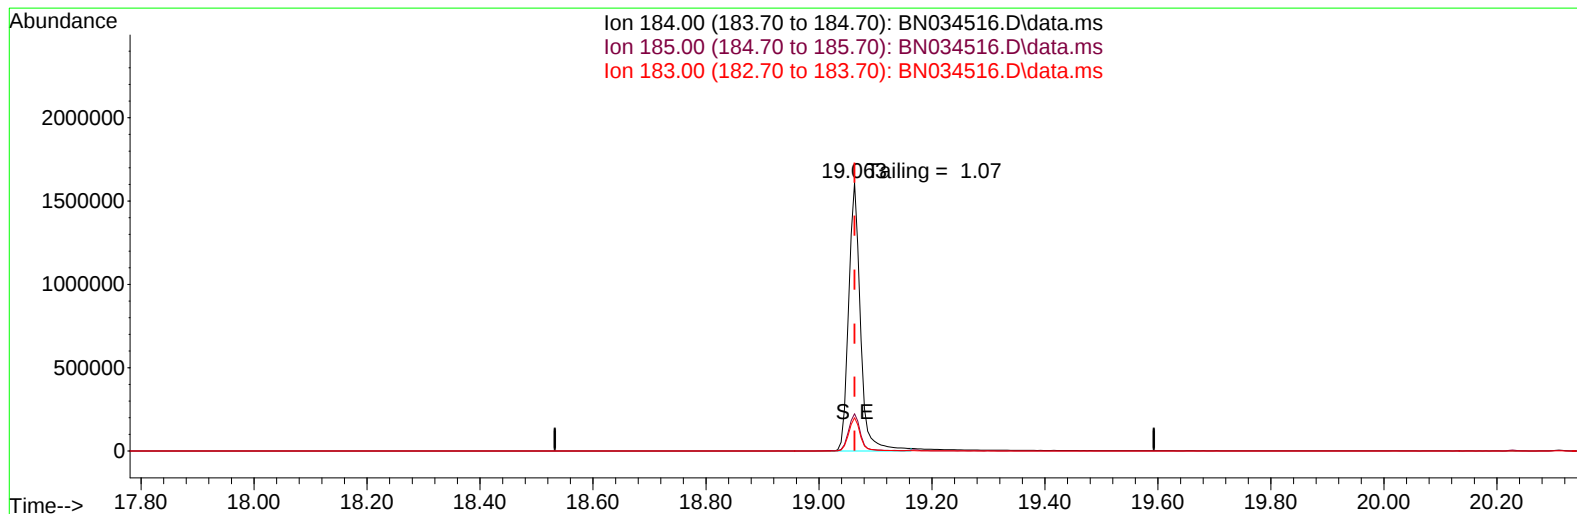

TIC: BN034516.D\data.ms

(77) Benzidine

19.063min (0.000) 134287.98 ng

response 2405036

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.88
183.00	13.20	12.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/10/2024	BNA_N	<u>BN034516.D</u>
Compound Name	Response	Retention Time
DDT	1282147	20.31
DDD	72837	19.869
DDE	1417	19.351
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
74254	1356401	5.47

Instrument :
BNA_N
ClientSampleId :
DFTPP