


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101024\
Data File : BN034535.D
Acq On : 11 Oct 2024 00:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 111 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 11 00:21:08 2024

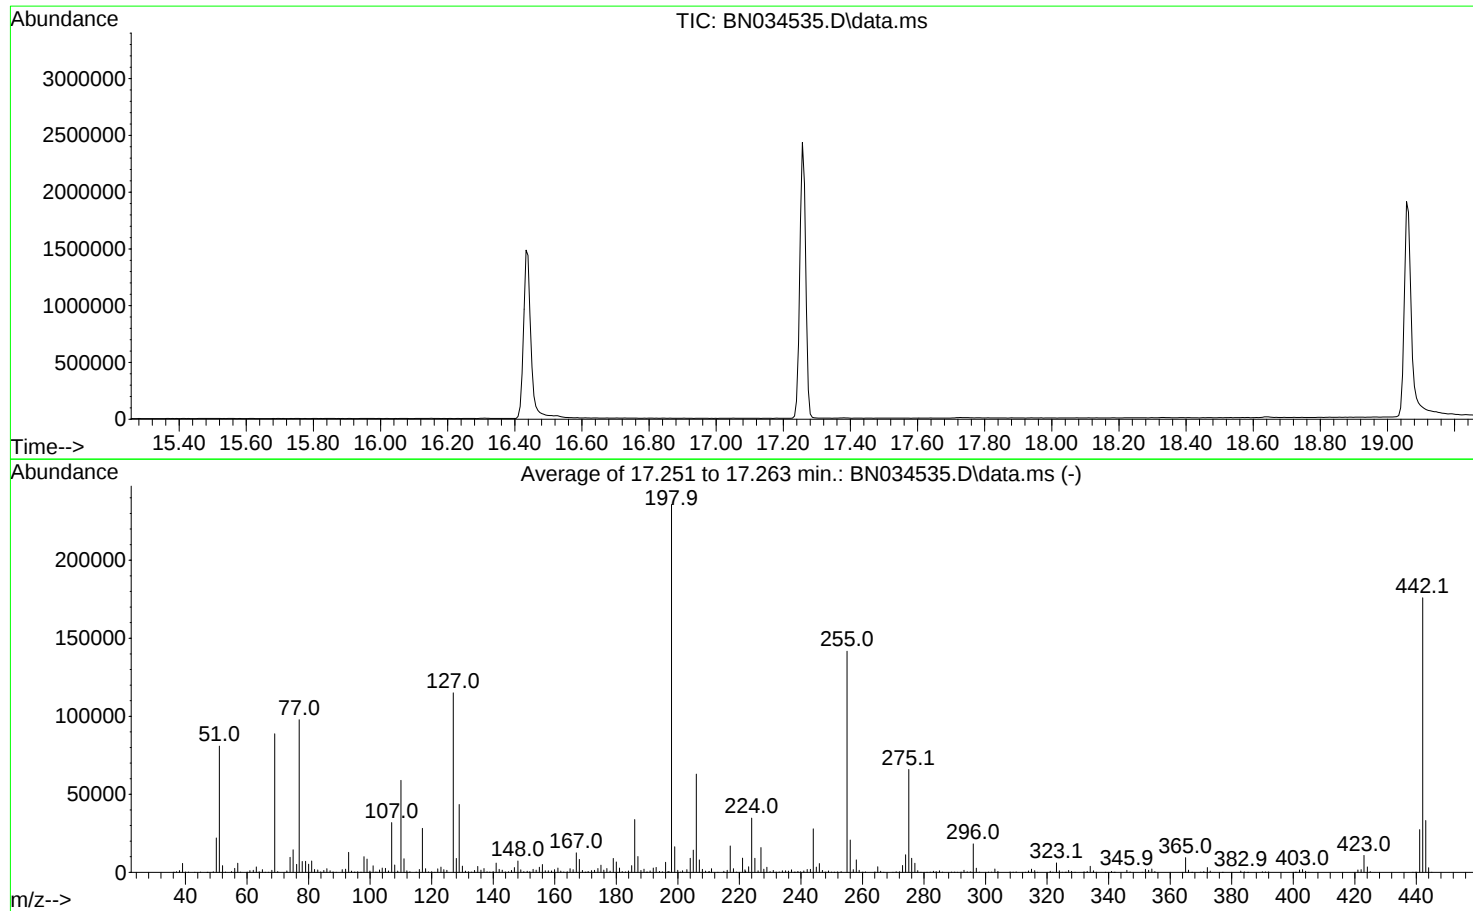




AutoFind: Scans 2442, 2443, 2444; Background Corrected with Scan 2436

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	80864	PASS
68	69	0.00	2	1.5	1298	PASS
69	198	0.00	100	37.7	88816	PASS
70	69	0.00	2	0.6	493	PASS
127	198	10	80	48.8	115000	PASS
197	198	0.00	2	0.3	635	PASS
198	198	100	100	100.0	235712	PASS
199	198	5	9	7.0	16387	PASS
275	198	10	60	28.0	65928	PASS
365	198	1	100	4.0	9449	PASS
441	198	0.01	100	11.6	27387	PASS
442	442	50	100	100.0	175896	PASS
443	442	15	24	18.9	33243	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101024\
Data File : BN034535.D
Acq On : 11 Oct 2024 00:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 111 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 11 04:35:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 11 04:35:48 2024
Response via : Initial Calibration

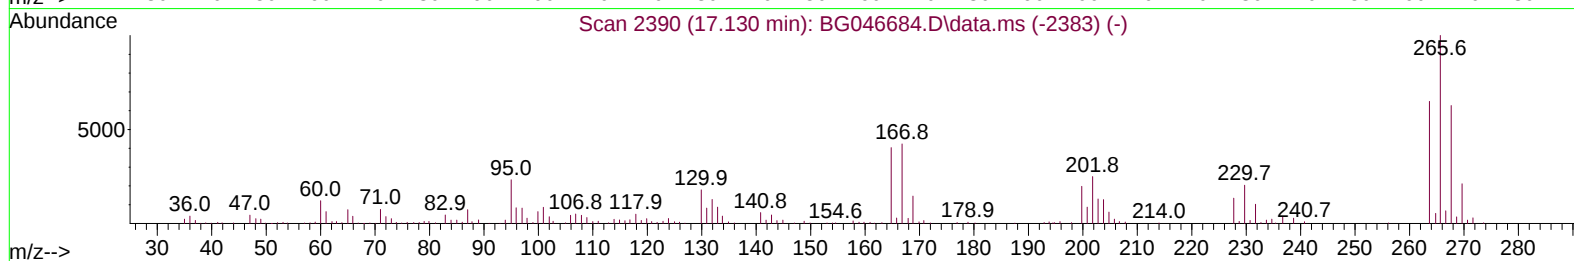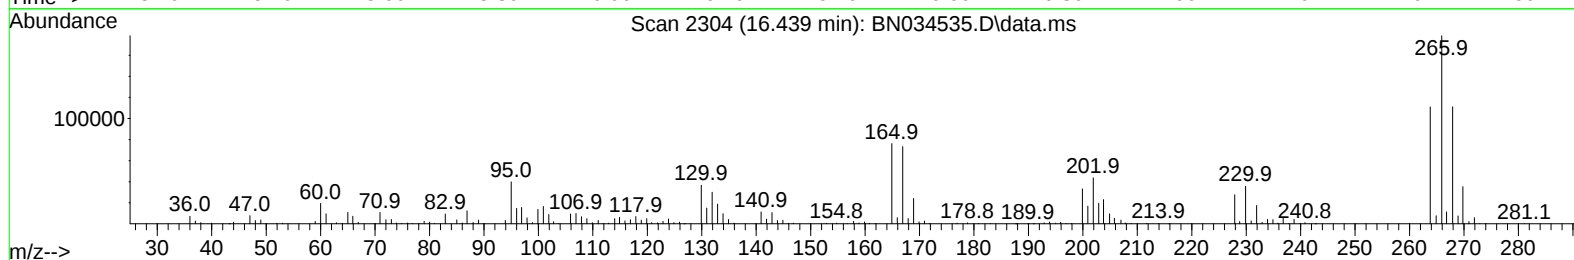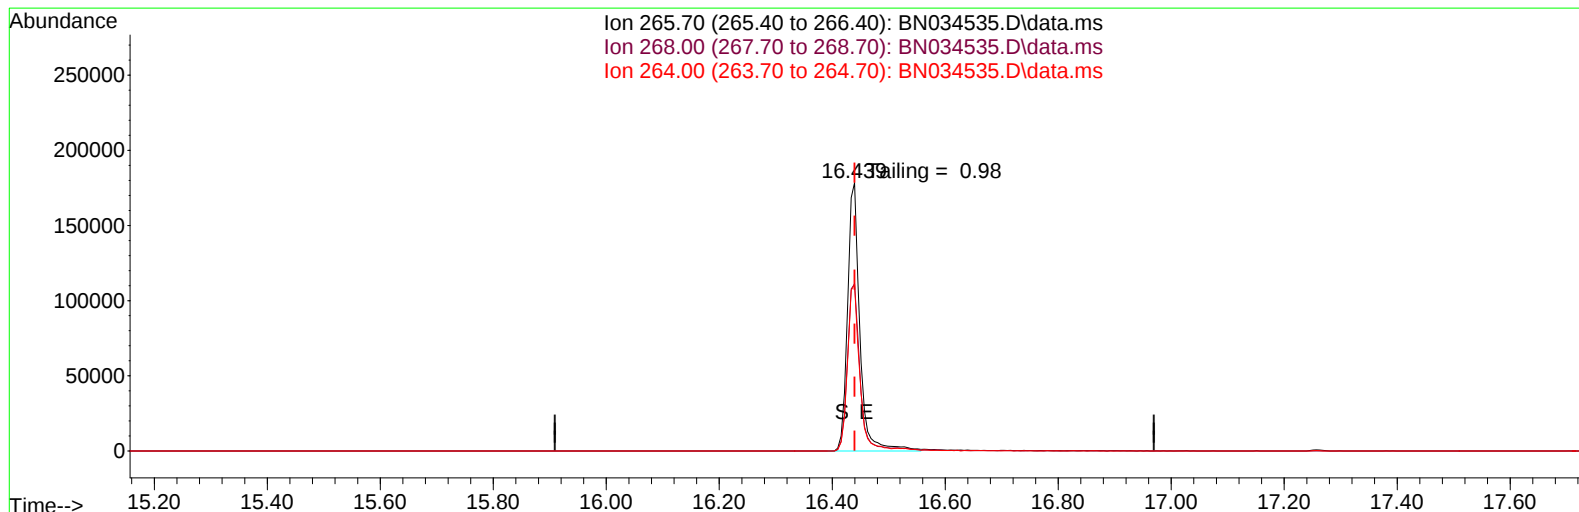

TIC: BN034535.D\data.ms

(70) Pentachlorophenol (C)

16.439min (0.000) 489005.44 ng

response 272469

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.28
264.00	61.60	62.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/10/2024	BNA_N	<u>BN034535.D</u>
Compound Name	Response	Retention Time
DDT	765254	20.31
DDD	21143	19.869
DDE	950	19.357
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22093	787347	2.81

Instrument :
BNA_N
ClientSampleId :
DFTPP